
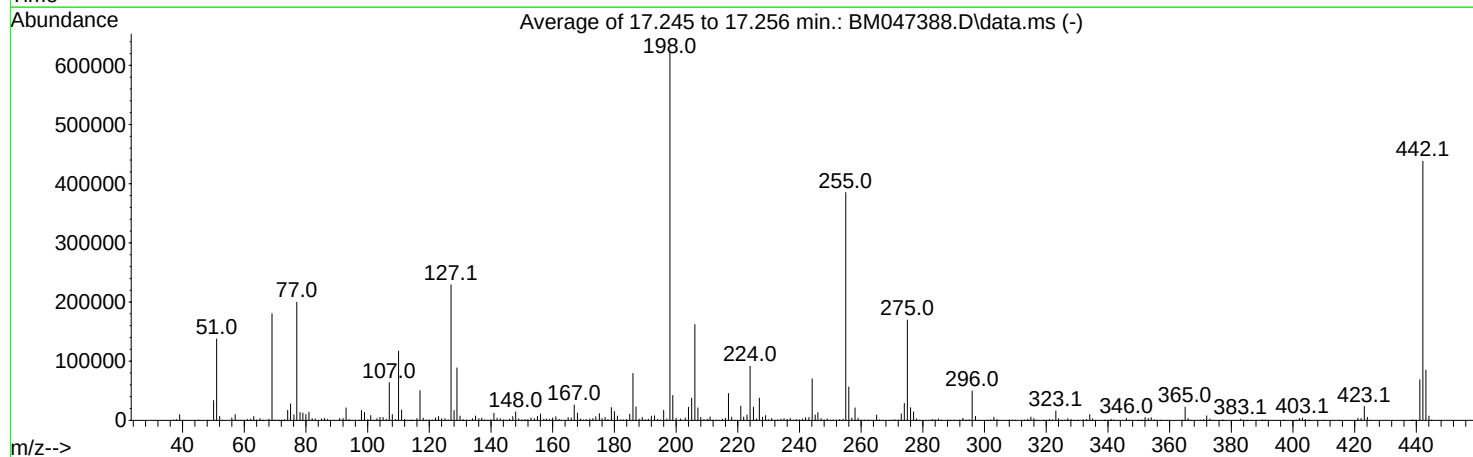


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082924\
Data File : BM047388.D
Acq On : 29 Aug 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

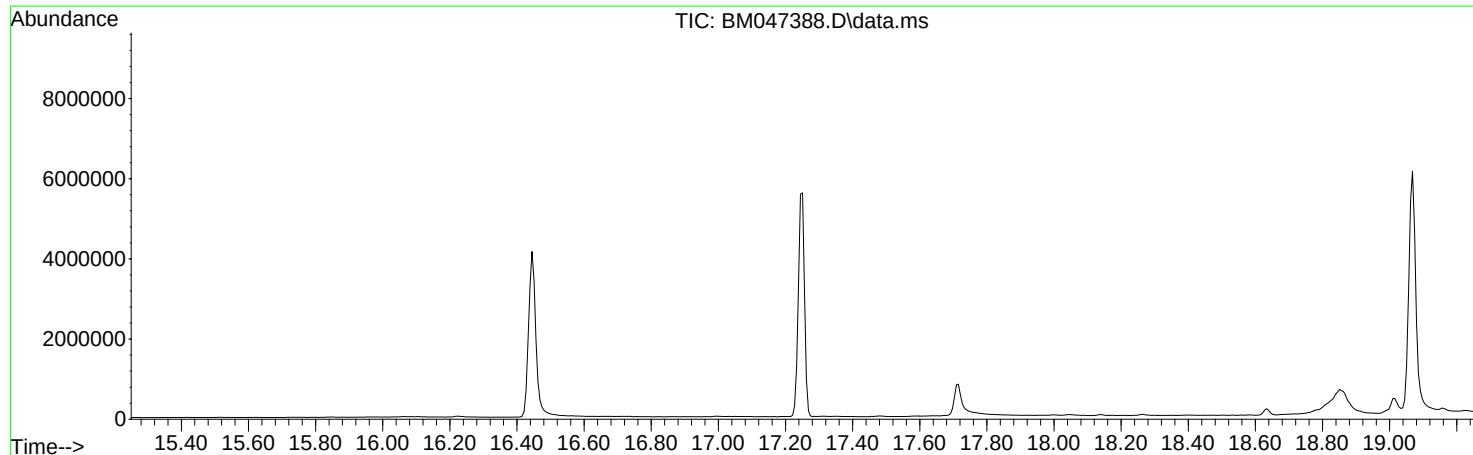

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	137748	PASS
68	69	0.00	2	1.2	2243	PASS
69	198	0.00	100	29.0	180364	PASS
70	69	0.00	2	0.4	771	PASS
127	198	10	80	36.8	229120	PASS
197	198	0.00	2	0.4	2552	PASS
198	198	100	100	100.0	621803	PASS
199	198	5	9	6.8	42255	PASS
275	198	10	60	27.3	169669	PASS
365	198	1	100	3.6	22363	PASS
441	198	0.01	100	11.1	68856	PASS
442	442	50	100	100.0	438208	PASS
443	442	15	24	19.4	84845	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2024	BNA_M	<u>BM047388.D</u>
Compound Name	Response	Retention Time
DDT	2333381	20.309
DDD	71937	19.868
DDE	3369	19.35
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
75306	2408687	3.13

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082924\
Data File : BM047388.D
Acq On : 29 Aug 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 29 11:16:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

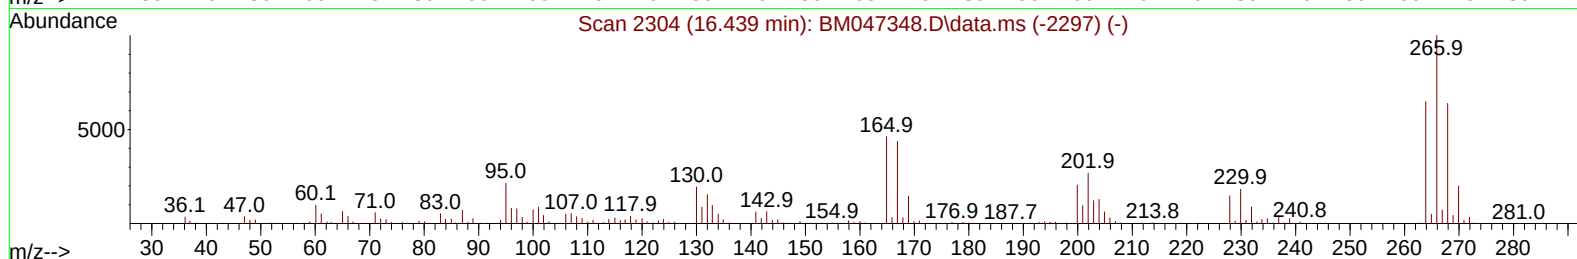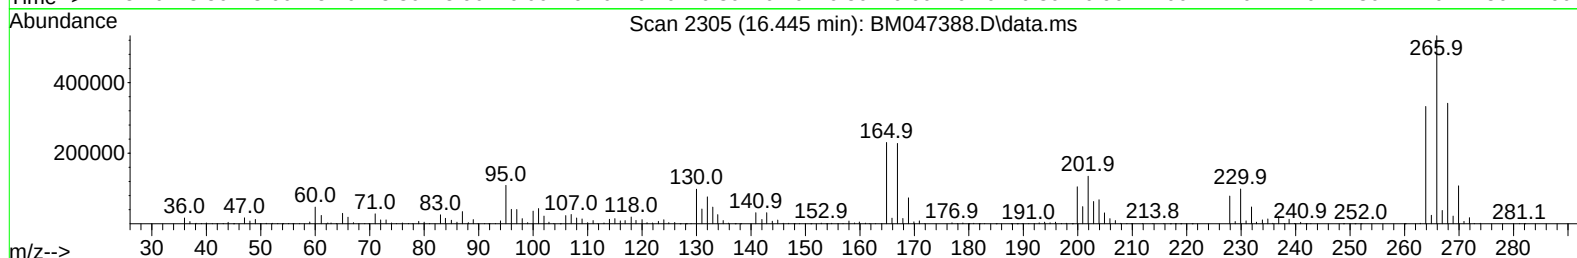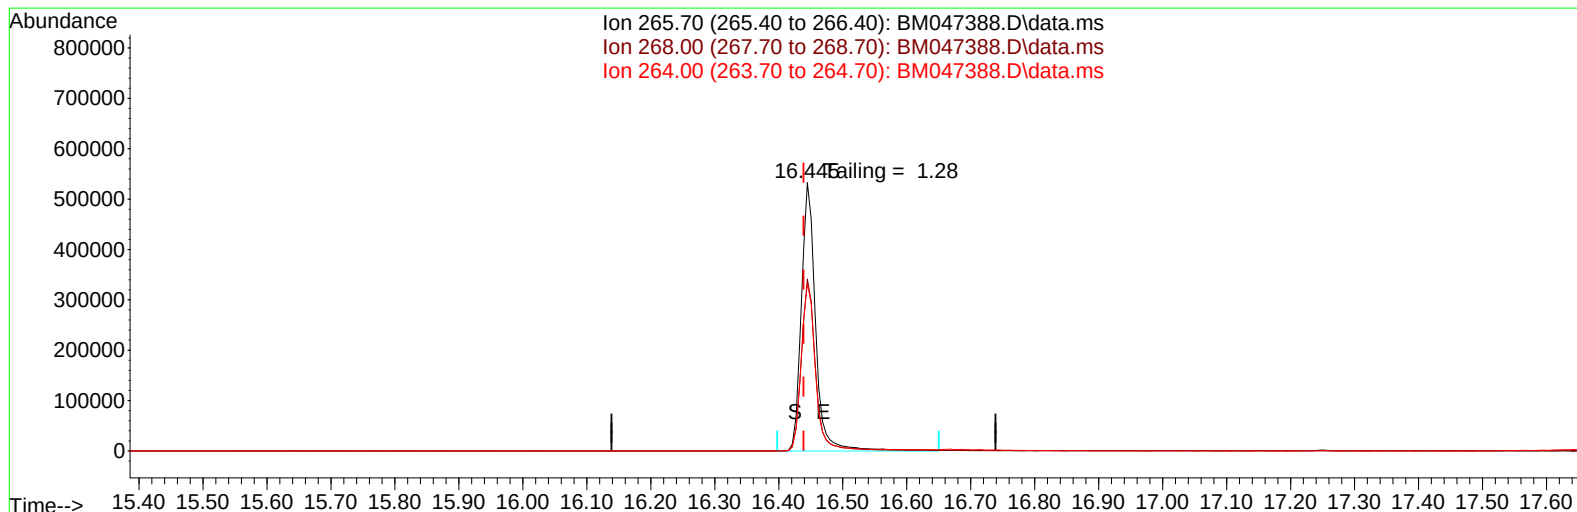

TIC: BM047388.D\data.ms

(70) Pentachlorophenol (C)

16.445min (+ 0.006) 106487.81 ng




response 829653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.08
264.00	64.90	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082924\
Data File : BM047388.D
Acq On : 29 Aug 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 29 11:16:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

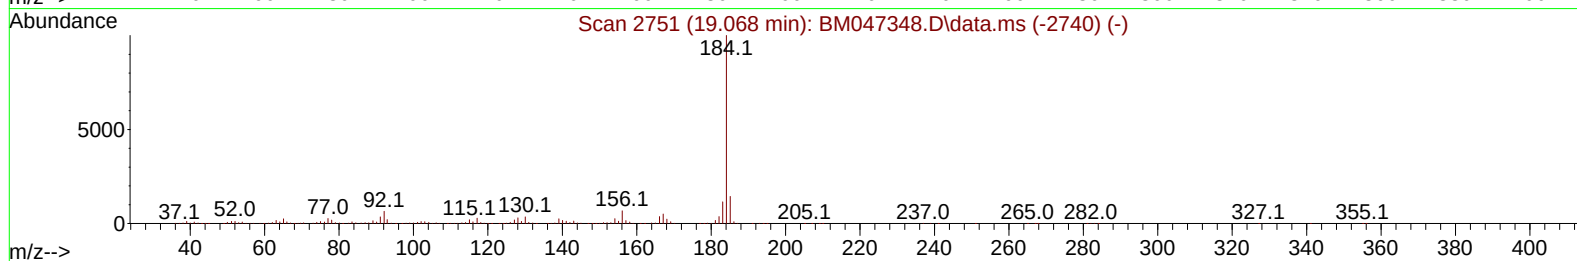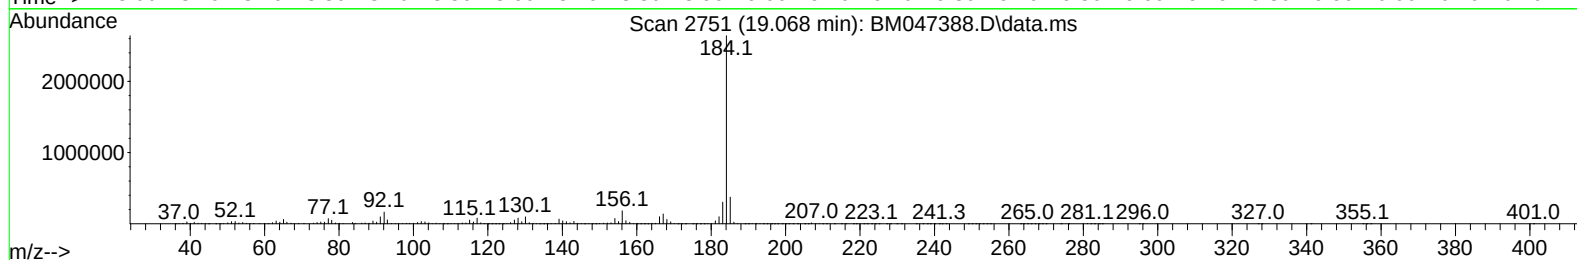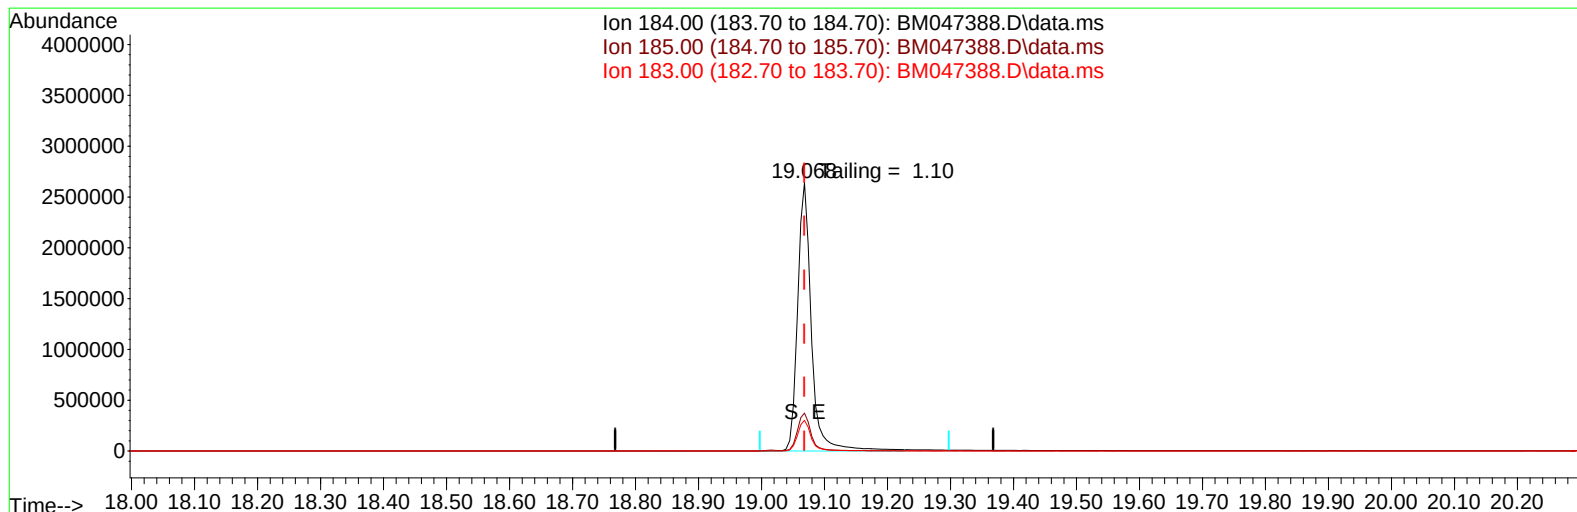

TIC: BM047388.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 105128.63 ng

response 4071227

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.50	11.49
0.00	0.00	0.00