


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031948.D
Acq On : 30 Aug 2021 13:32
Operator : CG/JU
Sample : M3365-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK83

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

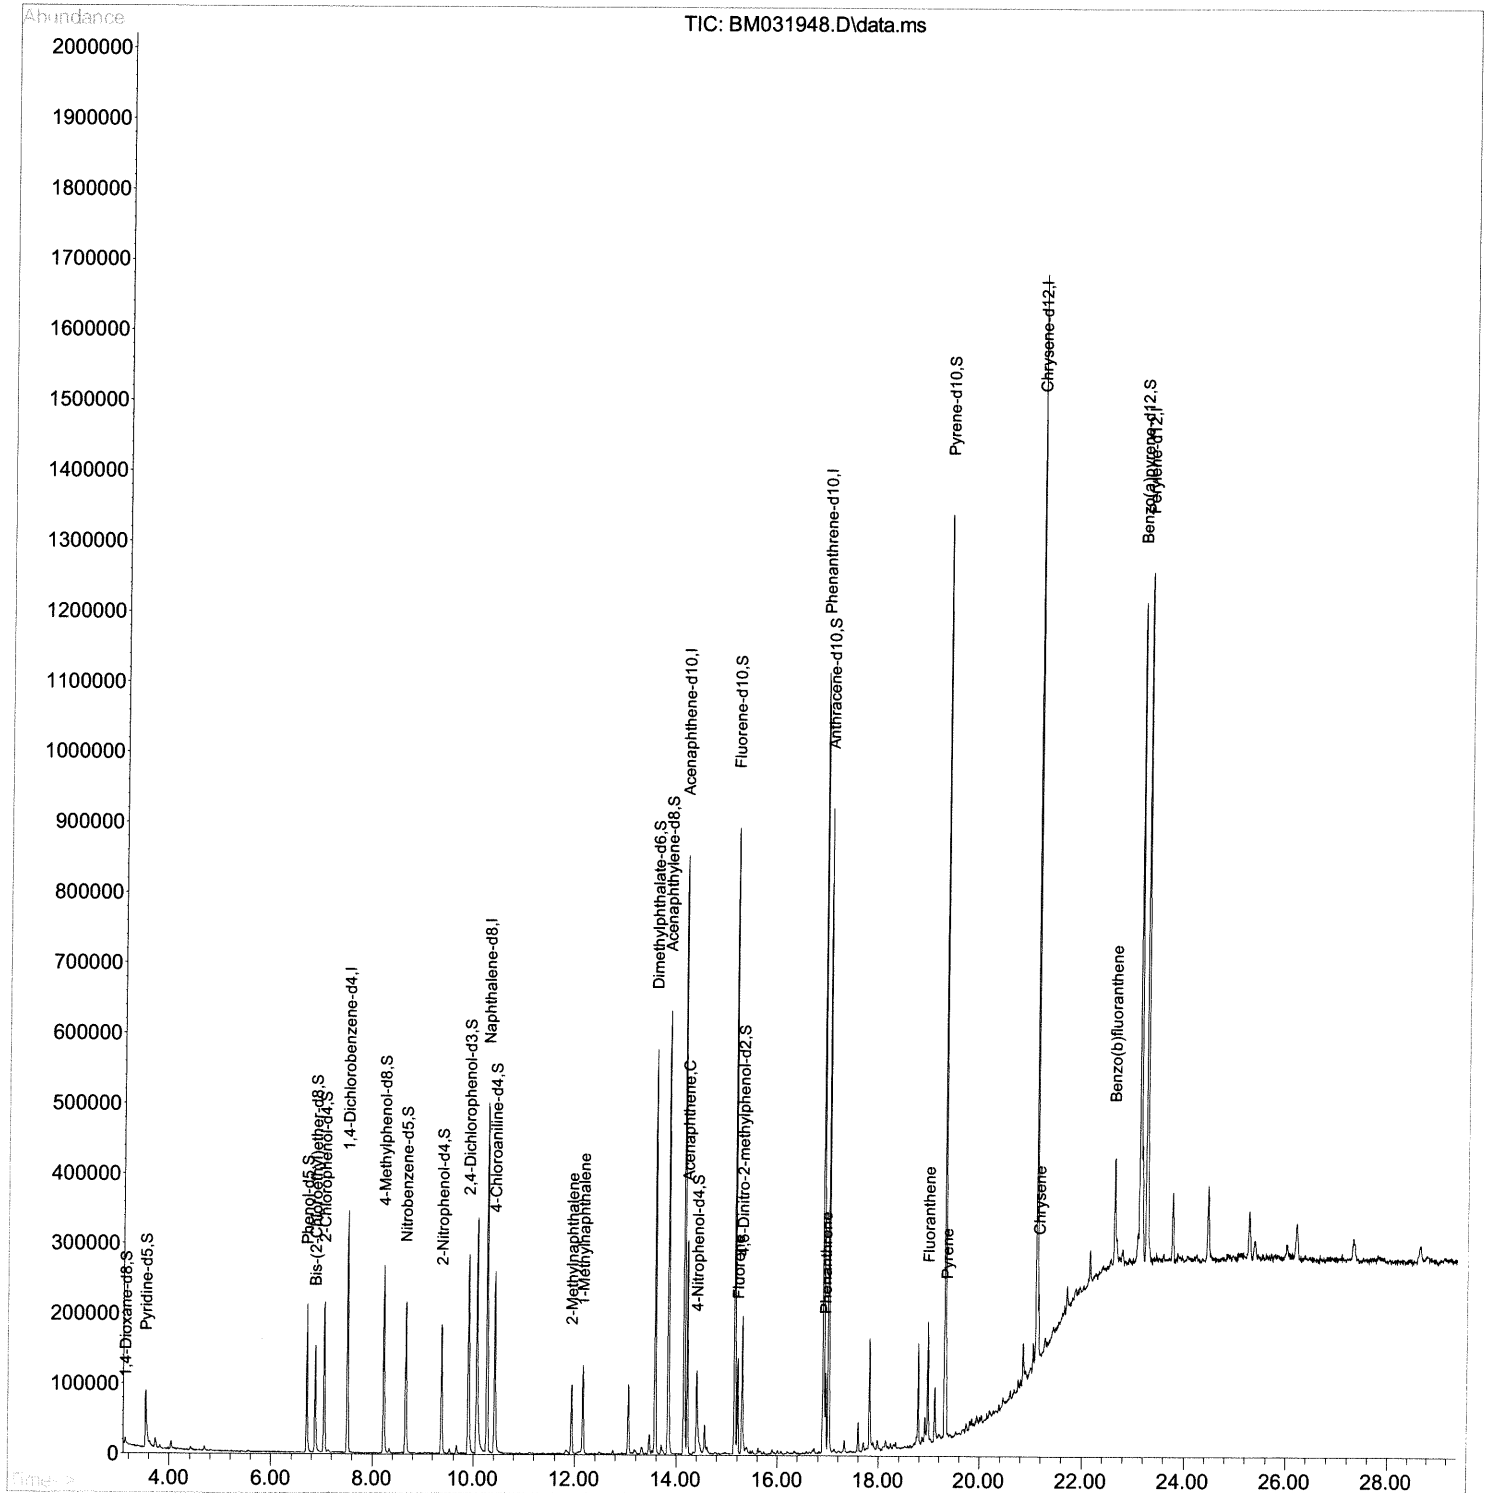

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031948.D
 Acq On : 30 Aug 2021 13:32
 Operator : CG/JU
 Sample : M3365-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK83

Manual Integrations
 APPROVED

mohammad
 8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

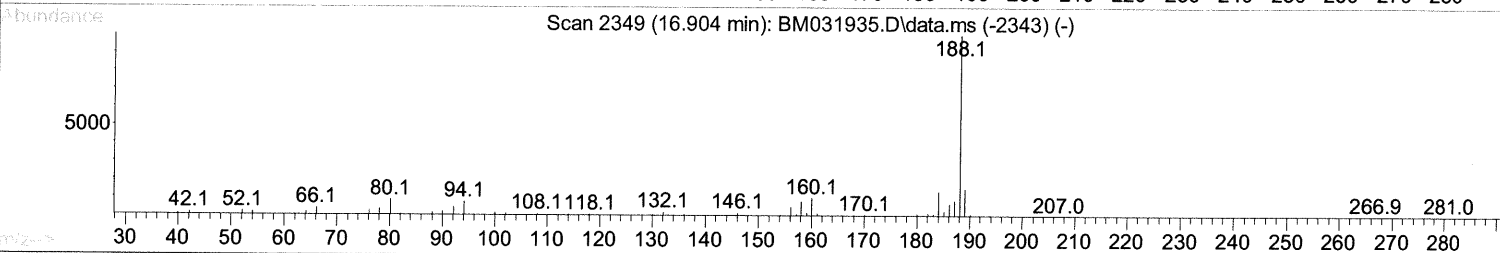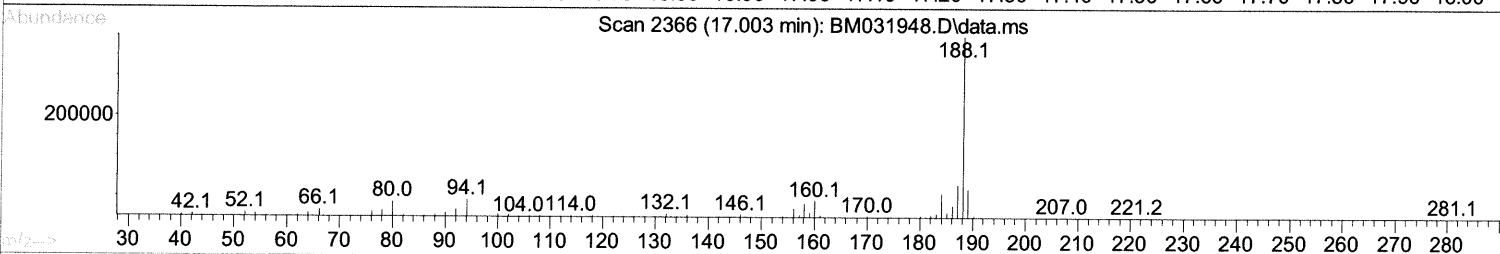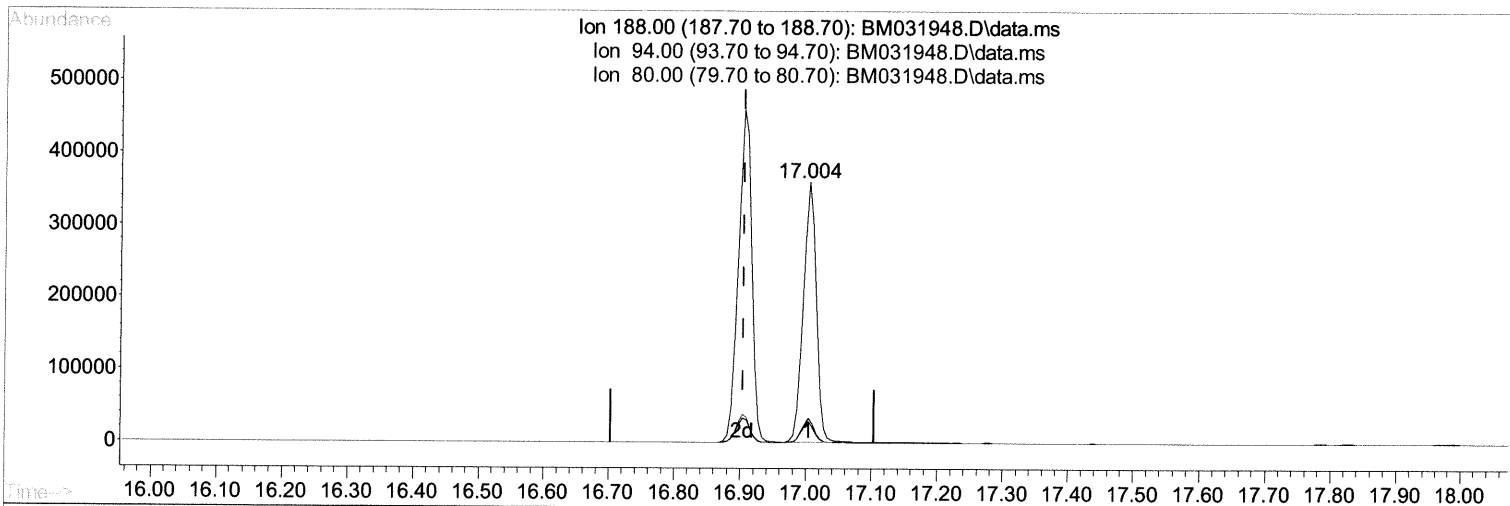

TIC: BM031948.D\data.ms

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031948.D
Acq On : 30 Aug 2021 13:32
Operator : CG/JU
Sample : M3365-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK83

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

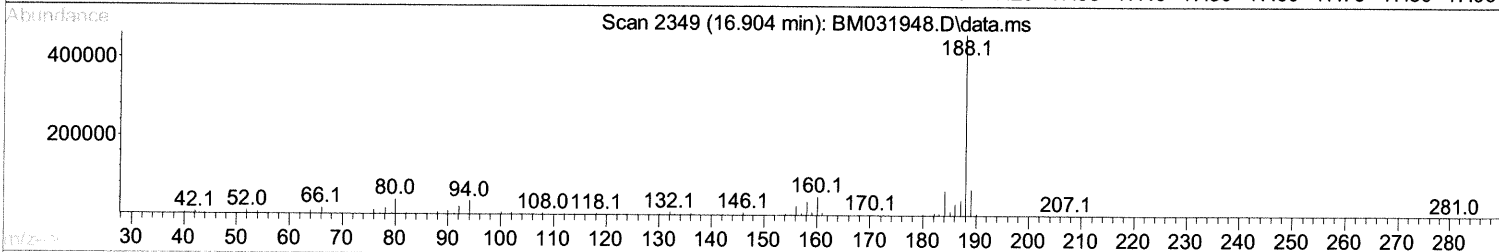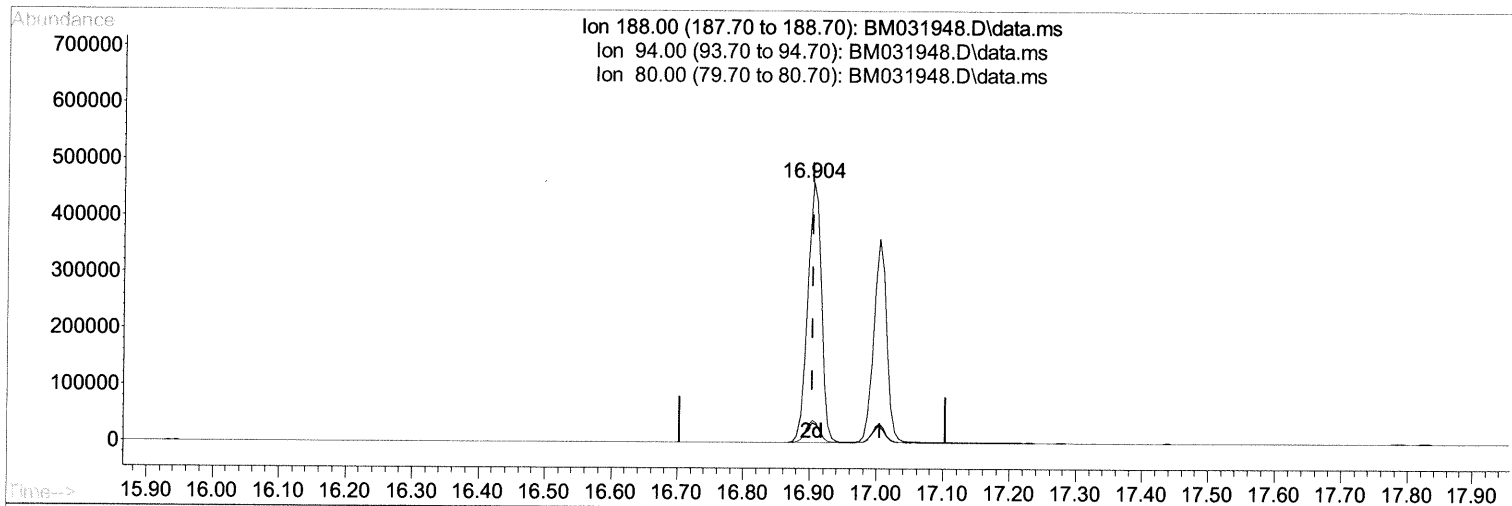

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031948.D
 Acq On : 30 Aug 2021 13:32
 Operator : CG/JU
 Sample : M3365-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK83

Manual Integrations
 APPROVED

mohammad
 8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

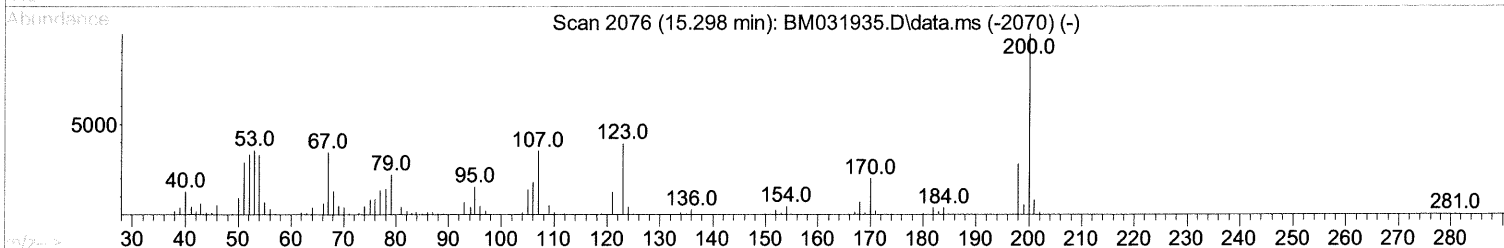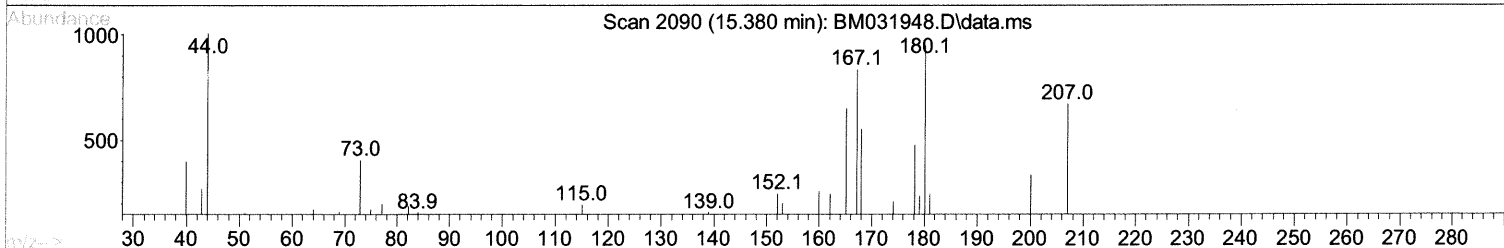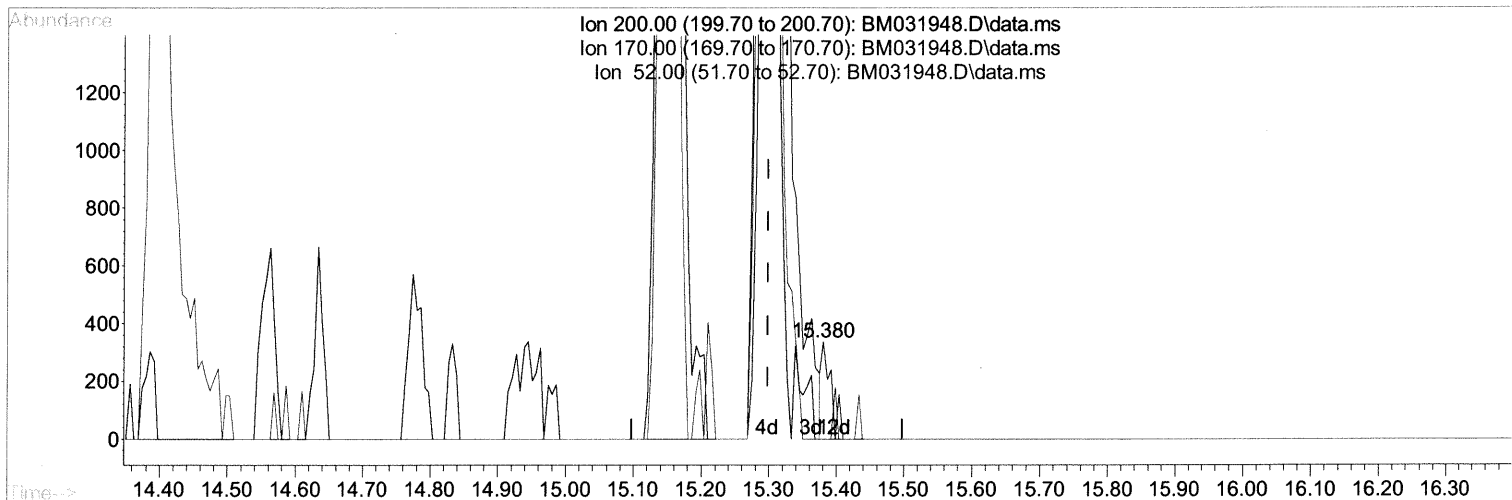

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031948.D
Acq On : 30 Aug 2021 13:32
Operator : CG/JU
Sample : M3365-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK83

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

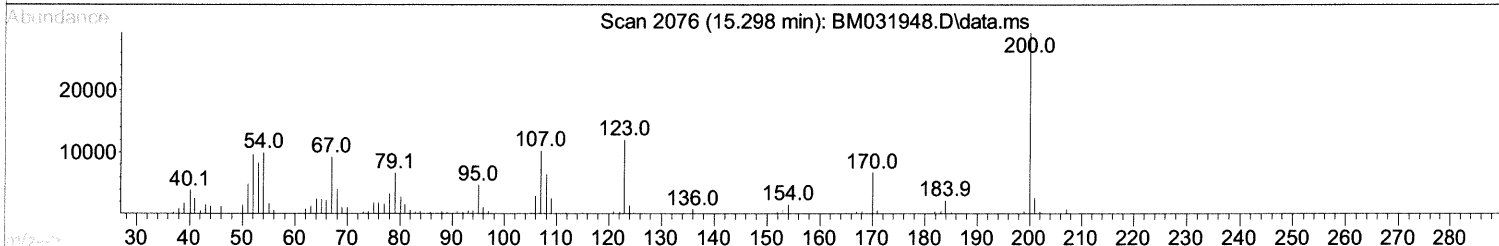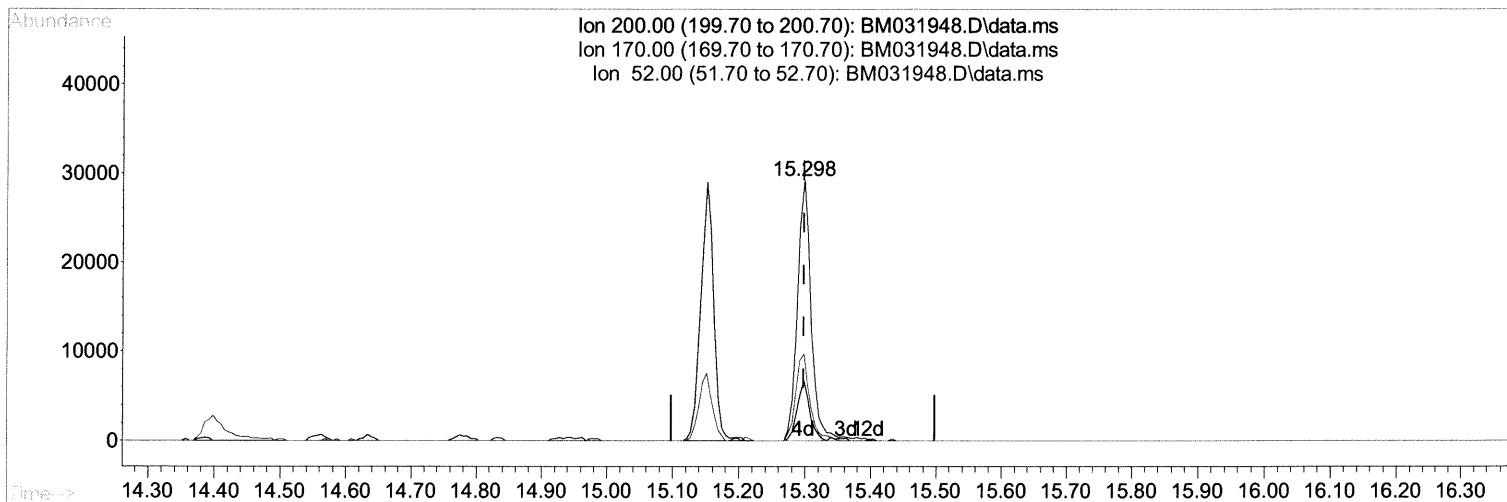

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031948.D
Acq On : 30 Aug 2021 13:32
Operator : CG/JU
Sample : M3365-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK83

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
Qlast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

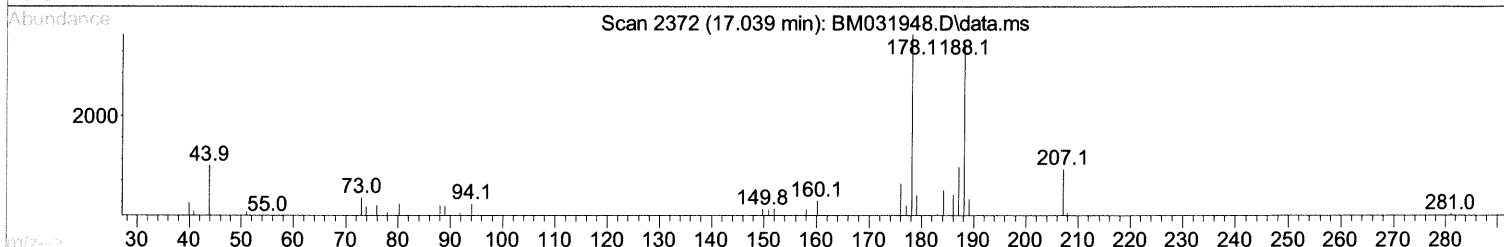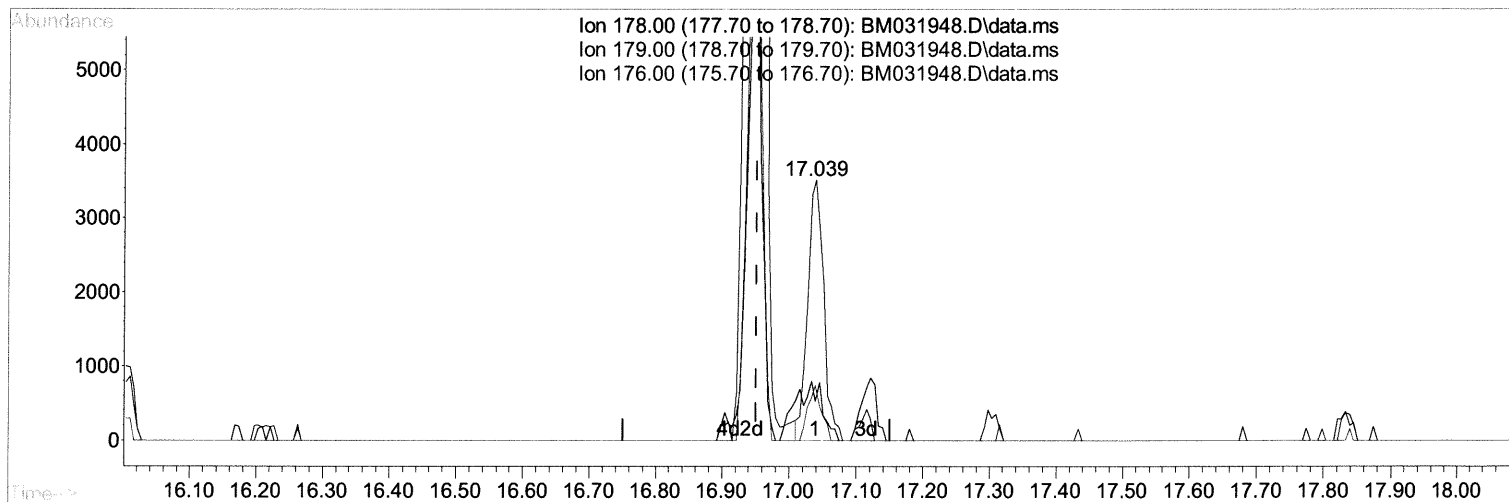

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031948.D
 Acq On : 30 Aug 2021 13:32
 Operator : CG/JU
 Sample : M3365-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK83

Manual Integrations
 APPROVED

mohammad
 8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

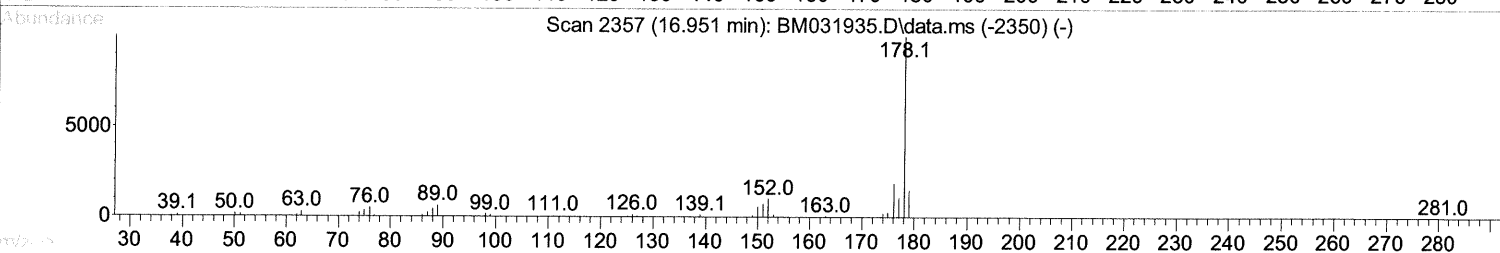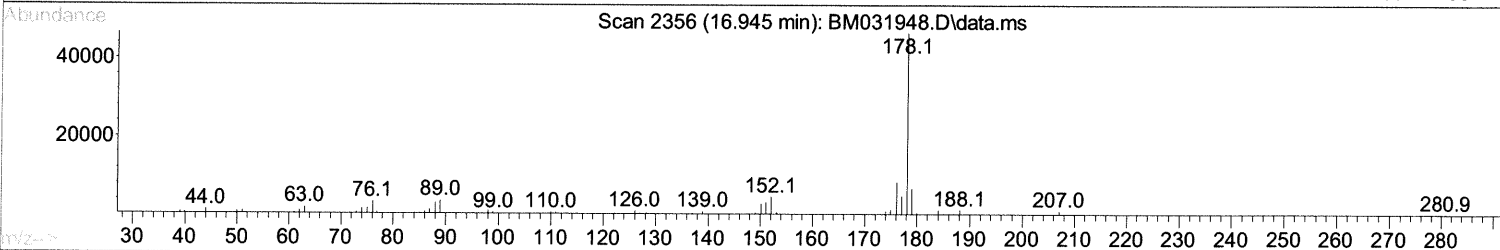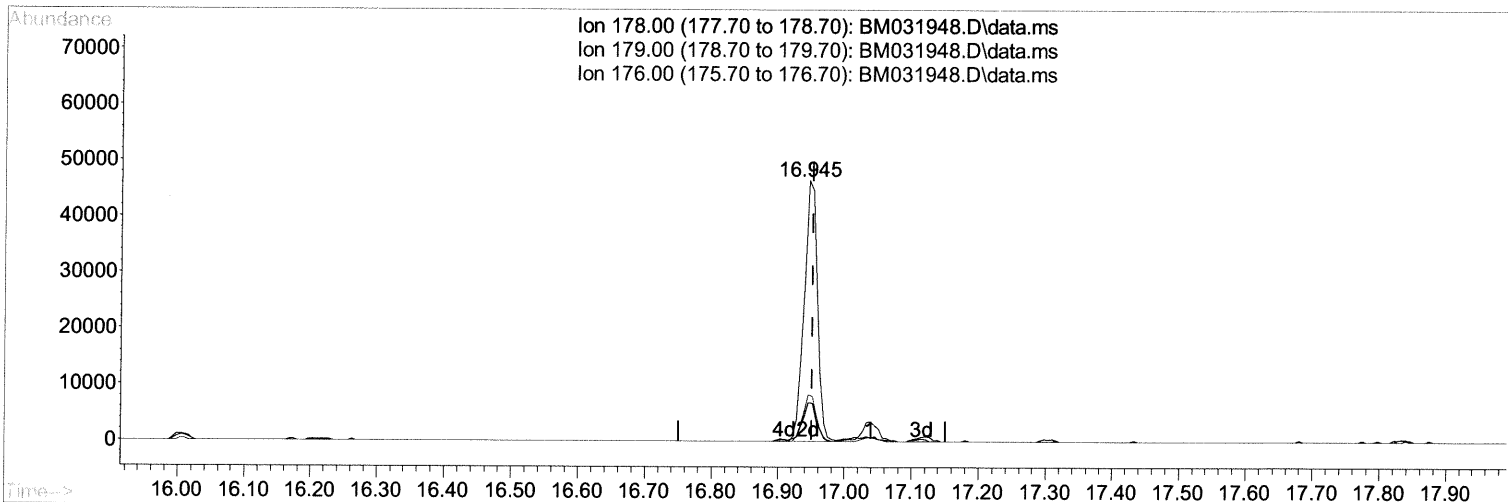

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031948.D
 Acq On : 30 Aug 2021 13:32
 Operator : CG/JU
 Sample : M3365-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK83

Manual Integrations
 APPROVED

mohammad
 8/31/2021 11:37:02 AM

Quant Time: Aug 30 14:09:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	92752	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	398842	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	292611	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	651258m	20.000	ng/ul	0.00
79) Chrysene-d12	21.115	240	684116	20.000	ng/ul	# 0.00
88) Perylene-d12	23.256	264	658066	20.000	ng/ul	0.00
System						