

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031953.D
 Acq On : 30 Aug 2021 16:37
 Operator : CG/JU
 Sample : M3365-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKB6

Quant Time: Aug 30 17:14:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	86937	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	383316	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	282834	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	625867	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.115	240	653342	20.000	ng/ul	# 0.00
88) Perylene-d12	23.251	264	648567	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6375	3.383	ng/uL	0.00
4) Pyridine-d5	3.534	84	45535	8.510	ng/ul	0.01
7) Phenol-d5	6.705	99	124348	17.248	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67	78396	18.795	ng/ul	0.00
11) 2-Chlorophenol-d4	7.052	132	108174	19.499	ng/ul	0.00
15) 4-Methylphenol-d8	8.222	113	107087	17.314	ng/ul	0.00
21) Nitrobenzene-d5	8.663	128	56220	20.193	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	60286	18.297	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.904	165	116044	17.554	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	156407	16.773	ng/ul	0.00
46) Dimethylphthalate-d6	13.575	166	459054	21.450	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	530888	20.946	ng/ul	0.00
54) 4-Nitrophenol-d4	14.392	143	50603	13.063	ng/ul	0.00
60) Fluorene-d10	15.151	176	395605	21.028	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	53504	12.441	ng/ul	0.00
73) Anthracene-d10	17.004	188	674599	22.709	ng/ul	0.00
81) Pyrene-d10	19.310	212	822618	26.881	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.121	264	808103	23.708	ng/ul	0.00
Target Compounds						
18) 4-Methylphenol	8.275	108	34776	5.599	ng/ul	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031953.D
Acq On : 30 Aug 2021 16:37
Operator : CG/JU
Sample : M3365-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKB6

Quant Time: Aug 30 17:14:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

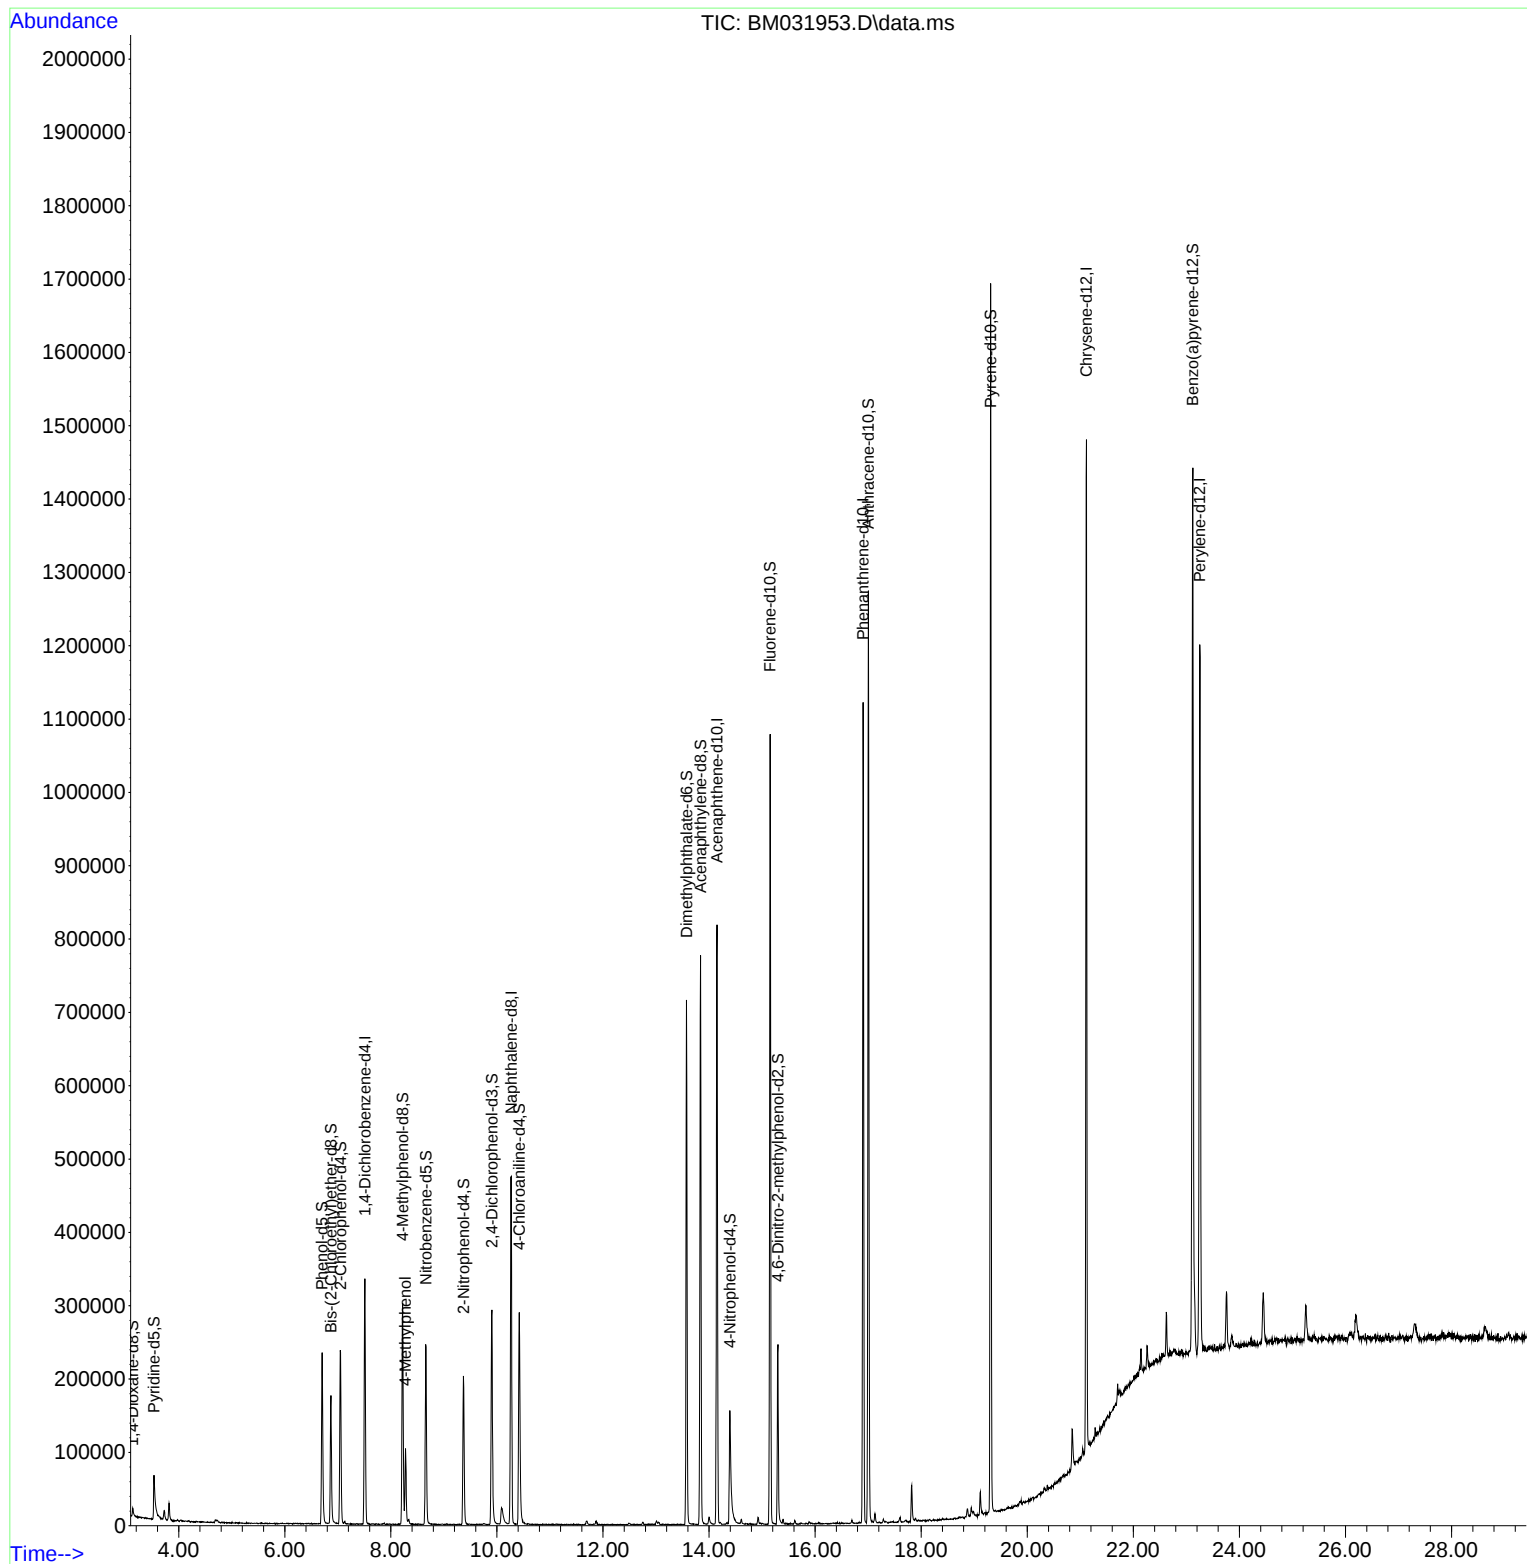

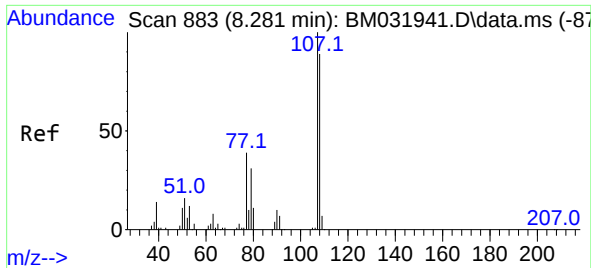

#18
4-Methylphenol
Concen: 5.599 ng/ul
RT: 8.275 min Scan# 882
Delta R.T. -0.011 min
Lab File: BM031953.D
Acq: 30 Aug 2021 16:37

Instrument :
BNA_M
ClientSampleId :
DBKB6

Tgt Ion:108 Resp: 34776
Ion Ratio Lower Upper
108 100
107 119.8 87.0 130.6

