

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031954.D
 Acq On : 30 Aug 2021 17:15
 Operator : CG/JU
 Sample : M3365-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKB5

Quant Time: Aug 30 18:06:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	89045	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	379962	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.151	164	282094	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	625950	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.115	240	666985	20.000	ng/ul	# 0.00
88) Perylene-d12	23.256	264	657688	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	13635	7.065	ng/uL	0.00
4) Pyridine-d5	3.522	84	187468	34.207	ng/ul	0.00
7) Phenol-d5	6.704	99	270572	36.643	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67	164462	38.495	ng/ul	0.00
11) 2-Chlorophenol-d4	7.051	132	228511	40.216	ng/ul	0.00
15) 4-Methylphenol-d8	8.222	113	240818	38.013	ng/ul	0.00
21) Nitrobenzene-d5	8.663	128	119725	43.382	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	140517	43.023	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.898	165	262512	40.060	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	346246	37.458	ng/ul	0.00
46) Dimethylphthalate-d6	13.580	166	895447	41.950	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	1099186	43.482	ng/ul	0.00
54) 4-Nitrophenol-d4	14.386	143	129466	33.509	ng/ul	0.00
60) Fluorene-d10	15.151	176	790015	42.103	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	125983	29.291	ng/ul	0.00
73) Anthracene-d10	17.004	188	1252496	42.156	ng/ul	0.00
81) Pyrene-d10	19.309	212	1467128	46.962	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.121	264	1453850	42.061	ng/ul	0.00
Target Compounds						
18) 4-Methylphenol	8.275	108	17015	2.675	ng/ul	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031954.D
Acq On : 30 Aug 2021 17:15
Operator : CG/JU
Sample : M3365-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKB5


Quant Time: Aug 30 18:06:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

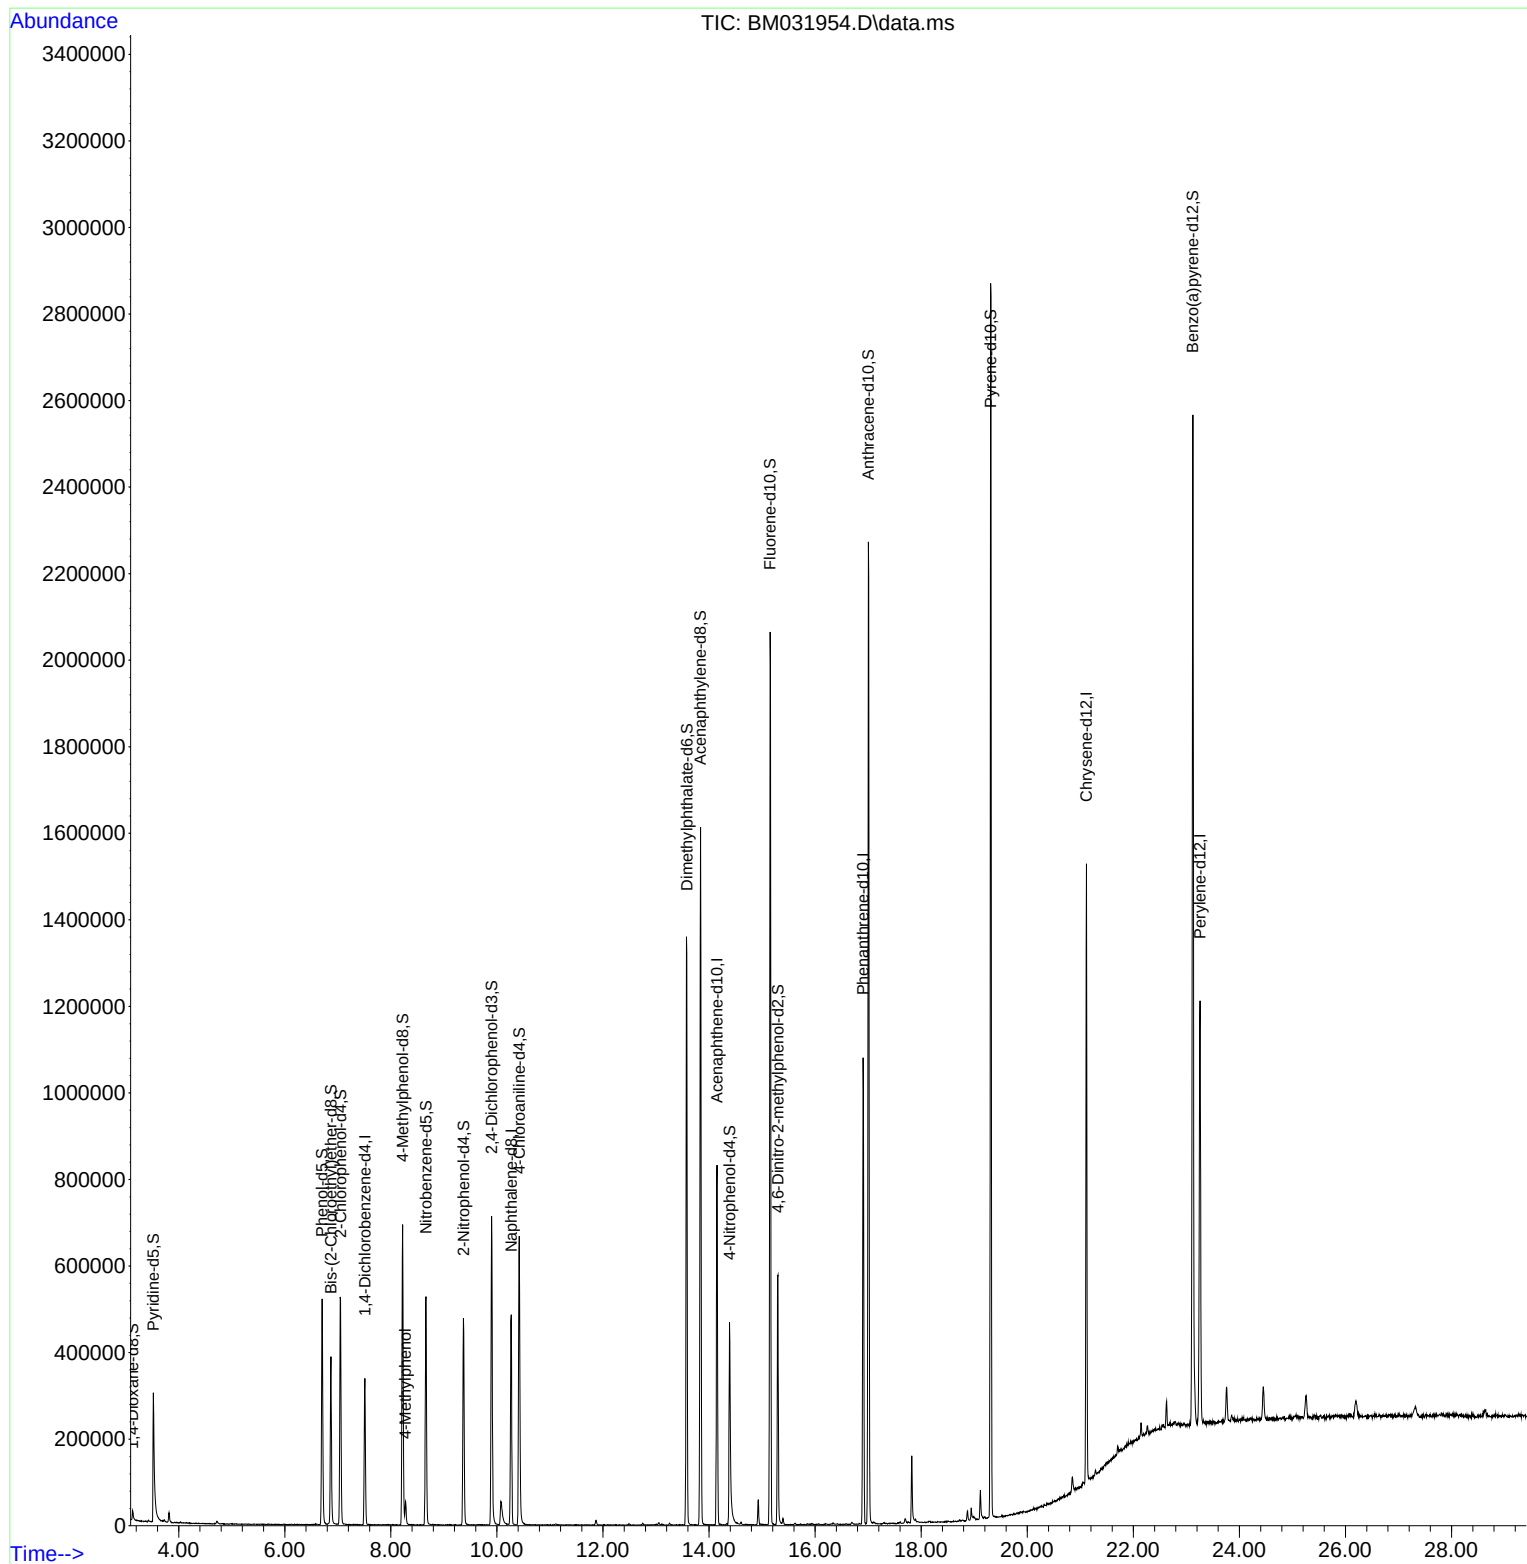

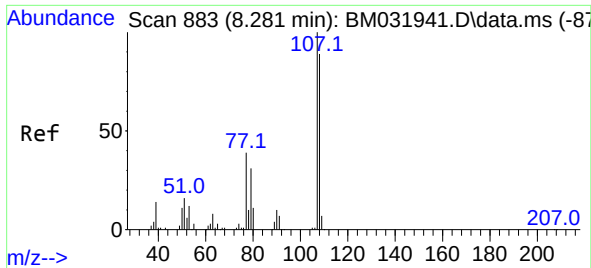

#18
4-Methylphenol
Concen: 2.675 ng/ul
RT: 8.275 min Scan# 882
Delta R.T. -0.012 min
Lab File: BM031954.D
Acq: 30 Aug 2021 17:15

Instrument :
BNA_M
ClientSampleId :
DBKB5

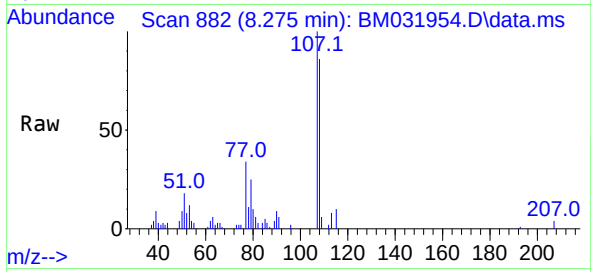

Tgt Ion:108 Resp: 17015
Ion Ratio Lower Upper
108 100
107 116.3 87.0 130.6

