

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031955.D
 Acq On : 30 Aug 2021 17:52
 Operator : CG/JU
 Sample : M3365-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKB4

Manual Integrations
 APPROVED

mohammad
 8/31/2021 11:37:16 AM

Quant Time: Aug 30 18:34:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	91809	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	393228	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.151	164	292073	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	640180m	20.000	ng/ul	0.00
79) Chrysene-d12	21.115	240	671380	20.000	ng/ul	# 0.00
88) Perylene-d12	23.256	264	652709	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	13833	6.952	ng/uL	0.00
4) Pyridine-d5	3.522	84	195087	34.526	ng/ul	0.00
7) Phenol-d5	6.704	99	271663	35.683	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67	159421	36.192	ng/ul	0.00
11) 2-Chlorophenol-d4	7.046	132	223471	38.145	ng/ul	0.00
15) 4-Methylphenol-d8	8.222	113	242441	37.117	ng/ul	0.00
21) Nitrobenzene-d5	8.663	128	114385	40.049	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	135677	40.140	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.898	165	261969	38.629	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	348822	36.464	ng/ul	0.00
46) Dimethylphthalate-d6	13.575	166	914147	41.363	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	1096357	41.888	ng/ul	0.00
54) 4-Nitrophenol-d4	14.386	143	130730	32.680	ng/ul	0.00
60) Fluorene-d10	15.151	176	793644	40.852	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.292	200	137229m	31.197	ng/ul	0.00
73) Anthracene-d10	17.004	188	1271775	41.854	ng/ul	0.00
81) Pyrene-d10	19.310	212	1504969	47.858	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.121	264	1431819	41.739	ng/ul	0.00
Target Compounds						
18) 4-Methylphenol	8.275	108	12381	1.888	ng/ul	Qvalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031955.D
Acq On : 30 Aug 2021 17:52
Operator : CG/JU
Sample : M3365-10
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBKB4

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:16 AM

Quant Time: Aug 30 18:34:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

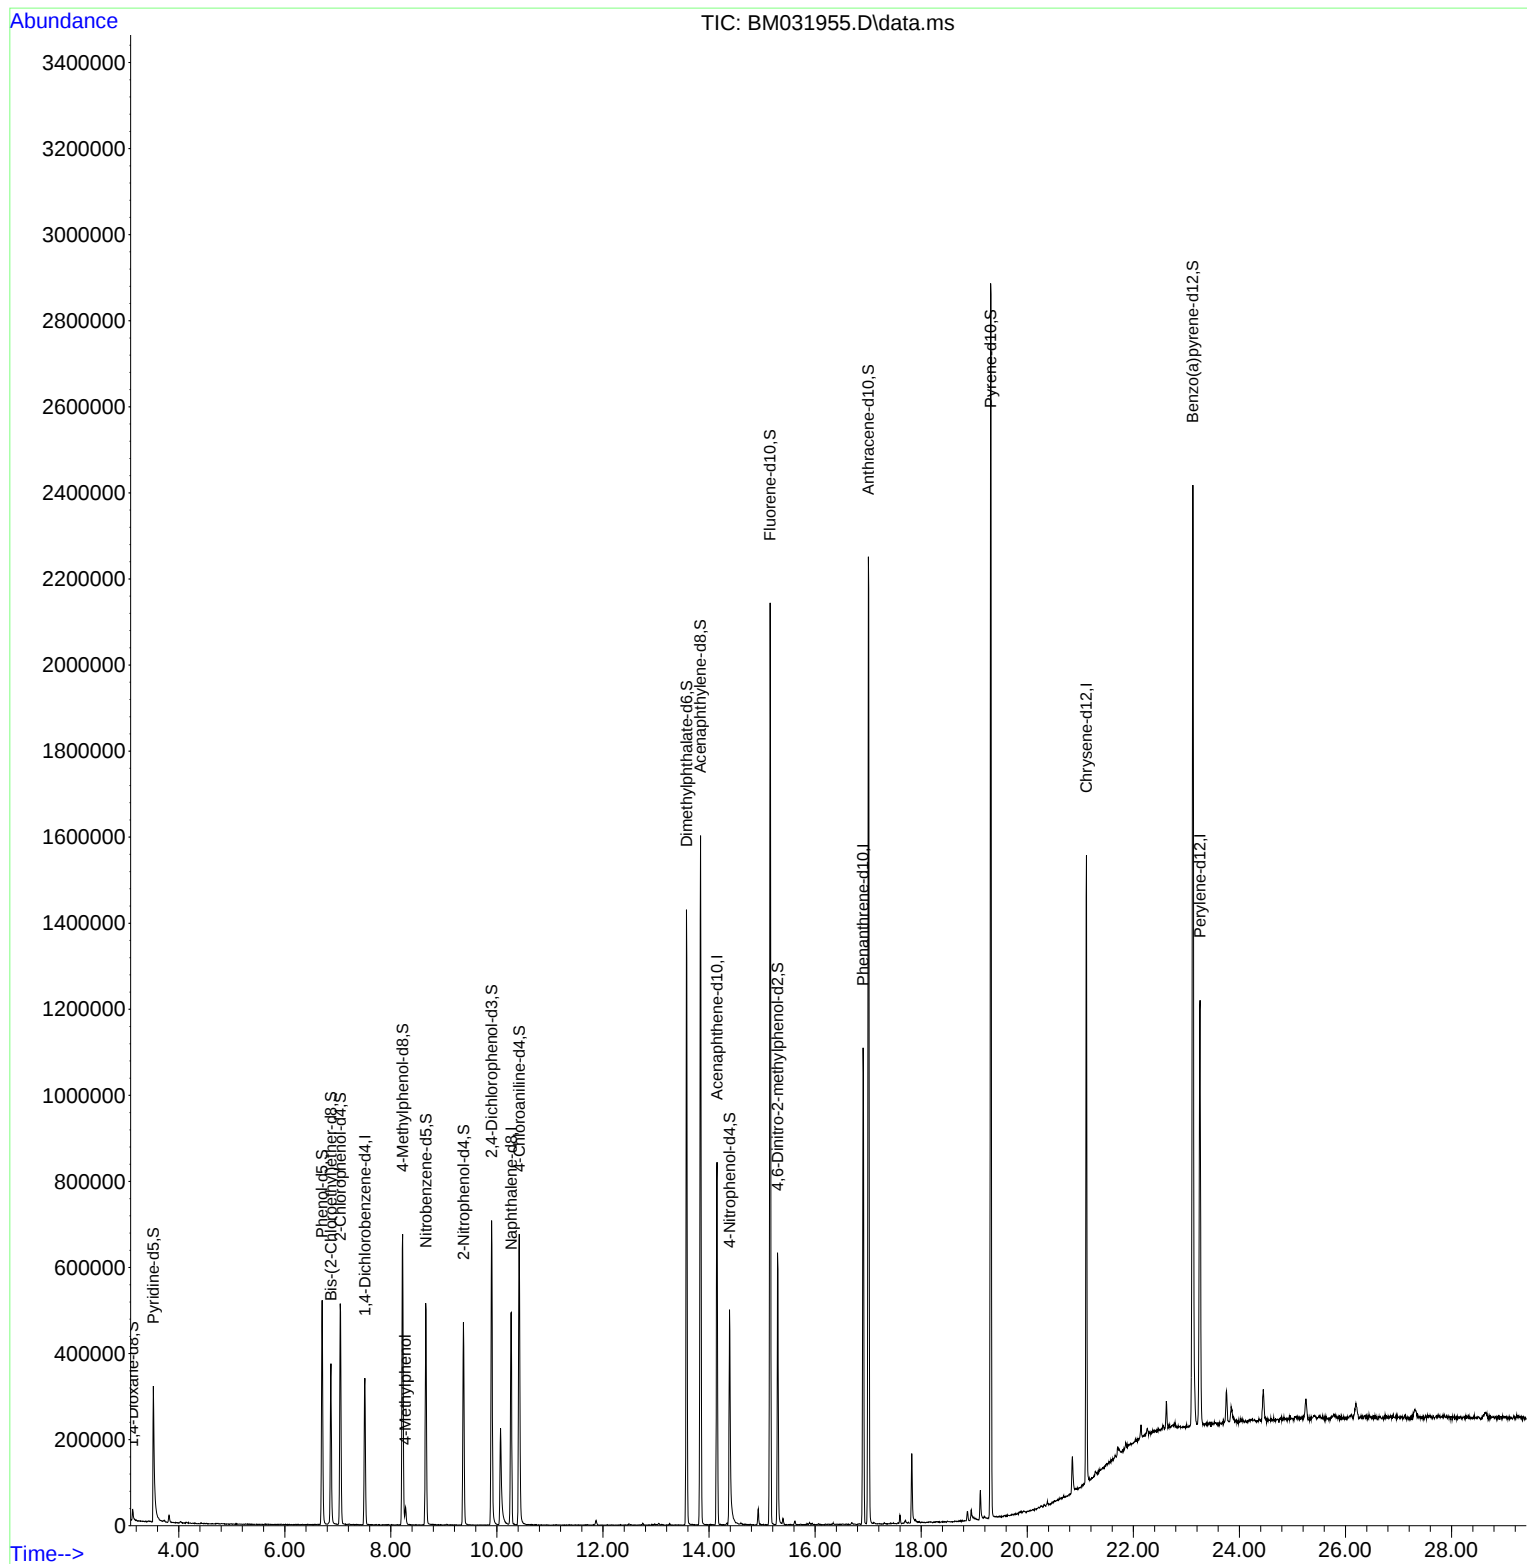

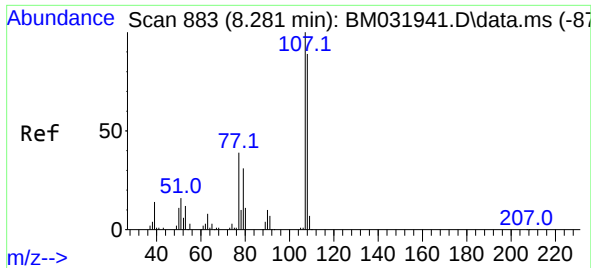

#18
4-Methylphenol
Concen: 1.888 ng/ul
RT: 8.275 min Scan# 882
Delta R.T. -0.012 min
Lab File: BM031955.D
Acq: 30 Aug 2021 17:52

Tgt Ion:108 Resp: 12381
Ion Ratio Lower Upper
108 100
107 122.3 87.0 130.6

Instrument :
BNA_M
ClientSampleId :
DBKB4

Manual Integrations
APPROVED

mohammad
8/31/2021 11:37:16 AM

