

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031979.D
 Acq On : 31 Aug 2021 10:41
 Operator : CG/JU
 Sample : M3474-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC4

Quant Time: Aug 31 11:42:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.505	152	80113	20.000	ng/ul	0.00
20) Naphthalene-d8	10.263	136	338944	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.145	164	244694	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	527336	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.110	240	557058	20.000	ng/ul	# 0.00
88) Perylene-d12	23.251	264	498736	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	7737	4.456	ng/uL	0.00
4) Pyridine-d5	3.540	84	18376	3.727	ng/ul	0.02
7) Phenol-d5	6.705	99	47498	7.150	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.863	67	117778	30.642	ng/ul	0.00
11) 2-Chlorophenol-d4	7.046	132	137036	26.806	ng/ul	0.00
15) 4-Methylphenol-d8	8.216	113	96564	16.942	ng/ul	0.00
21) Nitrobenzene-d5	8.657	128	86498	35.136	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	98922	33.953	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.899	165	195118	33.379	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	85469	10.365	ng/ul	0.00
46) Dimethylphthalate-d6	13.575	166	707966	38.237	ng/ul	0.00
49) Acenaphthylene-d8	13.834	160	817084	37.263	ng/ul	0.00
54) 4-Nitrophenol-d4	14.398	143	19416	5.793	ng/ul	0.01
60) Fluorene-d10	15.151	176	636060	39.080	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.292	200	100026	27.605	ng/ul	0.00
73) Anthracene-d10	17.004	188	1071481	42.808	ng/ul	0.00
81) Pyrene-d10	19.310	212	1286015	49.288	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.115	264	1134936	43.299	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.622	163	127441	7.010	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031979.D
Acq On : 31 Aug 2021 10:41
Operator : CG/JU
Sample : M3474-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC4

Quant Time: Aug 31 11:42:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

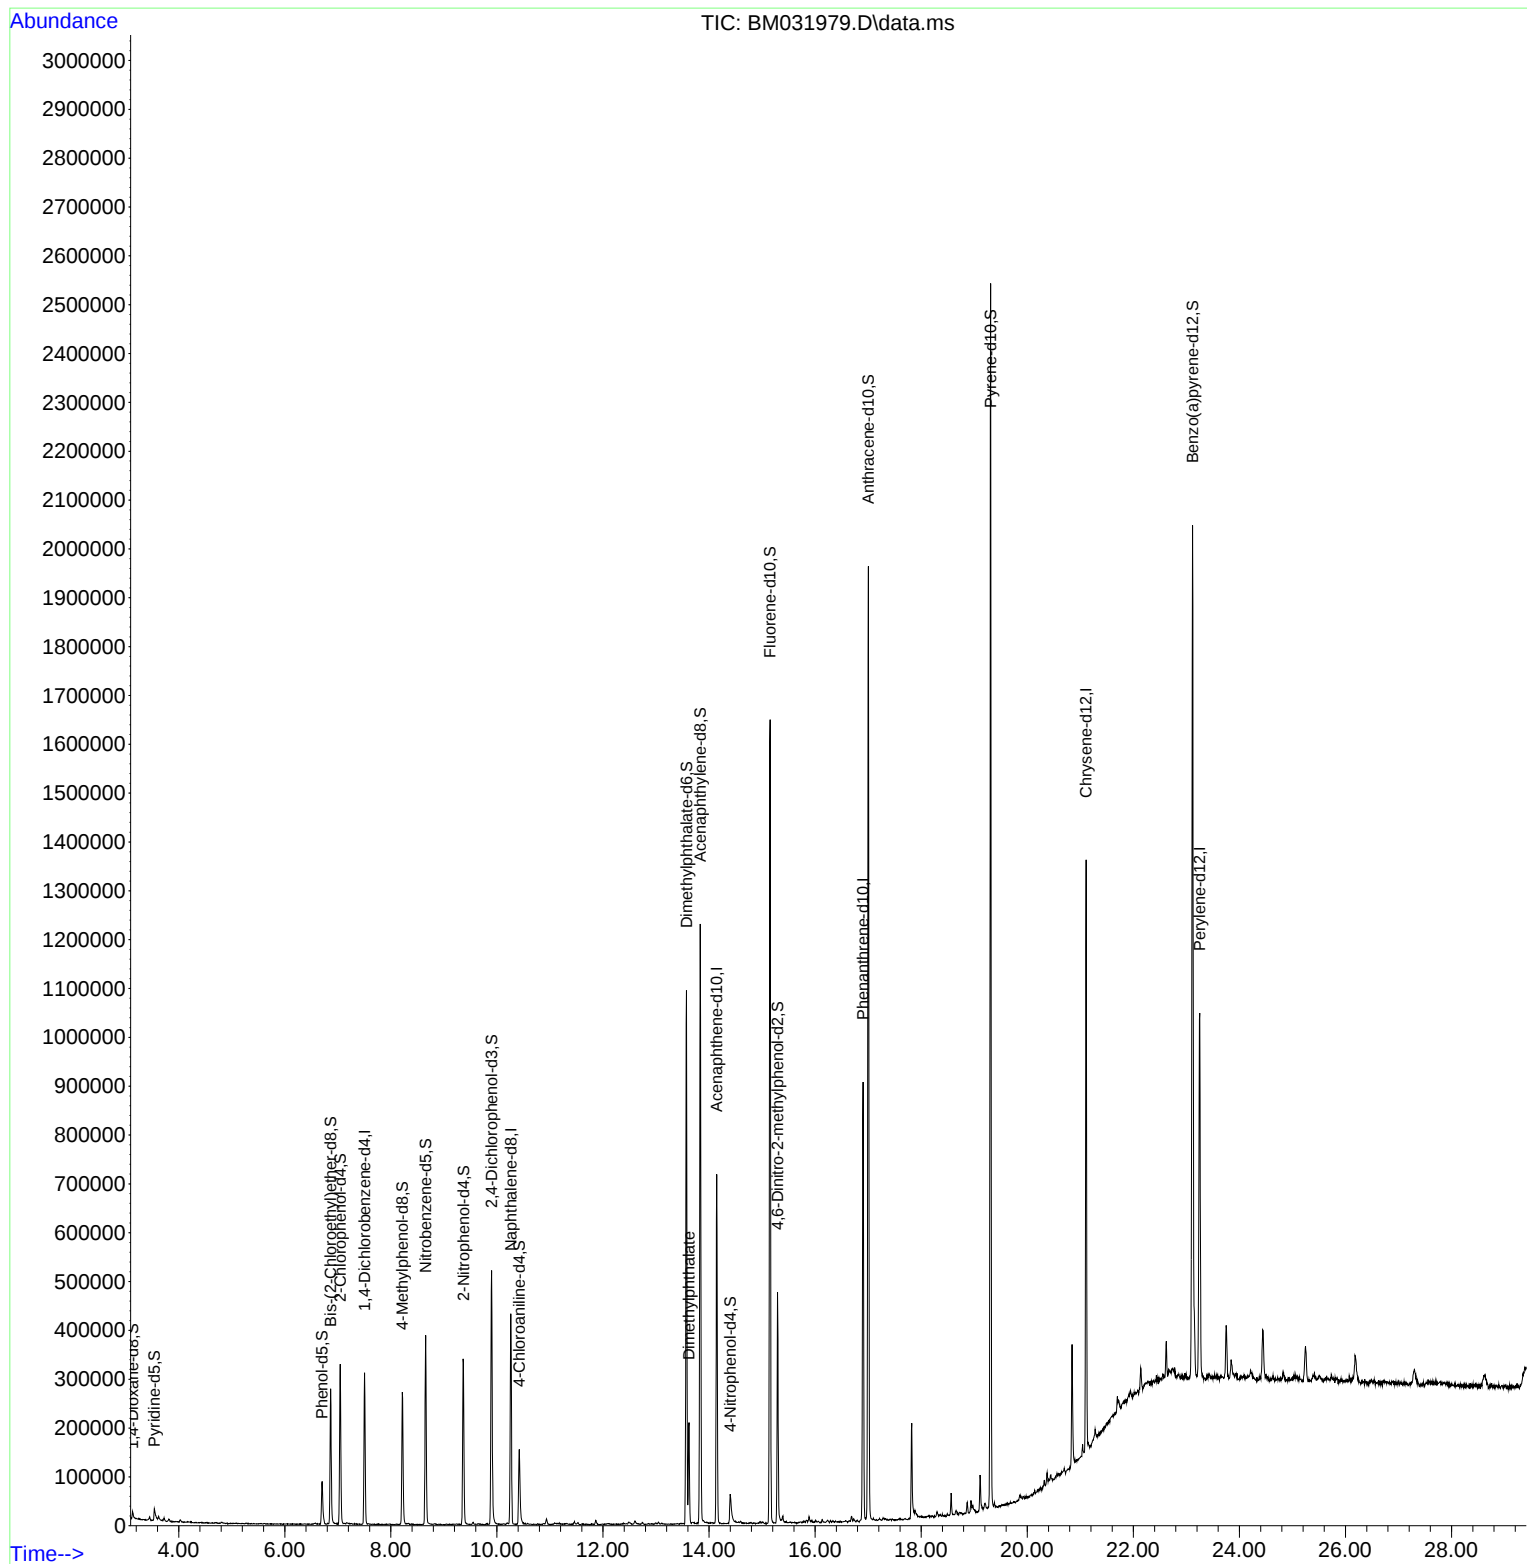

Abundance Scan 1791 (13.621 min): BM031974.D\data.ms (


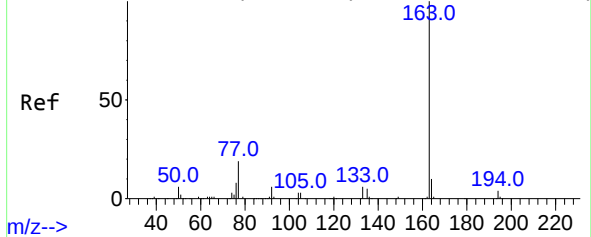


#47
Dimethylphthalate
Concen: 7.010 ng/ul
RT: 13.622 min Scan# 1791
Delta R.T. -0.006 min
Lab File: BM031979.D
Acq: 31 Aug 2021 10:41

Instrument :
BNA_M
ClientSampleId :
C0AC4

Tgt Ion:163 Resp: 127441
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 10.0 8.2 12.4

Abundance Scan 1791 (13.622 min): BM031979.D\data.ms

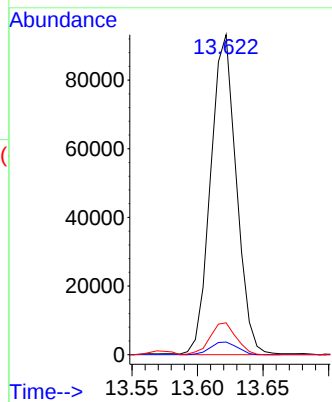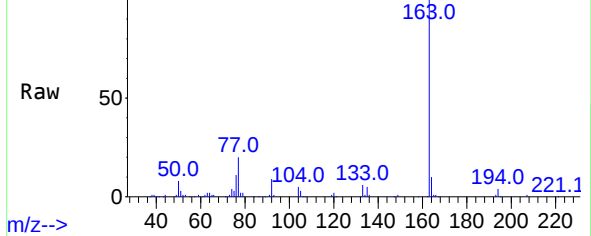

Abundance Scan 1791 (13.622 min): BM031979.D\data.ms (

