

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031980.D
 Acq On : 31 Aug 2021 11:18
 Operator : CG/JU
 Sample : M3474-11
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Quant Time: Aug 31 11:48:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.504	152	88249	20.000	ng/ul	0.00
20) Naphthalene-d8	10.263	136	384079	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.145	164	274612	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	579363	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.109	240	565902	20.000	ng/ul	# 0.00
88) Perylene-d12	23.250	264	494337	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	8832	4.618	ng/uL	0.00
4) Pyridine-d5	3.540	84	16936	3.118	ng/ul	0.02
7) Phenol-d5	6.704	99	46710	6.383	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.863	67	132735	31.349	ng/ul	0.00
11) 2-Chlorophenol-d4	7.045	132	152702	27.117	ng/ul	0.00
15) 4-Methylphenol-d8	8.216	113	101397	16.150	ng/ul	0.00
21) Nitrobenzene-d5	8.657	128	99077	35.516	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	111656	33.820	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.898	165	224416	33.880	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	77372	8.281	ng/ul	0.00
46) Dimethylphthalate-d6	13.574	166	793850	38.204	ng/ul	0.00
49) Acenaphthylene-d8	13.833	160	932322	37.886	ng/ul	0.00
54) 4-Nitrophenol-d4	14.398	143	18653	4.959	ng/ul	0.01
60) Fluorene-d10	15.151	176	710504	38.898	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.292	200	115671	29.056	ng/ul	0.00
73) Anthracene-d10	17.004	188	1148144	41.752	ng/ul	0.00
81) Pyrene-d10	19.309	212	1335086	50.369	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.115	264	1083034	41.687	ng/ul	0.00
Target Compounds						
					Qvalue	
47) Dimethylphthalate	13.622	163	138845	6.805	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031980.D
Acq On : 31 Aug 2021 11:18
Operator : CG/JU
Sample : M3474-11
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Quant Time: Aug 31 11:48:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

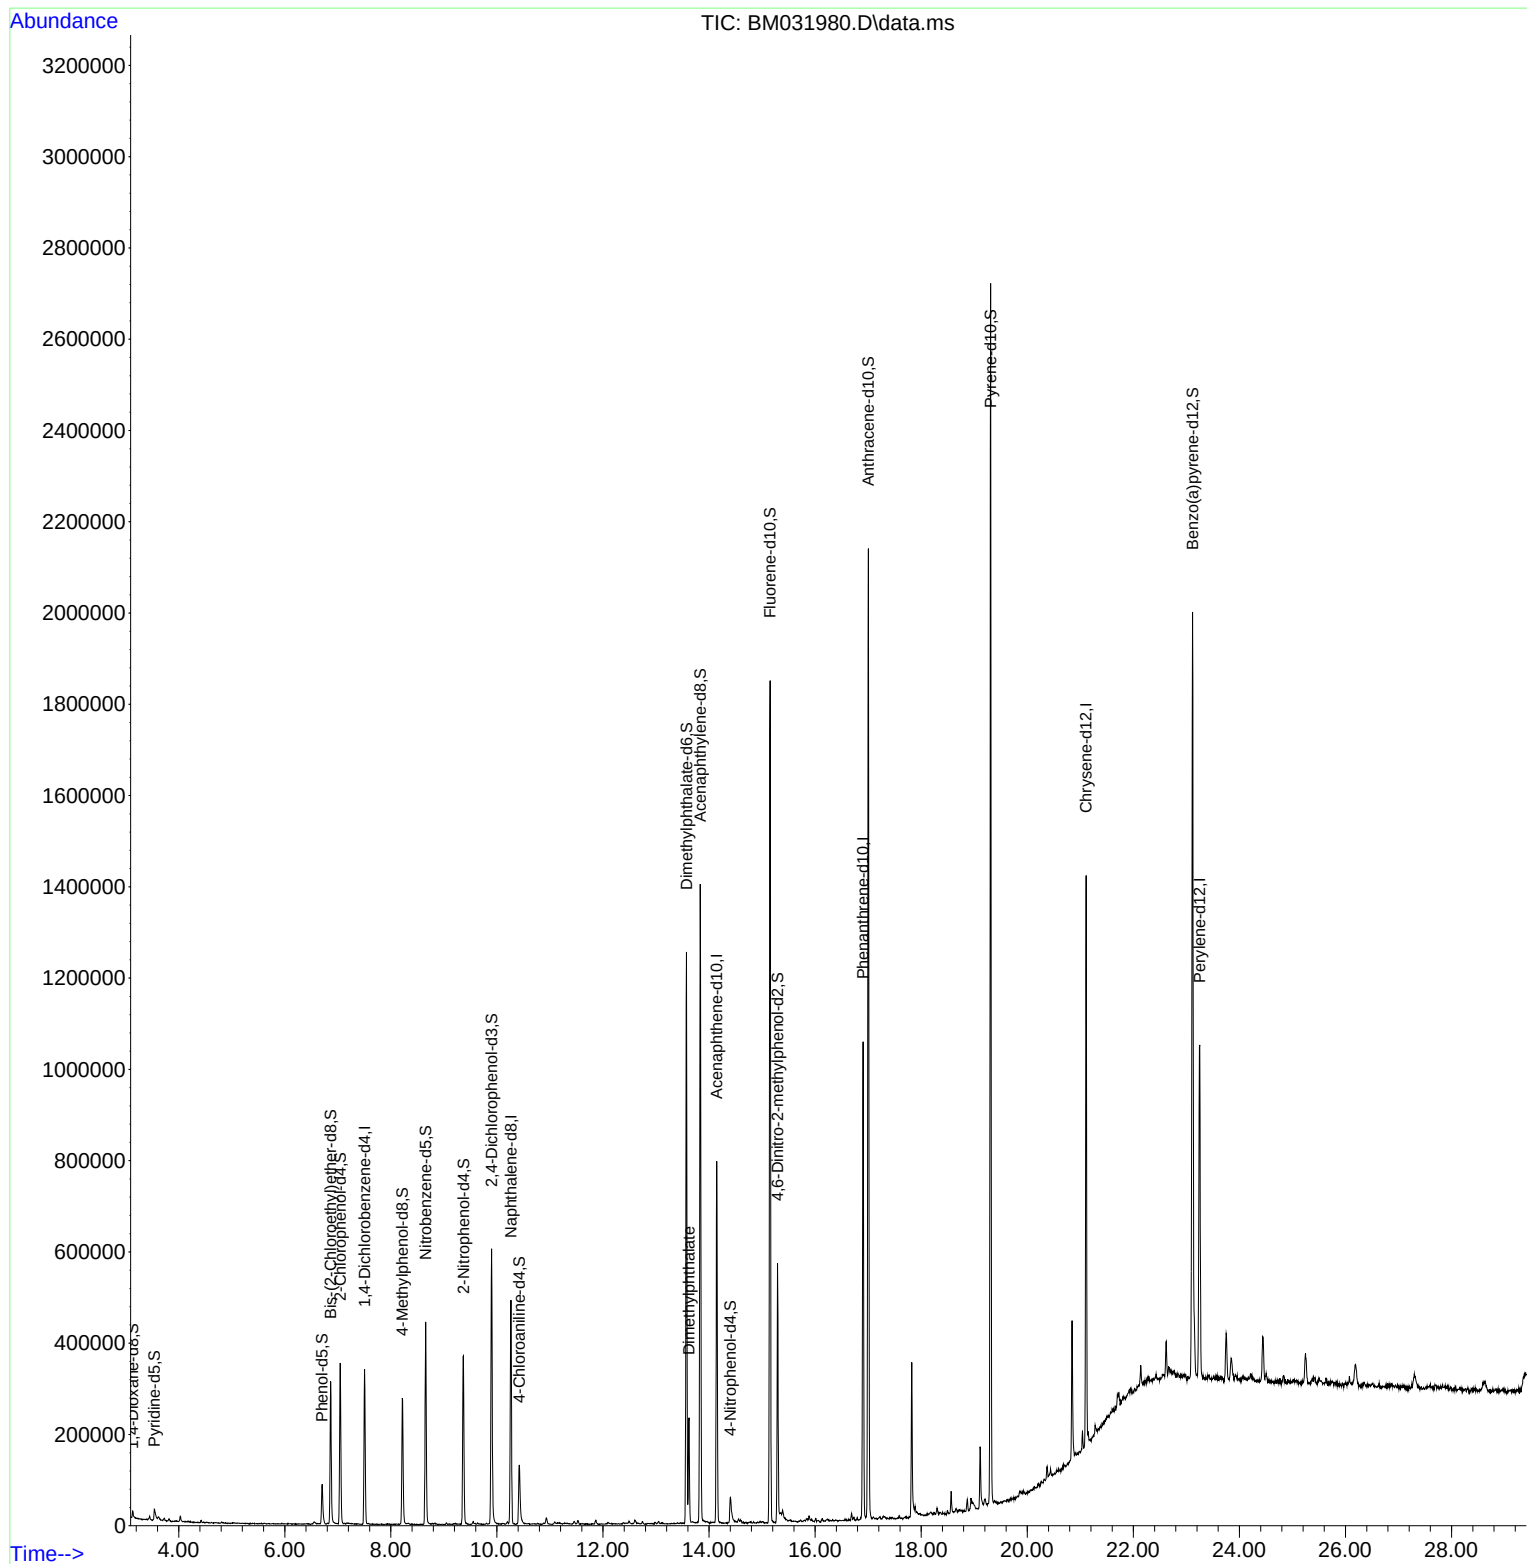

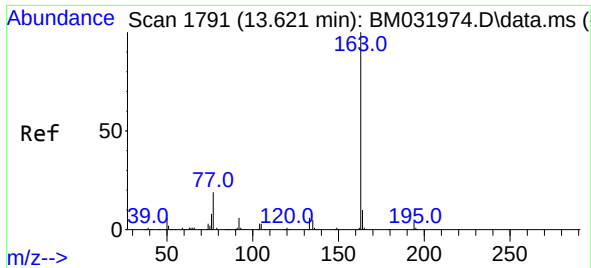

#47
Dimethylphthalate
Concen: 6.805 ng/ul
RT: 13.622 min Scan# 1791
Delta R.T. -0.006 min
Lab File: BM031980.D
Acq: 31 Aug 2021 11:18

Instrument :
BNA_M
ClientSampleId :
C0AC2

Tgt Ion:163 Resp: 138845
Ion Ratio Lower Upper
163 100
194 4.1 3.2 4.8
164 10.0 8.2 12.4

