

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031981.D
 Acq On : 31 Aug 2021 11:55
 Operator : CG/JU
 Sample : M3474-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC5

Quant Time: Aug 31 12:37:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 09:21:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.504	152	95326	20.000	ng/ul	0.00
20) Naphthalene-d8	10.263	136	404768	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.145	164	287145	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	606687	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.109	240	583945	20.000	ng/ul	# 0.00
88) Perylene-d12	23.244	264	492857	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	9597	4.645	ng/uL	0.00
4) Pyridine-d5	3.534	84	29368	5.006	ng/ul	0.01
7) Phenol-d5	6.704	99	31810	4.024	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.863	67	104836	22.922	ng/ul	0.00
11) 2-Chlorophenol-d4	7.045	132	107814	17.724	ng/ul	0.00
15) 4-Methylphenol-d8	8.222	113	62235	9.177	ng/ul	0.00
21) Nitrobenzene-d5	8.657	128	78372	26.658	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	83941	24.126	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.898	165	156373	22.401	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131	65494	6.651	ng/ul	0.00
46) Dimethylphthalate-d6	13.574	166	690733	31.791	ng/ul	0.00
49) Acenaphthylene-d8	13.833	160	730978	28.408	ng/ul	0.00
54) 4-Nitrophenol-d4	14.410	143	10518	2.674	ng/ul	0.02
60) Fluorene-d10	15.151	176	612636	32.076	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	51724	12.408	ng/ul	0.00
73) Anthracene-d10	17.004	188	1058707	36.765	ng/ul	0.00
81) Pyrene-d10	19.309	212	1236164	45.196	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.115	264	963007	37.178	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.621	163	141543	6.634	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031981.D
Acq On : 31 Aug 2021 11:55
Operator : CG/JU
Sample : M3474-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC5

Quant Time: Aug 31 12:37:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 09:21:30 2021
Response via : Initial Calibration

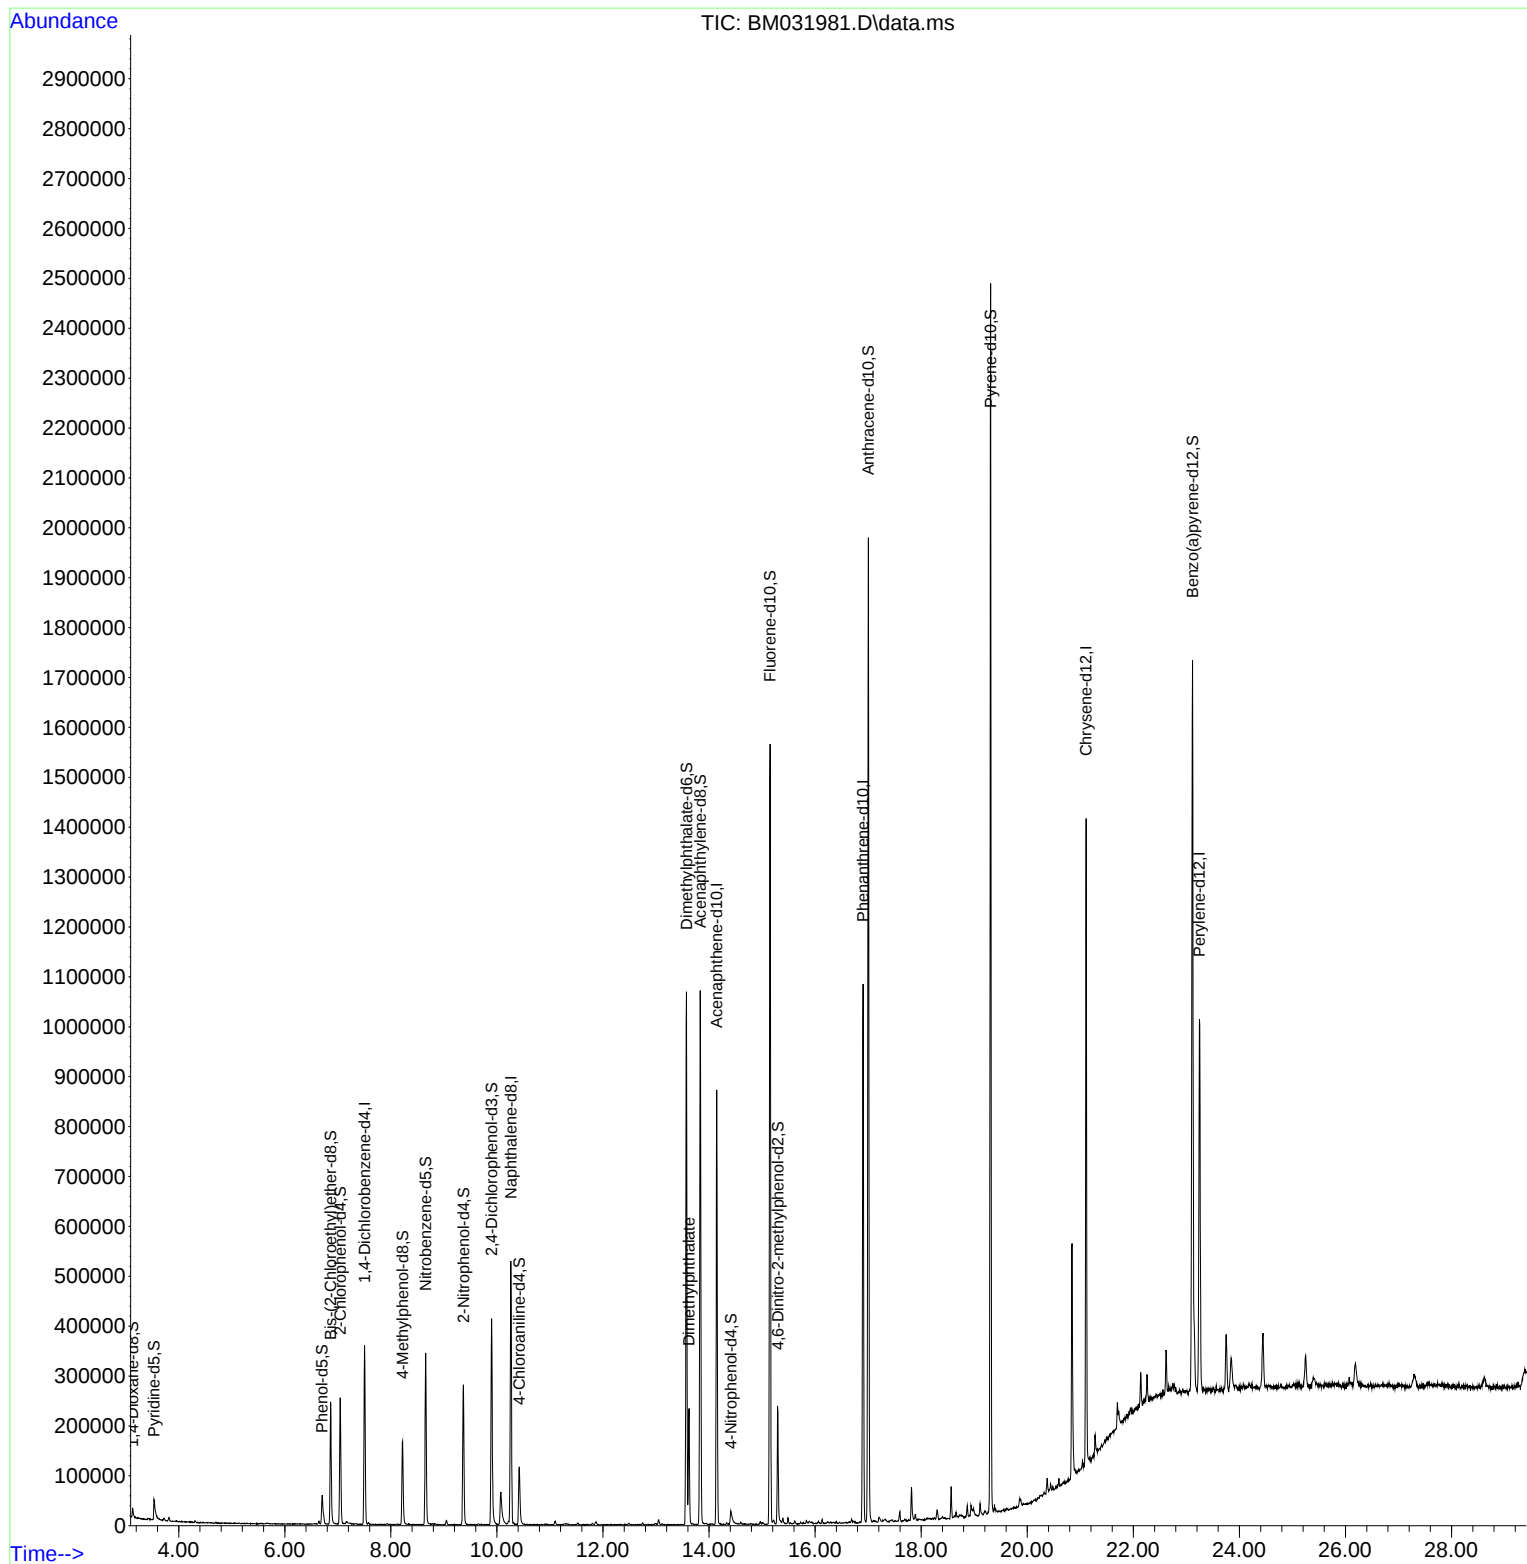

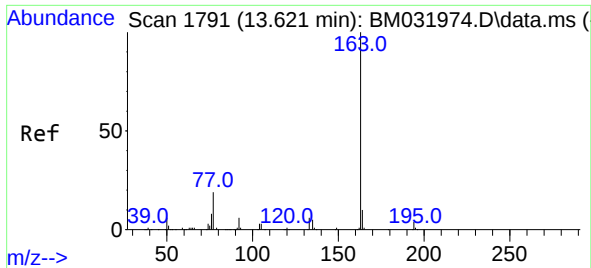

#47
 Dimethylphthalate
 Concen: 6.634 ng/ul
 RT: 13.621 min Scan# 1791
 Delta R.T. -0.006 min
 Lab File: BM031981.D
 Acq: 31 Aug 2021 11:55

Instrument :
 BNA_M
 ClientSampleId :
 C0AC5

Tgt Ion:163	Resp:	141543
Ion	Ratio	Lower Upper
163	100	
194	4.1	3.2 4.8
164	10.6	8.2 12.4

