

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM083021\  
 Data File : BM031984.D  
 Acq On : 31 Aug 2021 13:47  
 Operator : CG/JU  
 Sample : M3474-05  
 Misc :  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AC6

Quant Time: Aug 31 14:28:20 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM082821.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Aug 30 09:21:30 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)  |
|-------------------------------|--------|------|----------|--------|-------|-----------|
| -----                         |        |      |          |        |       |           |
| Internal Standards            |        |      |          |        |       |           |
| 1) 1,4-Dichlorobenzene-d4     | 7.504  | 152  | 85489    | 20.000 | ng/ul | 0.00      |
| 20) Naphthalene-d8            | 10.263 | 136  | 369487   | 20.000 | ng/ul | # 0.00    |
| 38) Acenaphthene-d10          | 14.145 | 164  | 269005   | 20.000 | ng/ul | 0.00      |
| 64) Phenanthrene-d10          | 16.904 | 188  | 578085   | 20.000 | ng/ul | # 0.00    |
| 79) Chrysene-d12              | 21.109 | 240  | 568925   | 20.000 | ng/ul | # 0.00    |
| 88) Perylene-d12              | 23.250 | 264  | 489960   | 20.000 | ng/ul | 0.00      |
| System Monitoring Compounds   |        |      |          |        |       |           |
| 3) 1,4-Dioxane-d8             | 3.134  | 96   | 8208     | 4.430  | ng/uL | 0.00      |
| 4) Pyridine-d5                | 3.534  | 84   | 24384    | 4.634  | ng/ul | 0.01      |
| 7) Phenol-d5                  | 6.704  | 99   | 40192    | 5.670  | ng/ul | 0.00      |
| 9) Bis-(2-Chloroethyl)eth...  | 6.863  | 67   | 108824   | 26.532 | ng/ul | 0.00      |
| 11) 2-Chlorophenol-d4         | 7.045  | 132  | 119054   | 21.824 | ng/ul | 0.00      |
| 15) 4-Methylphenol-d8         | 8.222  | 113  | 80402    | 13.219 | ng/ul | 0.00      |
| 21) Nitrobenzene-d5           | 8.657  | 128  | 81678    | 30.435 | ng/ul | 0.00      |
| 24) 2-Nitrophenol-d4          | 9.369  | 143  | 87852    | 27.661 | ng/ul | 0.00      |
| 28) 2,4-Dichlorophenol-d3     | 9.898  | 165  | 161237   | 25.303 | ng/ul | 0.00      |
| 31) 4-Chloroaniline-d4        | 10.422 | 131  | 96954    | 10.786 | ng/ul | 0.00      |
| 46) Dimethylphthalate-d6      | 13.574 | 166  | 633400   | 31.118 | ng/ul | 0.00      |
| 49) Acenaphthylene-d8         | 13.833 | 160  | 727703   | 30.188 | ng/ul | 0.00      |
| 54) 4-Nitrophenol-d4          | 14.410 | 143  | 16359    | 4.440  | ng/ul | 0.02      |
| 60) Fluorene-d10              | 15.151 | 176  | 559603   | 31.275 | ng/ul | 0.00      |
| 65) 4,6-Dinitro-2-methylph... | 15.292 | 200  | 88222    | 22.210 | ng/ul | 0.00      |
| 73) Anthracene-d10            | 17.004 | 188  | 1007719  | 36.726 | ng/ul | 0.00      |
| 81) Pyrene-d10                | 19.309 | 212  | 1163394  | 43.658 | ng/ul | 0.00      |
| 92) Benzo(a)pyrene-d12        | 23.115 | 264  | 940025   | 36.505 | ng/ul | 0.00      |
| Target Compounds              |        |      |          |        |       |           |
| 47) Dimethylphthalate         | 13.622 | 163  | 178298   | 8.921  | ng/ul | Qvalue 99 |
| -----                         |        |      |          |        |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM083021\  
Data File : BM031984.D  
Acq On : 31 Aug 2021 13:47  
Operator : CG/JU  
Sample : M3474-05  
Misc :  
ALS Vial : 44 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0AC6

Quant Time: Aug 31 14:28:20 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM082821.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Aug 30 09:21:30 2021  
Response via : Initial Calibration

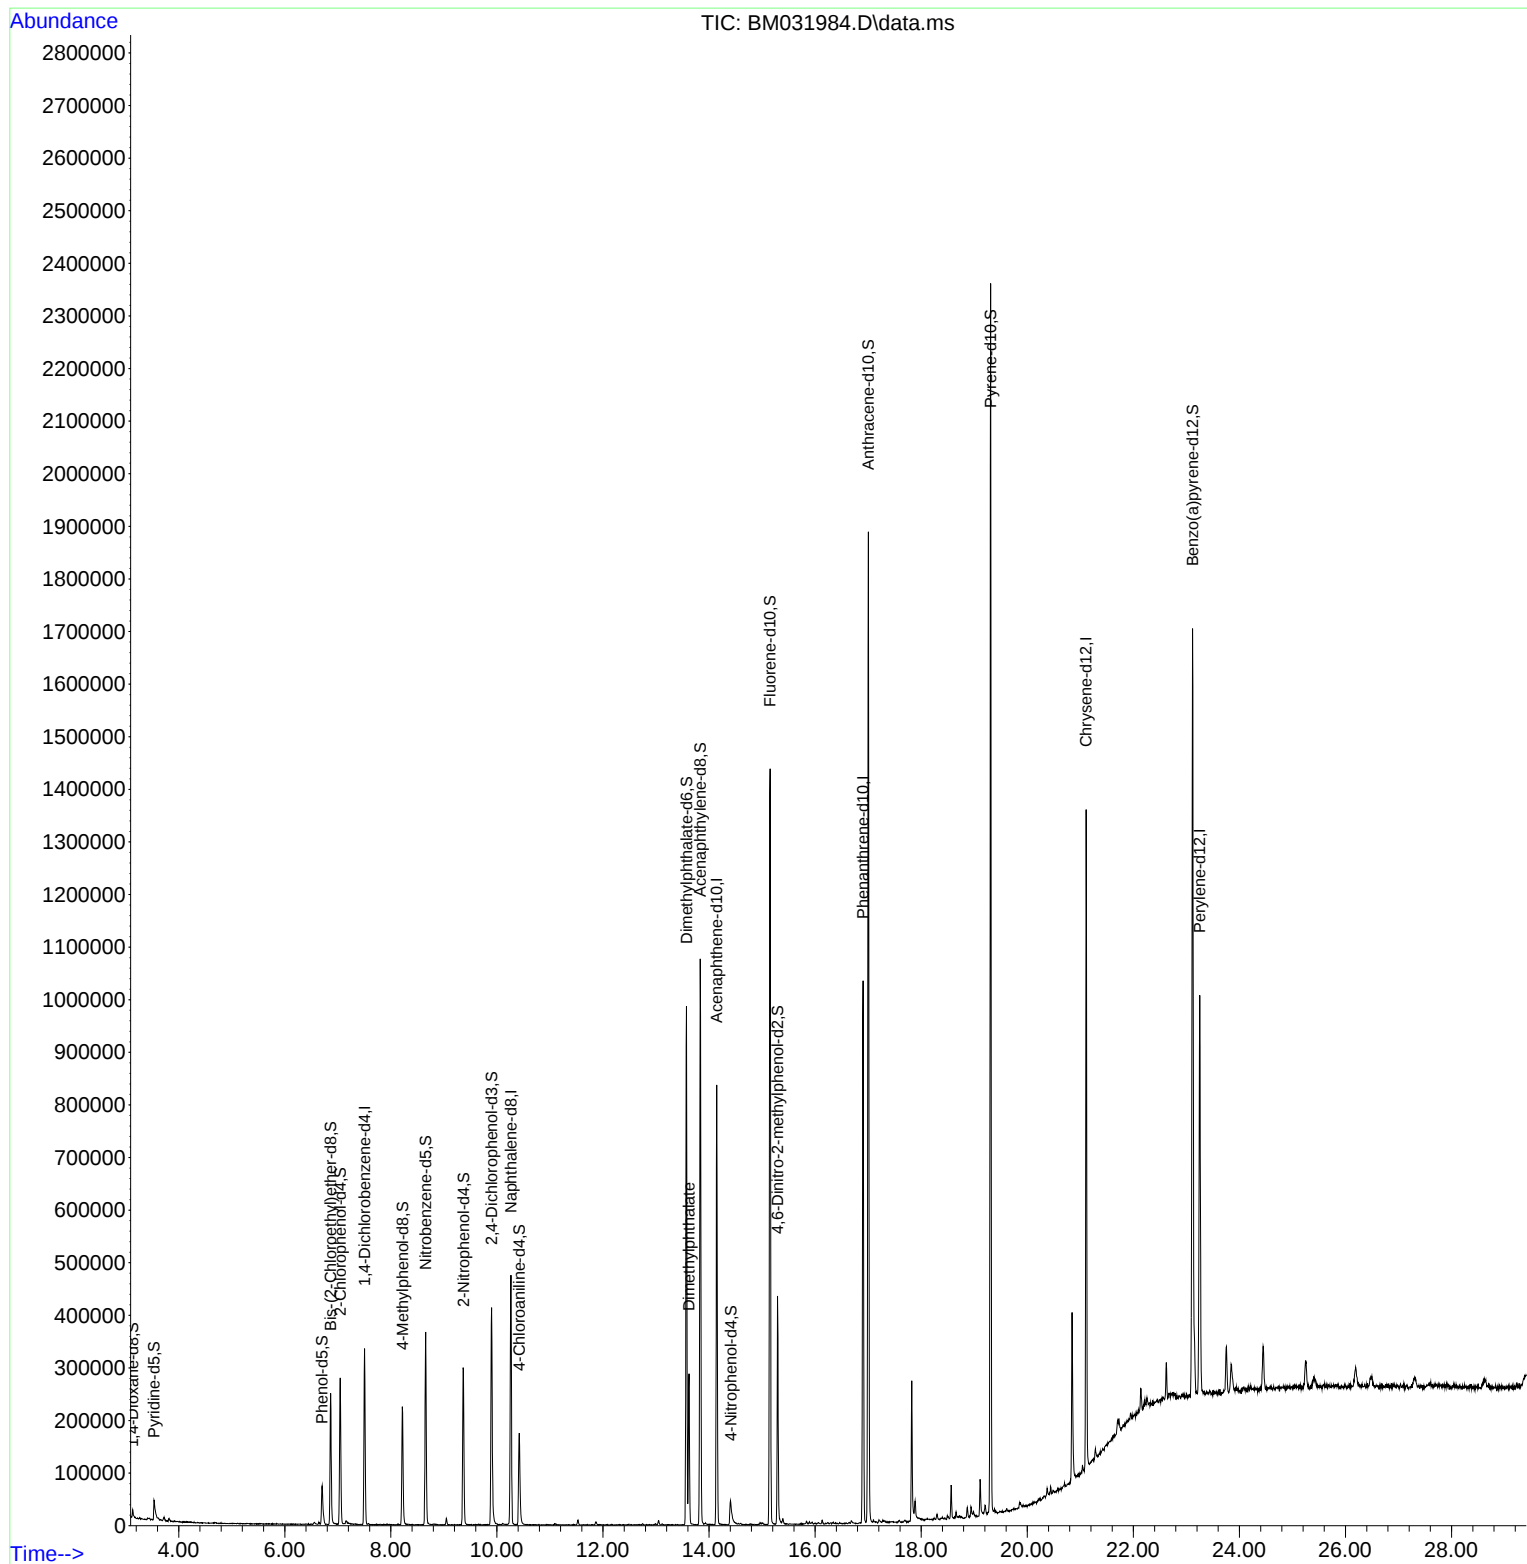

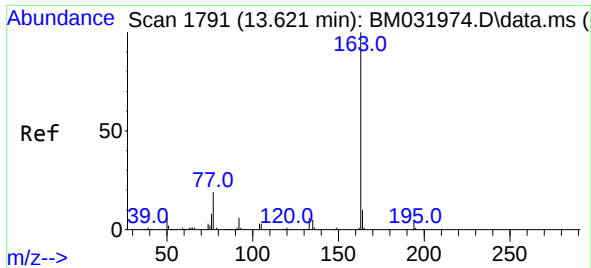

#47  
 Dimethylphthalate  
 Concen: 8.921 ng/ul  
 RT: 13.622 min Scan# 1791  
 Delta R.T. -0.006 min  
 Lab File: BM031984.D  
 Acq: 31 Aug 2021 13:47

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AC6

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:163 | Resp: | 178298      |
| Ion         | Ratio | Lower Upper |
| 163         | 100   |             |
| 194         | 3.9   | 3.2 4.8     |
| 164         | 9.7   | 8.2 12.4    |

