

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031942.D
 Acq On : 30 Aug 2021 09:50
 Operator : CG/JU
 Sample : PB138564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	12	rBV	16943	23454	0.74%	0.091%
2	3.522	71	74	93	rBV	207618	399991	12.63%	1.556%
3	3.816	120	124	131	rBV8	3529	6328	0.20%	0.025%
4	6.704	609	615	628	rBV	335913	549468	17.35%	2.137%
5	6.869	637	643	660	rVB	246961	408147	12.89%	1.588%
6	7.045	667	673	685	rVB	346198	565279	17.85%	2.199%
7	7.510	746	752	762	rBV	241048	382103	12.07%	1.486%
8	8.222	867	873	888	rBV	423070	700075	22.11%	2.723%
9	8.657	940	947	960	rBV	344981	584490	18.46%	2.274%
10	9.369	1061	1068	1079	rBV	310226	505728	15.97%	1.967%
11	9.898	1152	1158	1177	rBV	414118	763571	24.11%	2.970%
12	10.269	1213	1221	1232	rBV	347839	578296	18.26%	2.250%
13	10.422	1240	1247	1260	rBV	415571	784363	24.77%	3.051%
14	11.886	1491	1496	1501	rBV3	5481	10081	0.32%	0.039%
15	13.574	1777	1783	1794	rBV	931589	1352615	42.71%	5.262%
16	13.839	1819	1828	1837	rBV	1084683	1538171	48.57%	5.984%
17	14.151	1874	1881	1888	rBV	624650	888345	28.05%	3.456%
18	14.386	1914	1921	1945	rBV	332573	643290	20.31%	2.502%
19	15.151	2044	2051	2059	rBV	1401341	1986108	62.72%	7.726%
20	15.298	2070	2076	2090	rBV	449555	671544	21.21%	2.612%
21	15.392	2090	2092	2096	rVB3	10689	12320	0.39%	0.048%
22	16.692	2309	2313	2320	rBV4	2446	5374	0.17%	0.021%
23	16.904	2343	2349	2358	rBV	827567	1137056	35.91%	4.423%
24	17.004	2360	2366	2378	rBV	1663160	2301830	72.69%	8.954%
25	18.633	2641	2643	2648	rBV7	1887	3613	0.11%	0.014%
26	18.874	2680	2684	2691	rVB3	16093	21419	0.68%	0.083%
27	18.945	2691	2696	2700	rBV2	15729	22499	0.71%	0.088%
28	19.250	2746	2748	2751	rBV3	2850	3210	0.10%	0.012%
29	19.309	2752	2758	2769	rVV	2061355	2755261	87.01%	10.718%
30	19.539	2795	2797	2799	rBV3	3067	3381	0.11%	0.013%
31	21.109	3059	3064	3072	rBV	1021952	1393083	43.99%	5.419%
32	23.115	3399	3405	3418	rVB2	1796276	3166637	100.00%	12.318%
33	23.250	3422	3428	3441	rVB2	822979	1539458	48.61%	5.989%




Sum of corrected areas: 25706588

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031942.D
Acq On : 30 Aug 2021 09:50
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

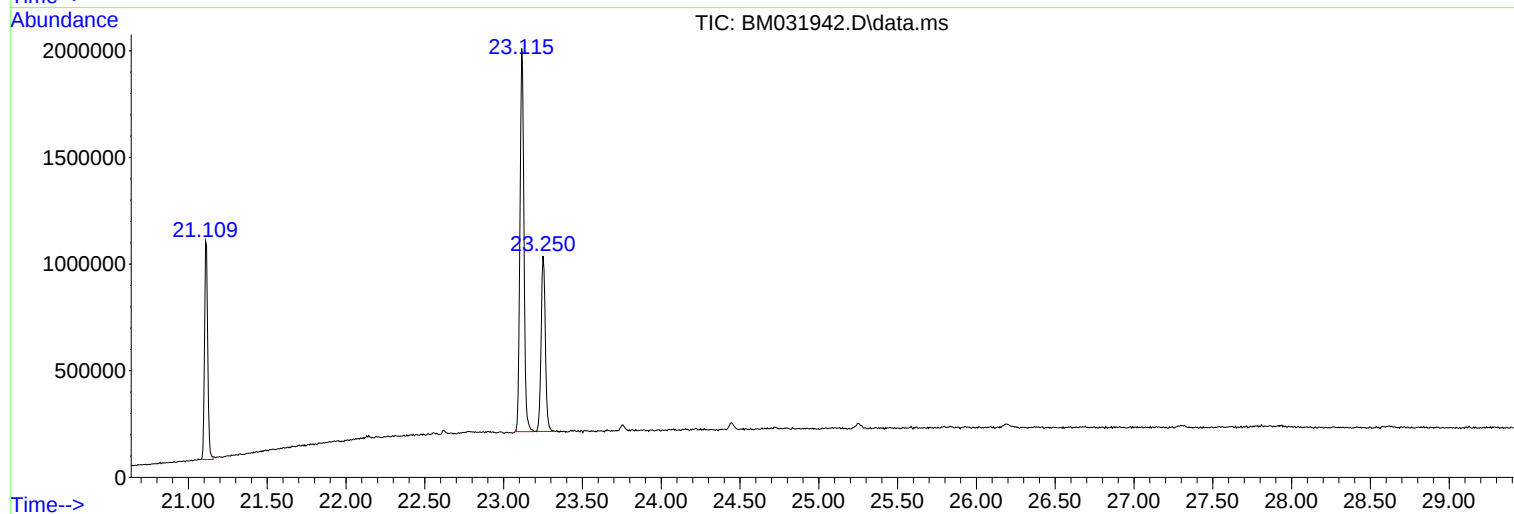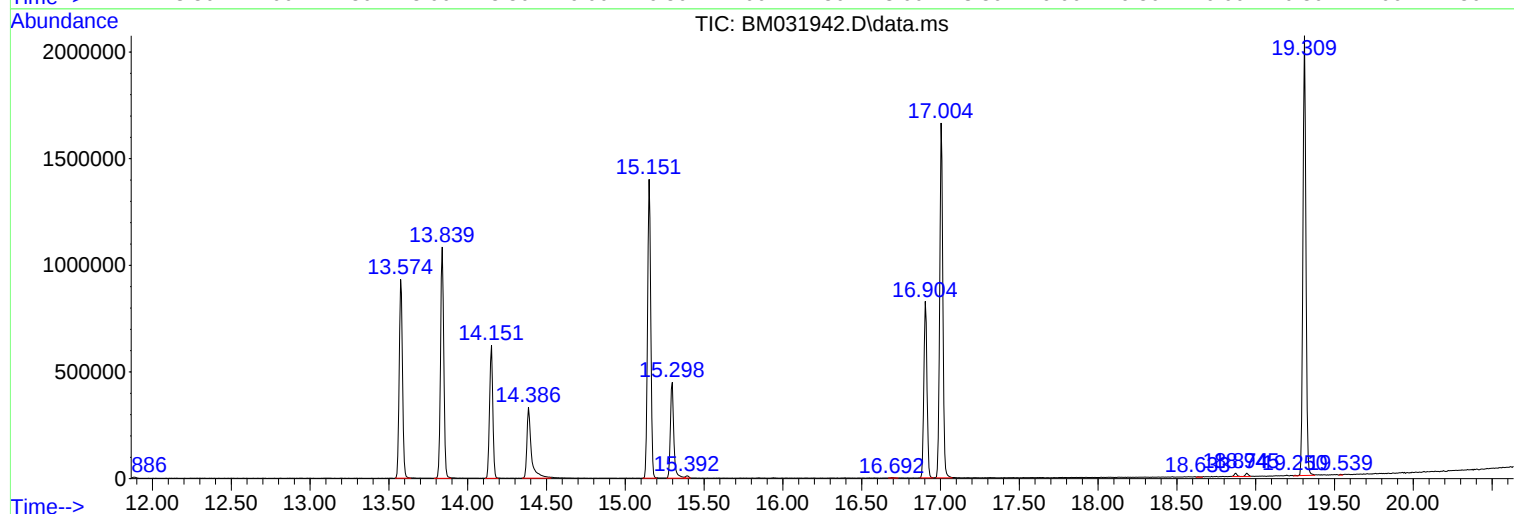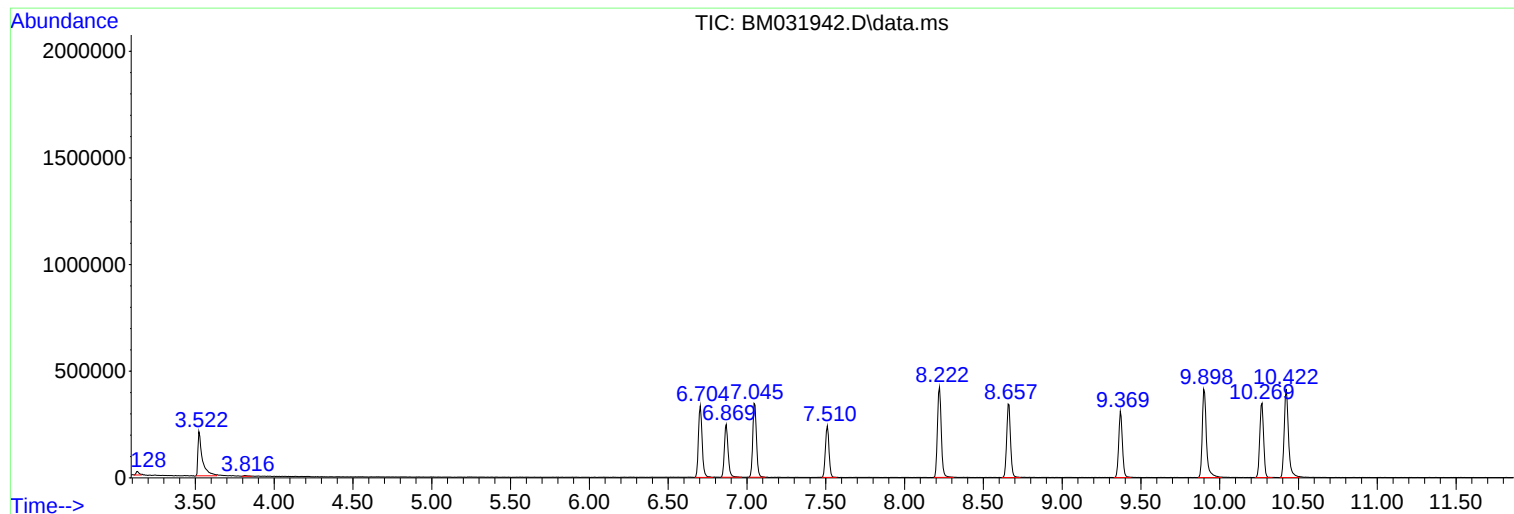

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031942.D
Acq On : 30 Aug 2021 09:50
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031942.D
Acq On : 30 Aug 2021 09:50
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
