

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031945.D
 Acq On : 30 Aug 2021 11:40
 Operator : CG/JU
 Sample : M3365-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	18	rVB4	6947	14414	0.36%	0.049%
2	3.540	71	77	87	rBV2	36444	87743	2.20%	0.297%
3	3.622	87	91	99	rVV	64030	99747	2.50%	0.337%
4	3.687	99	102	105	rVV	10921	16013	0.40%	0.054%
5	3.728	105	109	116	rVB3	11018	19519	0.49%	0.066%
6	3.816	121	124	129	rVB2	8632	13298	0.33%	0.045%
7	4.352	211	215	222	rVB5	8363	13602	0.34%	0.046%
8	4.693	269	273	279	rVB3	5122	8171	0.20%	0.028%
9	4.804	288	292	298	rBV3	6037	10591	0.27%	0.036%
10	5.546	413	418	427	rVB5	4124	8106	0.20%	0.027%
11	6.704	605	615	627	rBV	123190	259609	6.51%	0.878%
12	6.869	636	643	653	rBV	93772	158986	3.99%	0.538%
13	7.051	666	674	683	rVV	128372	212981	5.34%	0.720%
14	7.134	683	688	693	rVB7	3495	6503	0.16%	0.022%
15	7.510	745	752	761	rBV	669370	1045587	26.22%	3.536%
16	8.228	868	874	882	rBV	45061	76062	1.91%	0.257%
17	8.334	886	892	901	rBV	56129	99519	2.50%	0.337%
18	8.663	942	948	956	rBV	131678	221302	5.55%	0.749%
19	8.769	961	966	972	rVB5	3158	5949	0.15%	0.020%
20	9.375	1062	1069	1076	rBV	109106	188494	4.73%	0.638%
21	9.563	1095	1101	1110	rBV2	13332	32793	0.82%	0.111%
22	9.739	1126	1131	1137	rVB3	14483	22956	0.58%	0.078%
23	9.904	1153	1159	1178	rVB	152994	287277	7.20%	0.972%
24	10.081	1184	1189	1206	rBV2	32493	85426	2.14%	0.289%
25	10.269	1212	1221	1230	rBV	970774	1605173	40.25%	5.429%
26	10.428	1242	1248	1258	rBV2	83376	171986	4.31%	0.582%
27	10.839	1313	1318	1325	rBV6	4273	9957	0.25%	0.034%
28	11.104	1356	1363	1368	rBV5	6615	16201	0.41%	0.055%
29	12.745	1638	1642	1647	rBV5	3413	5084	0.13%	0.017%
30	13.574	1777	1783	1795	rBV	370321	535148	13.42%	1.810%
31	13.839	1821	1828	1838	rBV	406699	602751	15.12%	2.039%
32	14.151	1874	1881	1888	rBV	1738329	2444577	61.30%	8.268%
33	14.210	1888	1891	1897	rVB4	8711	14337	0.36%	0.048%
34	14.398	1918	1923	1938	rBV	71618	175043	4.39%	0.592%
35	14.563	1946	1951	1955	rBV3	11643	19492	0.49%	0.066%
36	14.598	1955	1957	1965	rVB5	16165	20817	0.52%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031945.D
 Acq On : 30 Aug 2021 11:40
 Operator : CG/JU
 Sample : M3365-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

37	15.151	2045	2051	2058	rBV	592224	823543	20.65%	2.785%
38	15.210	2058	2061	2066	rVB5	9108	15421	0.39%	0.052%
39	15.298	2071	2076	2086	rBV	121470	180047	4.52%	0.609%
40	15.392	2088	2092	2096	rVB3	6183	8793	0.22%	0.030%
41	15.892	2172	2177	2184	rBV3	10020	15963	0.40%	0.054%
42	16.210	2223	2231	2237	rBV	48873	64502	1.62%	0.218%
43	16.463	2272	2274	2278	rBV3	4134	5201	0.13%	0.018%
44	16.574	2288	2293	2299	rBV	15072	26072	0.65%	0.088%
45	16.645	2301	2305	2309	rBV3	2806	5039	0.13%	0.017%
46	16.692	2309	2313	2316	rVV2	7504	12658	0.32%	0.043%
47	16.727	2316	2319	2324	rVB	13313	17049	0.43%	0.058%
48	16.827	2333	2336	2339	rBV	4710	5065	0.13%	0.017%
49	16.904	2343	2349	2354	rVV	2064231	3082259	77.29%	10.425%
50	16.945	2354	2356	2361	rVV	363279	463230	11.62%	1.567%
51	17.004	2361	2366	2378	rVV	618198	904460	22.68%	3.059%
52	17.104	2378	2383	2392	rVV2	28147	44557	1.12%	0.151%
53	17.327	2412	2421	2426	rBV	33163	59396	1.49%	0.201%
54	17.433	2433	2439	2445	rBV6	6324	14535	0.36%	0.049%
55	17.598	2461	2467	2471	rBV9	7337	11860	0.30%	0.040%
56	17.698	2477	2484	2491	rBV7	10640	24028	0.60%	0.081%
57	17.786	2494	2499	2501	rVV	28769	40723	1.02%	0.138%
58	17.821	2501	2505	2512	rVV3	87870	152376	3.82%	0.515%
59	17.886	2512	2516	2525	rVV2	49521	79546	1.99%	0.269%
60	17.974	2525	2531	2535	rVV2	46937	76558	1.92%	0.259%
61	18.009	2535	2537	2543	rVB2	18365	25901	0.65%	0.088%
62	18.145	2557	2560	2564	rVV5	5912	9150	0.23%	0.031%
63	18.180	2564	2566	2572	rVB6	3642	5895	0.15%	0.020%
64	18.292	2581	2585	2588	rBV	31327	40416	1.01%	0.137%
65	18.339	2588	2593	2599	rVV	80872	115487	2.90%	0.391%
66	18.392	2599	2602	2609	rVB3	18636	29006	0.73%	0.098%
67	18.533	2623	2626	2630	rBV5	9299	14200	0.36%	0.048%
68	18.586	2632	2635	2638	rVB4	7009	8845	0.22%	0.030%
69	18.627	2638	2642	2646	rBV2	26904	35237	0.88%	0.119%
70	18.709	2652	2656	2660	rBV2	15472	22800	0.57%	0.077%
71	18.809	2670	2673	2675	rBV3	5602	6426	0.16%	0.022%
72	18.856	2675	2681	2693	rVV5	46250	138896	3.48%	0.470%
73	18.974	2695	2701	2709	rVV	814341	1081249	27.11%	3.657%
74	19.039	2709	2712	2716	rVB5	9924	14671	0.37%	0.050%
75	19.080	2716	2719	2721	rBV3	8999	9216	0.23%	0.031%
76	19.115	2721	2725	2730	rBV3	38255	55591	1.39%	0.188%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031945.D
 Acq On : 30 Aug 2021 11:40
 Operator : CG/JU
 Sample : M3365-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

77	19.309	2752	2758	2761	rBV	1001461	1446252	36.27%	4.892%
78	19.339	2761	2763	2771	rVV	646822	713005	17.88%	2.412%
79	19.415	2772	2776	2783	rVB2	28033	40098	1.01%	0.136%
80	19.527	2788	2795	2799	rVV2	31272	53697	1.35%	0.182%
81	19.680	2814	2821	2826	rBV5	27601	68918	1.73%	0.233%
82	19.803	2838	2842	2844	rBV4	31387	44286	1.11%	0.150%
83	19.845	2846	2849	2853	rVB	47283	60973	1.53%	0.206%
84	19.945	2863	2866	2870	rVB2	29575	32874	0.82%	0.111%
85	19.998	2870	2875	2879	rBV3	48579	81909	2.05%	0.277%
86	20.139	2896	2899	2902	rVB2	19737	24529	0.62%	0.083%
87	20.186	2904	2907	2912	rVV3	20153	29788	0.75%	0.101%
88	20.339	2931	2933	2937	rVB4	18824	15221	0.38%	0.051%
89	20.598	2973	2977	2982	rBV	67218	89221	2.24%	0.302%
90	20.756	3000	3004	3008	rBV2	74355	109606	2.75%	0.371%
91	20.798	3008	3011	3014	rVV	53044	61085	1.53%	0.207%
92	20.850	3014	3020	3024	rVV2	58624	133918	3.36%	0.453%
93	20.892	3024	3027	3032	rVB	68319	96316	2.42%	0.326%
94	21.115	3058	3065	3068	rBV	2958634	3987676	100.00%	13.488%
95	21.150	3068	3071	3078	rVB	392413	489673	12.28%	1.656%
96	22.621	3316	3321	3325	rBV	346934	666660	16.72%	2.255%
97	23.068	3393	3397	3400	rBV	158206	238226	5.97%	0.806%
98	23.115	3400	3405	3409	rVV2	588448	980473	24.59%	3.316%
99	23.156	3410	3412	3420	rVB	266870	369644	9.27%	1.250%
100	23.256	3422	3429	3435	rBV2	1893560	3370471	84.52%	11.400%




Sum of corrected areas: 29565600

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031945.D
Acq On : 30 Aug 2021 11:40
Operator : CG/JU
Sample : M3365-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK80

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

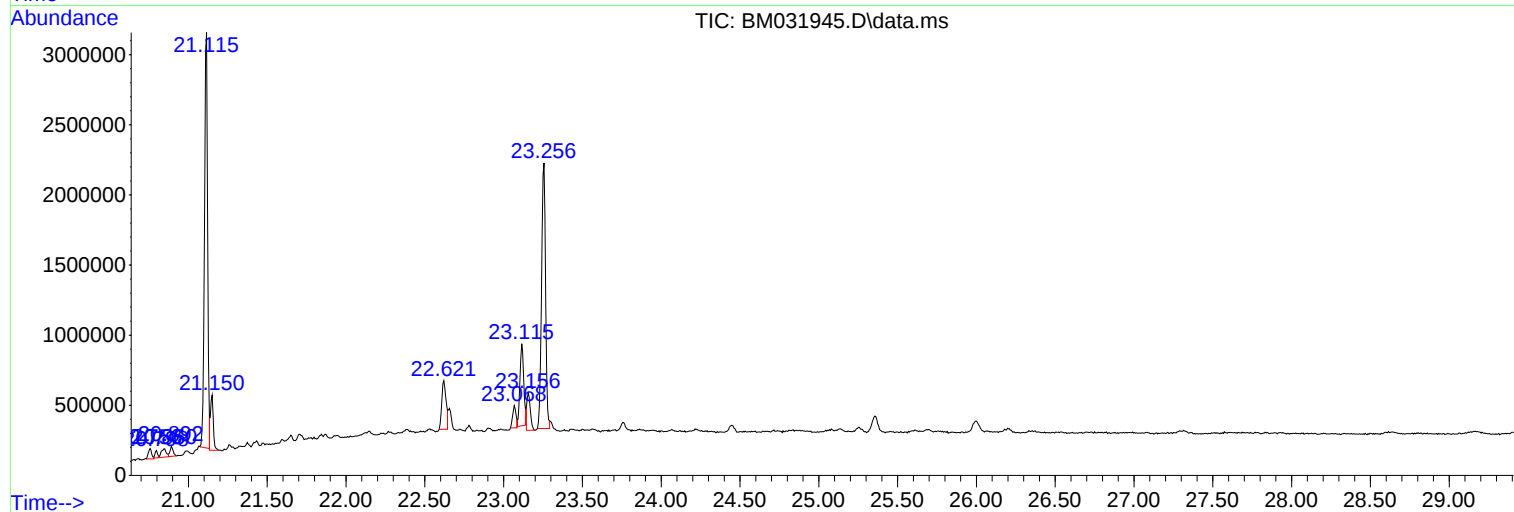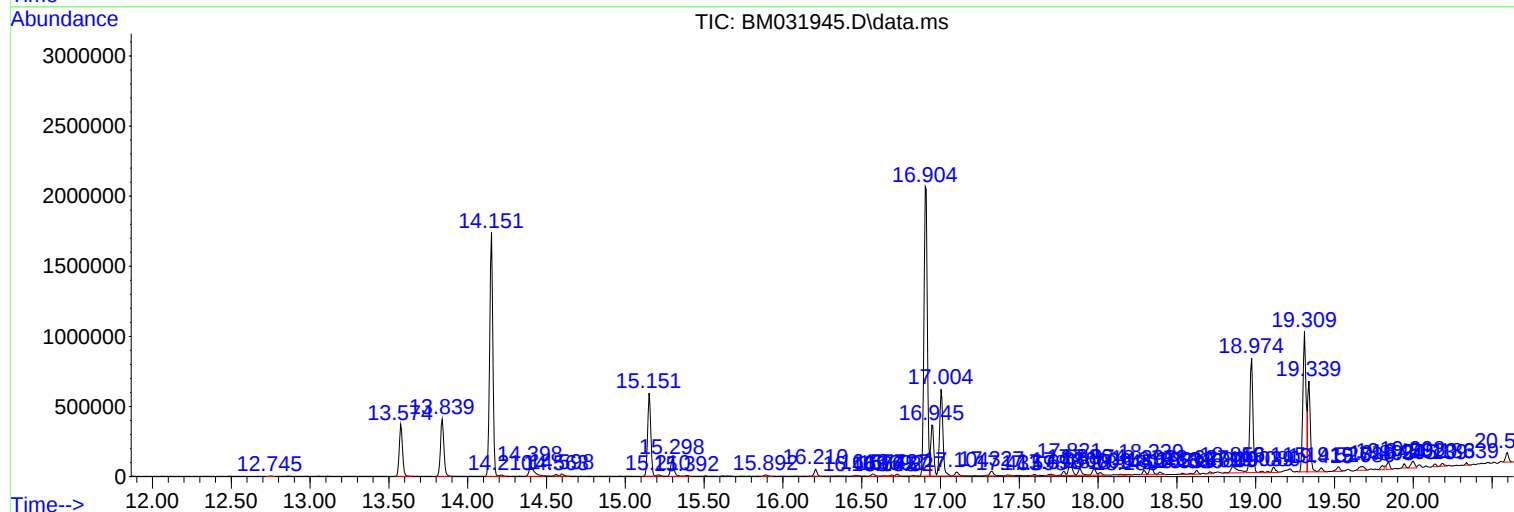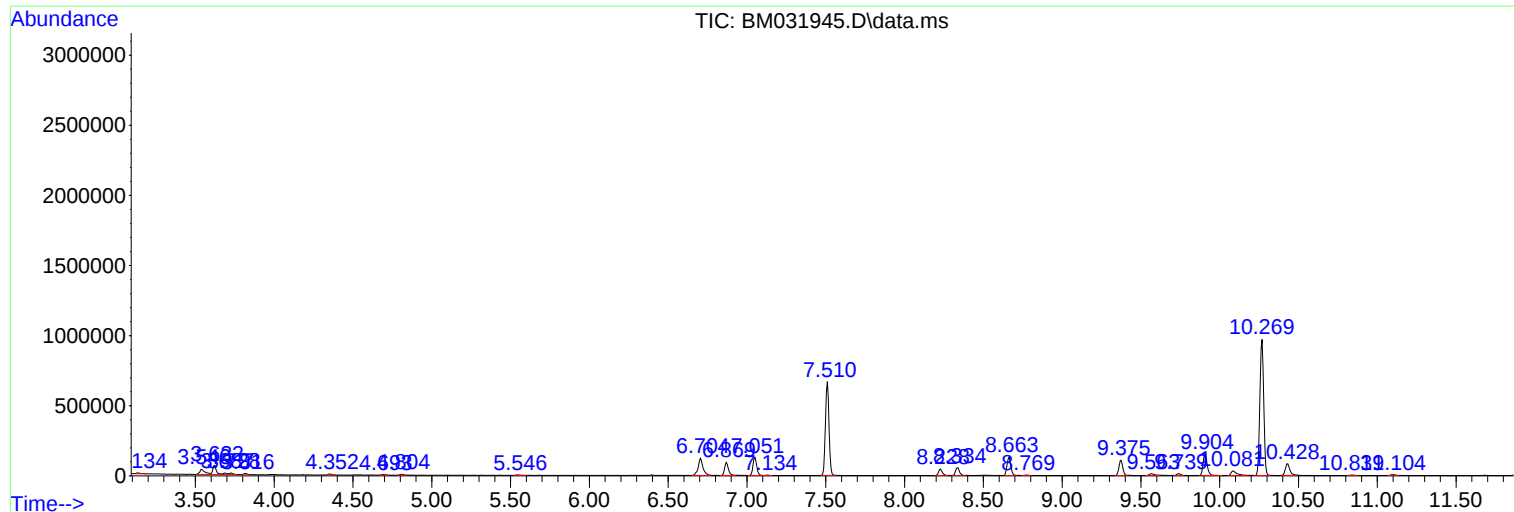

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031945.D
Acq On : 30 Aug 2021 11:40
Operator : CG/JU
Sample : M3365-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK80

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031945.D
Acq On : 30 Aug 2021 11:40
Operator : CG/JU
Sample : M3365-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK80

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
