

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031953.D
 Acq On : 30 Aug 2021 16:37
 Operator : CG/JU
 Sample : M3365-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	4	8	15	rVB2	11106	16879	0.74%	0.075%
2	3.534	72	76	98	rBV	59997	137172	6.03%	0.613%
3	3.728	104	109	116	rVB	13261	24807	1.09%	0.111%
4	3.817	119	124	131	rBV	23214	34677	1.52%	0.155%
5	4.040	157	162	165	rBV4	2179	3665	0.16%	0.016%
6	4.693	269	273	276	rBV3	4184	6976	0.31%	0.031%
7	4.716	276	277	284	rVB4	3574	5616	0.25%	0.025%
8	6.705	609	615	627	rBV	233789	385240	16.93%	1.721%
9	6.869	637	643	653	rBV	174157	286997	12.61%	1.282%
10	7.046	667	673	684	rBV	236452	393941	17.31%	1.760%
11	7.134	684	688	691	rVB4	3638	4456	0.20%	0.020%
12	7.510	745	752	761	rBV	334839	523685	23.01%	2.339%
13	8.222	866	873	878	rBV	301262	485428	21.33%	2.168%
14	8.275	878	882	890	rVV	102859	174510	7.67%	0.780%
15	8.340	890	893	898	rVB3	6395	9326	0.41%	0.042%
16	8.657	940	947	959	rBV	245405	418285	18.38%	1.868%
17	9.369	1062	1068	1079	rBV	202620	336178	14.77%	1.502%
18	9.904	1152	1159	1170	rBV	292424	535666	23.54%	2.393%
19	10.087	1184	1190	1210	rBV3	22188	70123	3.08%	0.313%
20	10.269	1213	1221	1231	rVB	473853	803339	35.30%	3.588%
21	10.422	1240	1247	1263	rBV	289060	547007	24.03%	2.443%
22	11.698	1453	1464	1471	rVB8	4998	11951	0.53%	0.053%
23	11.875	1489	1494	1498	rVB2	4760	7477	0.33%	0.033%
24	12.487	1593	1598	1606	rBV5	2124	4192	0.18%	0.019%
25	12.745	1637	1642	1647	rBV5	3166	5602	0.25%	0.025%
26	13.010	1683	1687	1690	rBV4	5147	8593	0.38%	0.038%
27	13.575	1777	1783	1799	rBV	715315	994246	43.69%	4.441%
28	13.839	1819	1828	1839	rBV	776221	1120256	49.22%	5.004%
29	13.998	1851	1855	1867	rVB2	9531	19110	0.84%	0.085%
30	14.151	1874	1881	1889	rBV	817135	1215475	53.41%	5.429%
31	14.210	1889	1891	1895	rVB2	2560	3290	0.14%	0.015%
32	14.339	1909	1913	1916	rBV2	2393	2445	0.11%	0.011%
33	14.392	1916	1922	1937	rBV2	154887	352536	15.49%	1.575%
34	14.610	1954	1959	1967	rVB7	6258	10074	0.44%	0.045%
35	14.922	2008	2012	2017	rBV2	9590	14815	0.65%	0.066%
36	14.963	2017	2019	2023	rVB4	2076	2468	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031953.D
 Acq On : 30 Aug 2021 16:37
 Operator : CG/JU
 Sample : M3365-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

37	15.151	2044	2051	2058	rBV	1077441	1471736	64.67%	6.574%
38	15.298	2070	2076	2089	rBV	245315	365541	16.06%	1.633%
39	15.392	2089	2092	2098	rVB3	6473	8686	0.38%	0.039%
40	15.616	2126	2130	2134	rBV2	4842	6210	0.27%	0.028%
41	15.886	2171	2176	2181	rBV4	3260	5859	0.26%	0.026%
42	16.692	2308	2313	2318	rBV3	4606	4941	0.22%	0.022%
43	16.904	2343	2349	2360	rVB	1119167	1523447	66.94%	6.805%
44	17.004	2360	2366	2376	rBV	1271471	1726349	75.85%	7.712%
45	17.127	2382	2387	2394	rVB7	12610	19380	0.85%	0.087%
46	17.286	2407	2414	2419	rBV8	5779	9892	0.43%	0.044%
47	17.604	2461	2468	2472	rVB7	7016	11836	0.52%	0.053%
48	17.710	2481	2486	2490	rVB5	2765	5243	0.23%	0.023%
49	17.822	2500	2505	2513	rBV2	50067	78606	3.45%	0.351%
50	17.892	2514	2517	2520	rVB5	3738	5185	0.23%	0.023%
51	18.110	2551	2554	2558	rBV5	1970	2311	0.10%	0.010%
52	18.163	2558	2563	2565	rBV6	2735	4534	0.20%	0.020%
53	18.227	2568	2574	2577	rBV6	2559	4162	0.18%	0.019%
54	18.621	2639	2641	2644	rBV4	2043	2680	0.12%	0.012%
55	18.727	2656	2659	2662	rBV5	1893	2323	0.10%	0.010%
56	18.874	2679	2684	2690	rBV5	11015	18591	0.82%	0.083%
57	18.945	2692	2696	2701	rBV	11292	18772	0.82%	0.084%
58	19.074	2716	2718	2721	rBV4	2955	4781	0.21%	0.021%
59	19.116	2721	2725	2730	rVV2	31793	45637	2.01%	0.204%
60	19.310	2752	2758	2770	rBV	1675476	2149602	94.45%	9.602%
61	20.845	3016	3019	3028	rBV4	49928	79856	3.51%	0.357%
62	21.115	3059	3065	3073	rBV	1381352	1796367	78.93%	8.024%
63	23.121	3399	3406	3419	rVB	1209580	2275916	100.00%	10.166%
64	23.251	3422	3428	3438	rVB2	963492	1761731	77.41%	7.870%




Sum of corrected areas: 22386677

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031953.D
Acq On : 30 Aug 2021 16:37
Operator : CG/JU
Sample : M3365-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

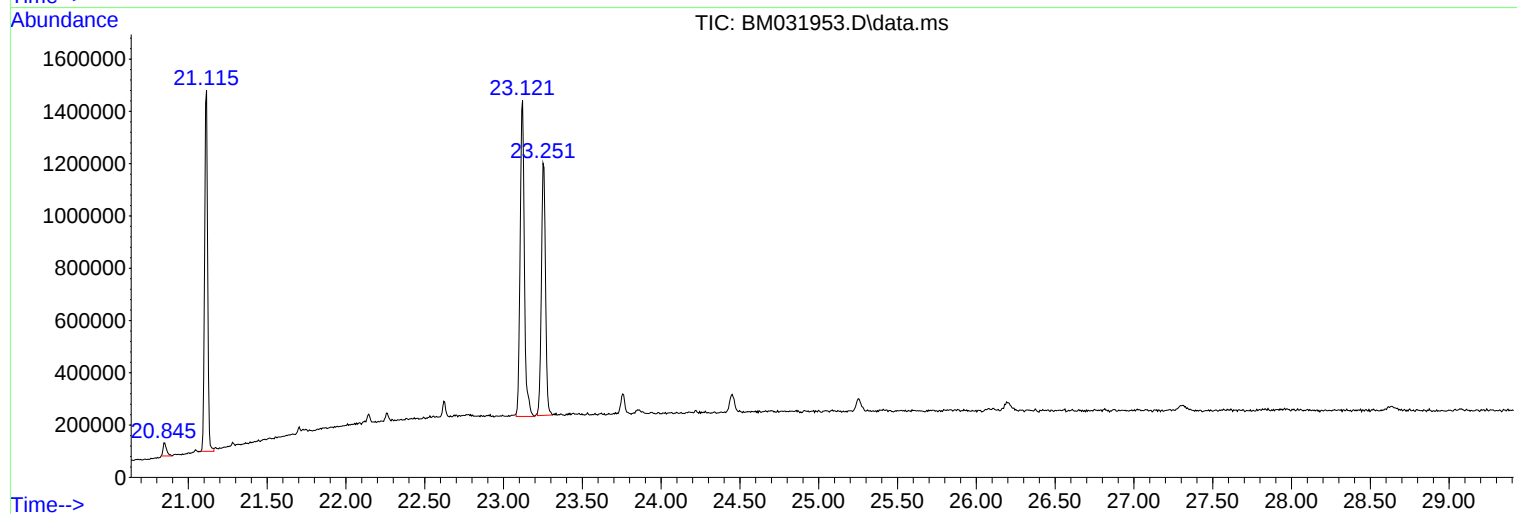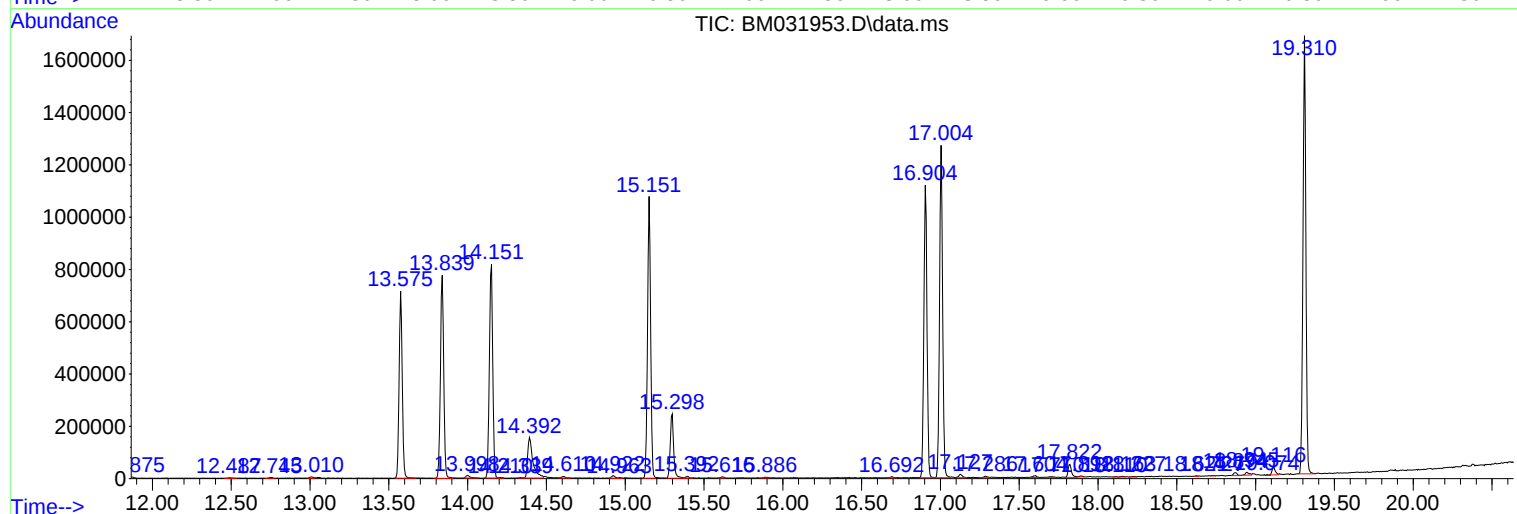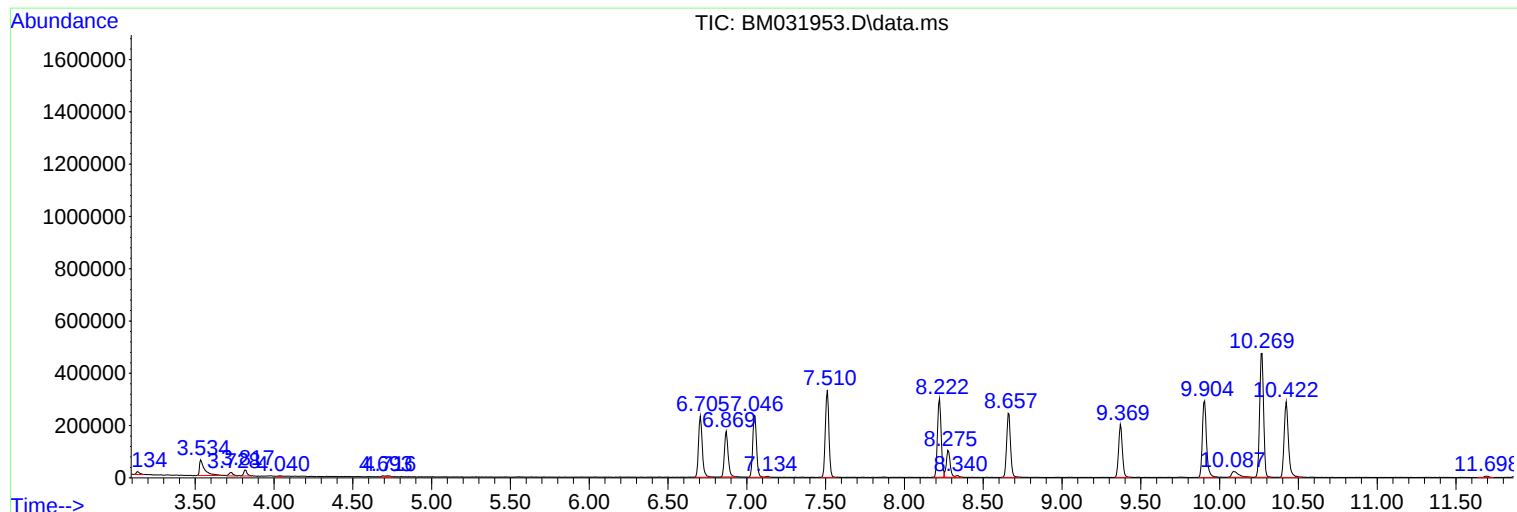

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031953.D
Acq On : 30 Aug 2021 16:37
Operator : CG/JU
Sample : M3365-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031953.D
Acq On : 30 Aug 2021 16:37
Operator : CG/JU
Sample : M3365-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
