

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031964.D
 Acq On : 31 Aug 2021 00:05
 Operator : CG/JU
 Sample : M3422-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBKD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	4	8	16	rVB	17099	25853	0.61%	0.082%
2	3.540	73	77	87	rBV	37679	80528	1.91%	0.254%
3	3.722	105	108	114	rVB5	7134	12095	0.29%	0.038%
4	3.816	121	124	128	rVB2	4416	5260	0.12%	0.017%
5	6.704	610	615	628	rVB	71554	123973	2.94%	0.392%
6	6.863	636	642	657	rBV	304674	513878	12.20%	1.624%
7	7.046	667	673	683	rBV	322237	530285	12.59%	1.676%
8	7.510	743	752	764	rBV	320856	517248	12.28%	1.634%
9	8.222	866	873	888	rBV	244750	400291	9.50%	1.265%
10	8.657	940	947	960	rBV	448731	748450	17.77%	2.365%
11	9.369	1061	1068	1083	rBV	386330	628520	14.92%	1.986%
12	9.898	1152	1158	1176	rBV	489041	887668	21.07%	2.805%
13	10.263	1213	1220	1232	rBV	474301	780765	18.53%	2.467%
14	10.422	1239	1247	1260	rBV	427128	799942	18.99%	2.528%
15	11.875	1488	1494	1504	rVB2	8055	15788	0.37%	0.050%
16	13.575	1777	1783	1794	rBV	1260306	1763012	41.85%	5.571%
17	13.839	1820	1828	1842	rBV	1417877	2039276	48.40%	6.444%
18	14.145	1873	1880	1892	rBV	808487	1203245	28.56%	3.802%
19	14.410	1919	1925	1934	rBV2	40074	103895	2.47%	0.328%
20	14.927	2009	2013	2017	rBV2	7750	9979	0.24%	0.032%
21	15.151	2043	2051	2060	rBV	1944380	2717948	64.51%	8.588%
22	15.298	2069	2076	2088	rBV	599757	890501	21.14%	2.814%
23	15.392	2088	2092	2098	rVB	21796	33331	0.79%	0.105%
24	15.933	2182	2184	2189	rVB5	3900	5432	0.13%	0.017%
25	16.692	2309	2313	2318	rVB3	3478	4898	0.12%	0.015%
26	16.904	2343	2349	2356	rBV	1089837	1499207	35.59%	4.737%
27	17.004	2359	2366	2382	rVV	2438797	3400102	80.71%	10.744%
28	17.821	2500	2505	2511	rBV7	12940	21123	0.50%	0.067%
29	17.892	2513	2517	2522	rVB	8503	12128	0.29%	0.038%
30	18.874	2679	2684	2688	rBV3	16369	23939	0.57%	0.076%
31	18.945	2692	2696	2701	rVV3	24472	32636	0.77%	0.103%
32	19.109	2720	2724	2729	rBV7	10852	18581	0.44%	0.059%
33	19.198	2735	2739	2744	rVB2	10181	13681	0.32%	0.043%
34	19.309	2752	2758	2767	rBV	3002212	4044768	96.01%	12.781%
35	21.109	3059	3064	3072	rBV	1395969	1778174	42.21%	5.619%
36	23.115	3398	3405	3420	rVB	2413176	4212981	100.00%	13.312%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031964.D
Acq On : 31 Aug 2021 00:05
Operator : CG/JU
Sample : M3422-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKD3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Title : SVOA CALIBRATION

37 23.250 3422 3428 3439 rVB2 985208 1747807 41.49% 5.523%




Sum of corrected areas: 31647188

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031964.D
Acq On : 31 Aug 2021 00:05
Operator : CG/JU
Sample : M3422-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKD3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

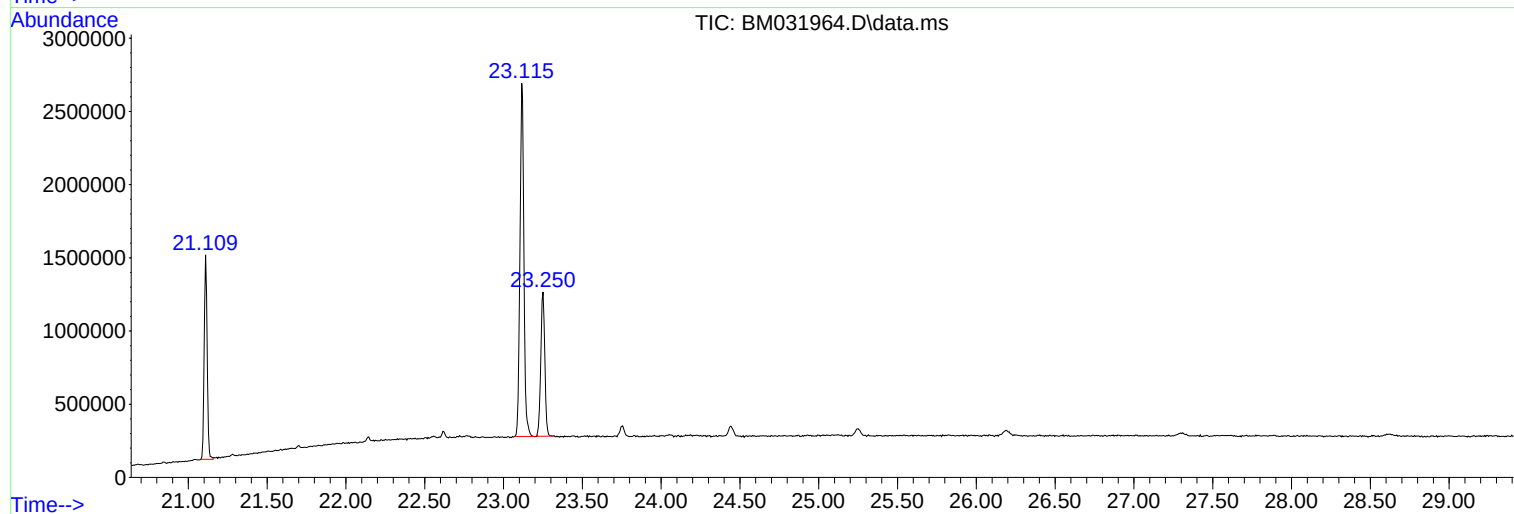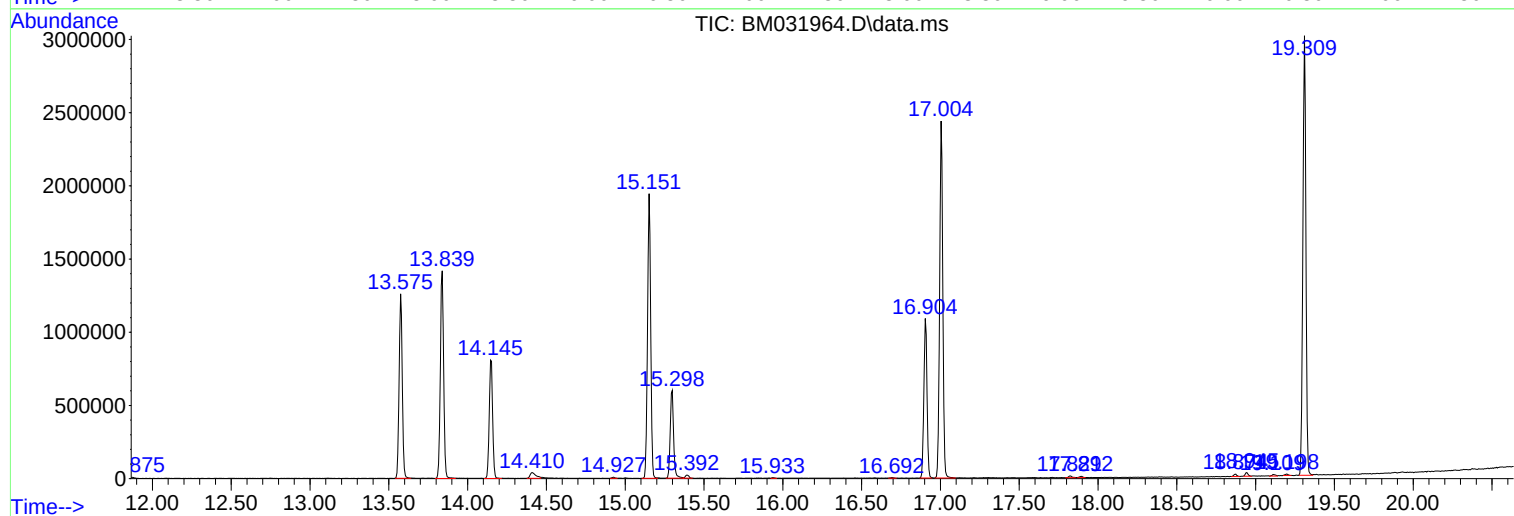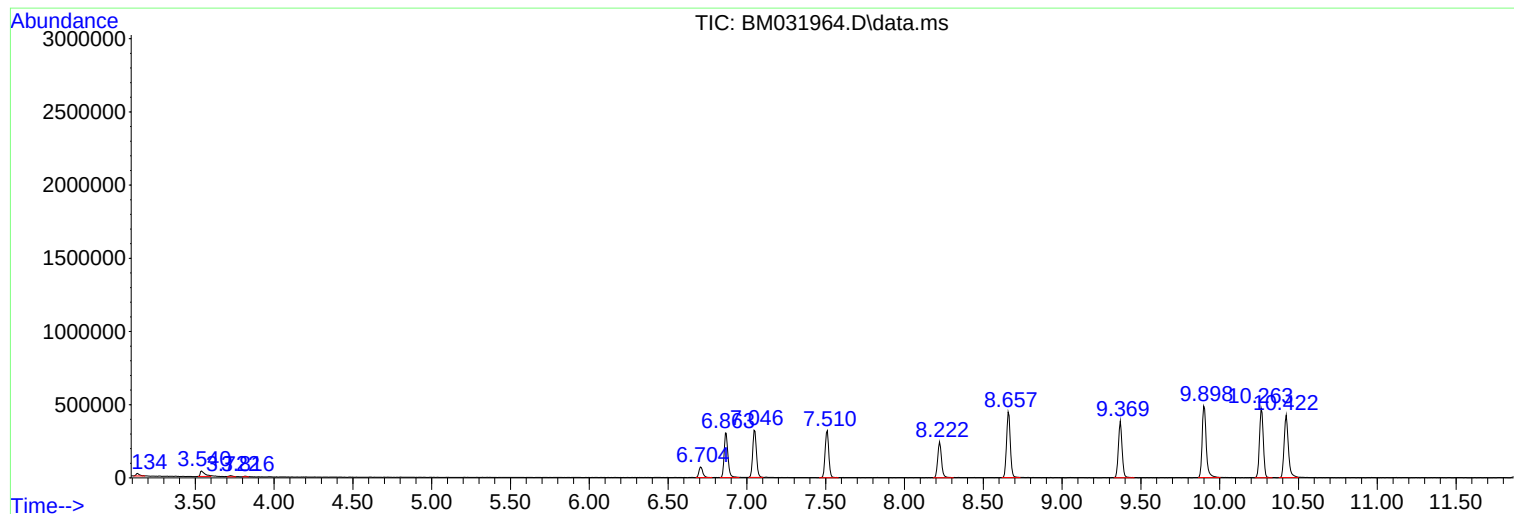

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031964.D
Acq On : 31 Aug 2021 00:05
Operator : CG/JU
Sample : M3422-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKD3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031964.D
Acq On : 31 Aug 2021 00:05
Operator : CG/JU
Sample : M3422-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBKD3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
