

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031975.D
 Acq On : 31 Aug 2021 08:11
 Operator : CG/JU
 Sample : PB138566BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK566

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	13	rBV	22055	27988	1.01%	0.099%
2	3.522	70	74	98	rBV	266865	498604	17.93%	1.758%
3	3.816	120	124	129	rVB3	7277	10344	0.37%	0.036%
4	6.698	607	614	626	rBV	450531	716071	25.75%	2.524%
5	6.863	636	642	652	rBV	297529	484185	17.41%	1.707%
6	7.045	666	673	681	rBV	446698	719275	25.87%	2.535%
7	7.504	744	751	760	rVB	348552	559063	20.11%	1.971%
8	8.216	866	872	888	rBV	572065	917910	33.01%	3.236%
9	8.657	937	947	959	rBV	415623	697607	25.09%	2.459%
10	9.363	1061	1067	1081	rBV	388667	627231	22.56%	2.211%
11	9.892	1150	1157	1178	rBV	550824	997987	35.89%	3.518%
12	10.263	1210	1220	1228	rBV	505386	835127	30.03%	2.944%
13	10.416	1239	1246	1262	rBV	518012	945876	34.02%	3.334%
14	11.869	1487	1493	1501	rVB	7691	13431	0.48%	0.047%
15	13.574	1776	1783	1792	rBV	1014977	1466533	52.74%	5.170%
16	13.833	1820	1827	1839	rBV	1180062	1753350	63.06%	6.181%
17	14.145	1872	1880	1889	rBV	846597	1220916	43.91%	4.304%
18	14.386	1914	1921	1943	rBV	346757	708711	25.49%	2.498%
19	15.151	2044	2051	2059	rBV	1508699	2201241	79.16%	7.759%
20	15.292	2069	2075	2088	rBV	412480	600089	21.58%	2.115%
21	15.392	2088	2092	2099	rVB2	22663	34698	1.25%	0.122%
22	15.939	2181	2185	2189	rVB2	3104	3999	0.14%	0.014%
23	16.692	2309	2313	2317	rBV3	4548	6020	0.22%	0.021%
24	16.904	2339	2349	2359	rBV	1075617	1512181	54.38%	5.330%
25	17.004	2359	2366	2377	rVV2	1716921	2437584	87.66%	8.593%
26	17.304	2414	2417	2420	rBV3	2277	3306	0.12%	0.012%
27	17.821	2501	2505	2509	rBV5	5360	7716	0.28%	0.027%
28	18.404	2600	2604	2606	rBV5	2291	2853	0.10%	0.010%
29	18.727	2656	2659	2661	rBV4	1998	2989	0.11%	0.011%
30	18.862	2679	2682	2691	rVB5	8807	13499	0.49%	0.048%
31	18.945	2691	2696	2700	rBV2	16787	24797	0.89%	0.087%
32	19.115	2721	2725	2727	rBV4	6961	8033	0.29%	0.028%
33	19.198	2735	2739	2741	rBV3	6453	7684	0.28%	0.027%
34	19.309	2751	2758	2768	rBV	2070034	2780663	100.00%	9.802%
35	21.109	3059	3064	3072	rBV	1287646	1628541	58.57%	5.741%
36	23.115	3399	3405	3416	rVB2	1339965	2464286	88.62%	8.687%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031975.D
Acq On : 31 Aug 2021 08:11
Operator : CG/JU
Sample : PB138566BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK566

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Title : SVOA CALIBRATION

37 23.250 3422 3428 3437 rVB2 798178 1428345 51.37% 5.035%




Sum of corrected areas: 28368733

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031975.D
Acq On : 31 Aug 2021 08:11
Operator : CG/JU
Sample : PB138566BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

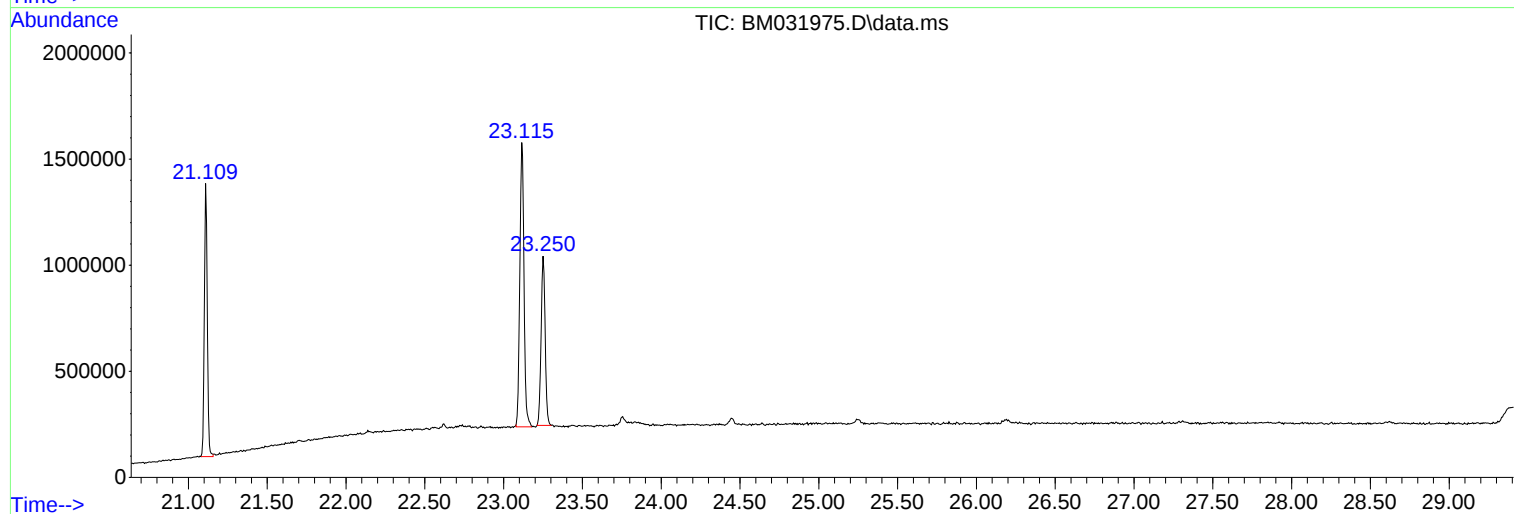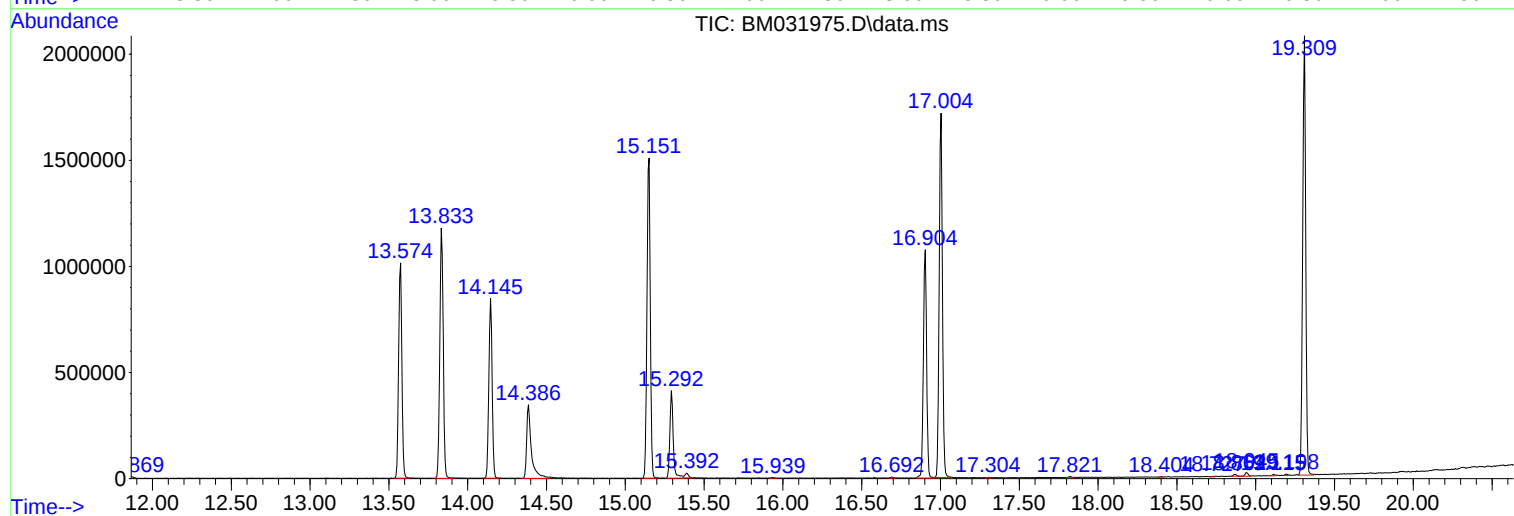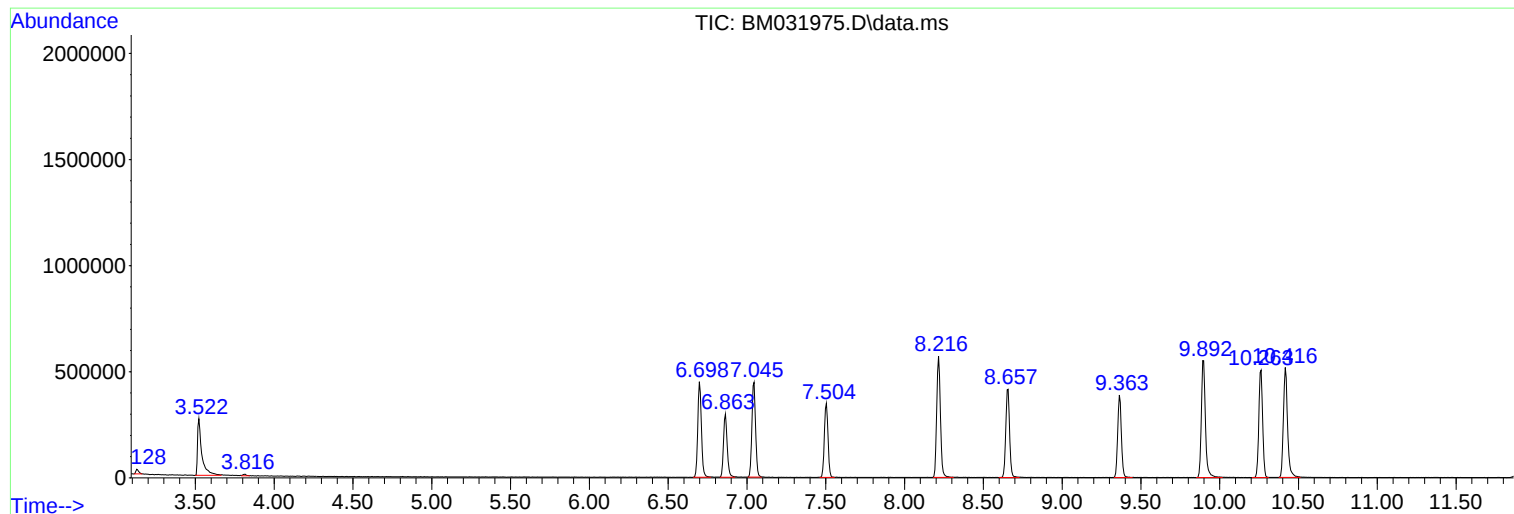

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031975.D
Acq On : 31 Aug 2021 08:11
Operator : CG/JU
Sample : PB138566BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031975.D
Acq On : 31 Aug 2021 08:11
Operator : CG/JU
Sample : PB138566BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
