

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031983.D
 Acq On : 31 Aug 2021 13:10
 Operator : CG/JU
 Sample : M3472-17
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	15	rVB	13885	20702	0.67%	0.083%
2	3.546	75	78	87	rBV2	19220	44481	1.45%	0.177%
3	3.722	105	108	115	rVB4	4681	7905	0.26%	0.032%
4	3.816	120	124	129	rVB6	5428	8011	0.26%	0.032%
5	6.704	609	615	622	rBV	87550	142634	4.64%	0.569%
6	6.863	636	642	655	rBV	284428	452089	14.71%	1.803%
7	7.046	666	673	683	rBV	310144	496298	16.14%	1.979%
8	7.504	745	751	760	rVB	299505	466973	15.19%	1.863%
9	8.216	866	872	887	rBV	258094	432360	14.06%	1.724%
10	8.657	940	947	957	rBV	398448	663648	21.59%	2.647%
11	9.369	1060	1068	1080	rBV	336272	563277	18.32%	2.247%
12	9.898	1151	1158	1173	rBV	478204	854021	27.78%	3.406%
13	10.263	1213	1220	1228	rBV	441192	714313	23.24%	2.849%
14	10.422	1240	1247	1260	rBV	199575	390411	12.70%	1.557%
15	11.869	1488	1493	1502	rVB3	7176	13062	0.42%	0.052%
16	13.574	1776	1783	1795	rBV	1061551	1479387	48.12%	5.901%
17	13.833	1820	1827	1839	rBV	1232199	1757297	57.16%	7.009%
18	14.145	1873	1880	1890	rBV	739005	1057839	34.41%	4.219%
19	14.404	1918	1924	1947	rBV3	37776	119217	3.88%	0.475%
20	15.151	2044	2051	2062	rBV	1586515	2270824	73.87%	9.057%
21	15.292	2069	2075	2086	rBV	369887	555747	18.08%	2.217%
22	15.386	2088	2091	2098	rVB4	12149	17943	0.58%	0.072%
23	15.492	2104	2109	2111	rBV2	1808	3079	0.10%	0.012%
24	16.692	2309	2313	2318	rVB4	3900	5990	0.19%	0.024%
25	16.904	2342	2349	2358	rBV	932521	1296833	42.18%	5.172%
26	17.004	2359	2366	2378	rVV	1920986	2691050	87.54%	10.733%
27	17.133	2384	2388	2393	rVB5	2158	3486	0.11%	0.014%
28	17.210	2395	2401	2407	rBV8	6441	12675	0.41%	0.051%
29	17.815	2500	2504	2509	rBV2	18107	23886	0.78%	0.095%
30	17.892	2513	2517	2521	rVB	7562	9602	0.31%	0.038%
31	18.868	2679	2683	2688	rBV3	16585	23806	0.77%	0.095%
32	18.939	2691	2695	2700	rVV	17885	22810	0.74%	0.091%
33	19.109	2721	2724	2729	rBV6	13934	18394	0.60%	0.073%
34	19.204	2733	2740	2742	rBV6	3887	7165	0.23%	0.029%
35	19.309	2751	2758	2766	rBV	2284519	3074169	100.00%	12.261%
36	21.109	3059	3064	3074	rBV	1133661	1432996	46.61%	5.716%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031983.D
Acq On : 31 Aug 2021 13:10
Operator : CG/JU
Sample : M3472-17
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AX6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Title : SVOA CALIBRATION

37	23.115	3399	3405	3418	rVB2	1508706	2678612	87.13%	10.684%
38	23.250	3422	3428	3438	rVB2	670553	1238952	40.30%	4.942%




Sum of corrected areas: 25071944

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031983.D
Acq On : 31 Aug 2021 13:10
Operator : CG/JU
Sample : M3472-17
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AX6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

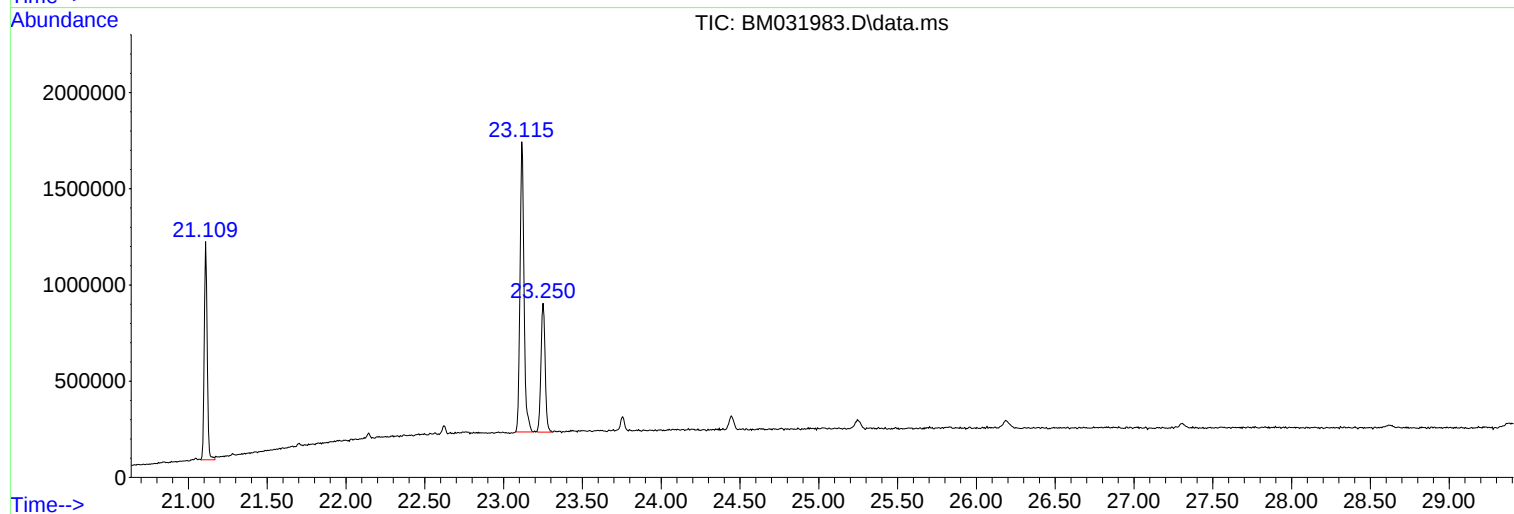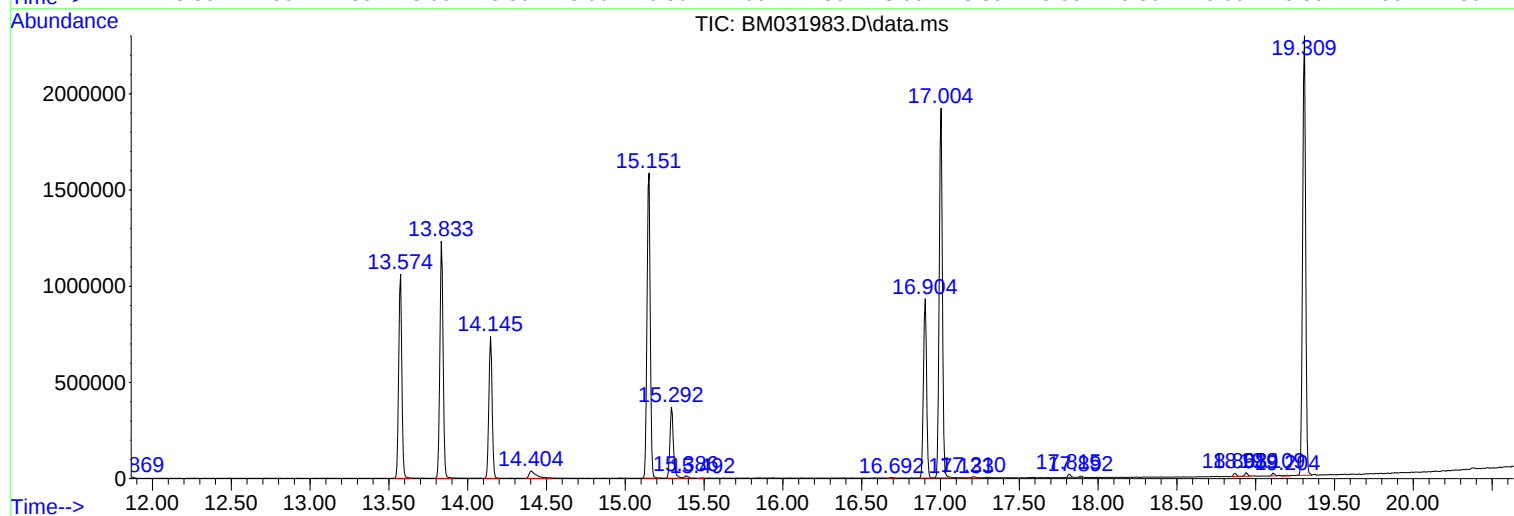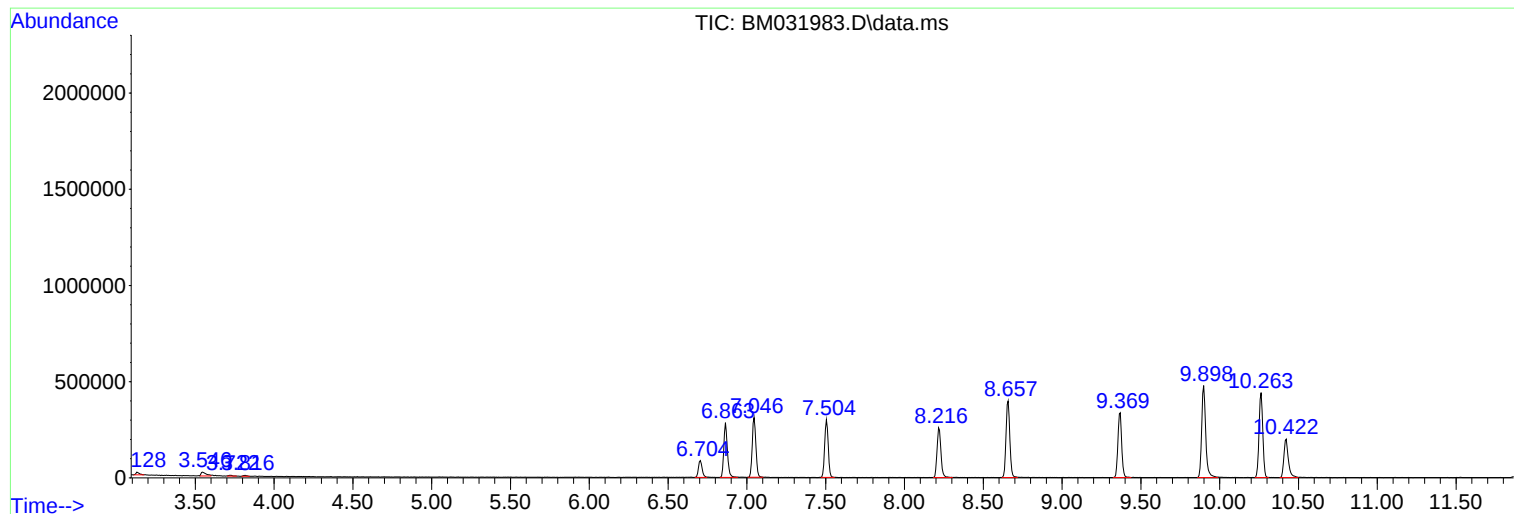

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031983.D
Acq On : 31 Aug 2021 13:10
Operator : CG/JU
Sample : M3472-17
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AX6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031983.D
Acq On : 31 Aug 2021 13:10
Operator : CG/JU
Sample : M3472-17
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AX6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
