

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM031989.D
 Acq On : 31 Aug 2021 17:47
 Operator : CG/JU
 Sample : PB138690BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK690

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM031989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	16	rVB	19558	27627	1.06%	0.106%
2	3.522	70	74	98	rBV	228913	435454	16.71%	1.677%
3	3.816	120	124	127	rVB3	5955	8247	0.32%	0.032%
4	6.698	608	614	629	rBV	377717	614892	23.60%	2.369%
5	6.863	636	642	654	rBV	259181	413358	15.86%	1.592%
6	7.046	666	673	683	rBV	387869	618265	23.73%	2.382%
7	7.504	745	751	762	rVB	314740	482773	18.53%	1.860%
8	8.216	865	872	887	rBV	496967	793411	30.45%	3.056%
9	8.657	939	947	960	rBV	373910	615661	23.63%	2.372%
10	9.363	1059	1067	1076	rBV	331761	549559	21.09%	2.117%
11	9.898	1149	1158	1176	rBV	491958	880558	33.80%	3.392%
12	10.263	1212	1220	1230	rBV	434666	743515	28.54%	2.864%
13	10.416	1238	1246	1264	rBV	463073	846782	32.50%	3.262%
14	11.875	1486	1494	1500	rBV	6225	11646	0.45%	0.045%
15	13.574	1776	1783	1793	rBV	953236	1334169	51.21%	5.140%
16	13.833	1820	1827	1837	rBV	1102909	1581301	60.69%	6.092%
17	14.145	1873	1880	1888	rBV	770858	1111169	42.65%	4.281%
18	14.386	1914	1921	1946	rBV	311789	654506	25.12%	2.521%
19	15.151	2044	2051	2059	rBV	1343649	2019144	77.50%	7.778%
20	15.292	2070	2075	2088	rBV	353378	517219	19.85%	1.992%
21	15.392	2088	2092	2099	rVB2	17265	24017	0.92%	0.093%
22	15.939	2181	2185	2188	rBV4	2848	3651	0.14%	0.014%
23	16.686	2307	2312	2315	rBV3	3624	5280	0.20%	0.020%
24	16.904	2343	2349	2357	rBV	982856	1365789	52.42%	5.261%
25	17.004	2359	2366	2378	rVV	1554441	2247957	86.28%	8.660%
26	17.827	2502	2506	2510	rBV5	2510	4761	0.18%	0.018%
27	18.874	2677	2684	2688	rBV4	9160	15617	0.60%	0.060%
28	18.939	2692	2695	2699	rBV	14853	20359	0.78%	0.078%
29	19.033	2706	2711	2714	rBV4	2991	5443	0.21%	0.021%
30	19.109	2723	2724	2728	rVB4	3275	3193	0.12%	0.012%
31	19.198	2735	2739	2741	rVB2	5601	6118	0.23%	0.024%
32	19.256	2747	2749	2751	rBV3	2975	2722	0.10%	0.010%
33	19.309	2751	2758	2768	rVV	1922694	2605492	100.00%	10.037%
34	21.109	3059	3064	3074	rBV	1154552	1509520	57.94%	5.815%
35	23.115	3398	3405	3415	rBV	1278083	2383979	91.50%	9.184%
36	23.250	3421	3428	3436	rVB2	723738	1325528	50.87%	5.106%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031989.D
Acq On : 31 Aug 2021 17:47
Operator : CG/JU
Sample : PB138690BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK690

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Title : SVOA CALIBRATION

37	23.750	3509	3513	3519	rVB2	99688	169938	6.52%	0.655%
----	--------	------	------	------	------	-------	--------	-------	--------


Sum of corrected areas: 25958620

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031989.D
Acq On : 31 Aug 2021 17:47
Operator : CG/JU
Sample : PB138690BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK690

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

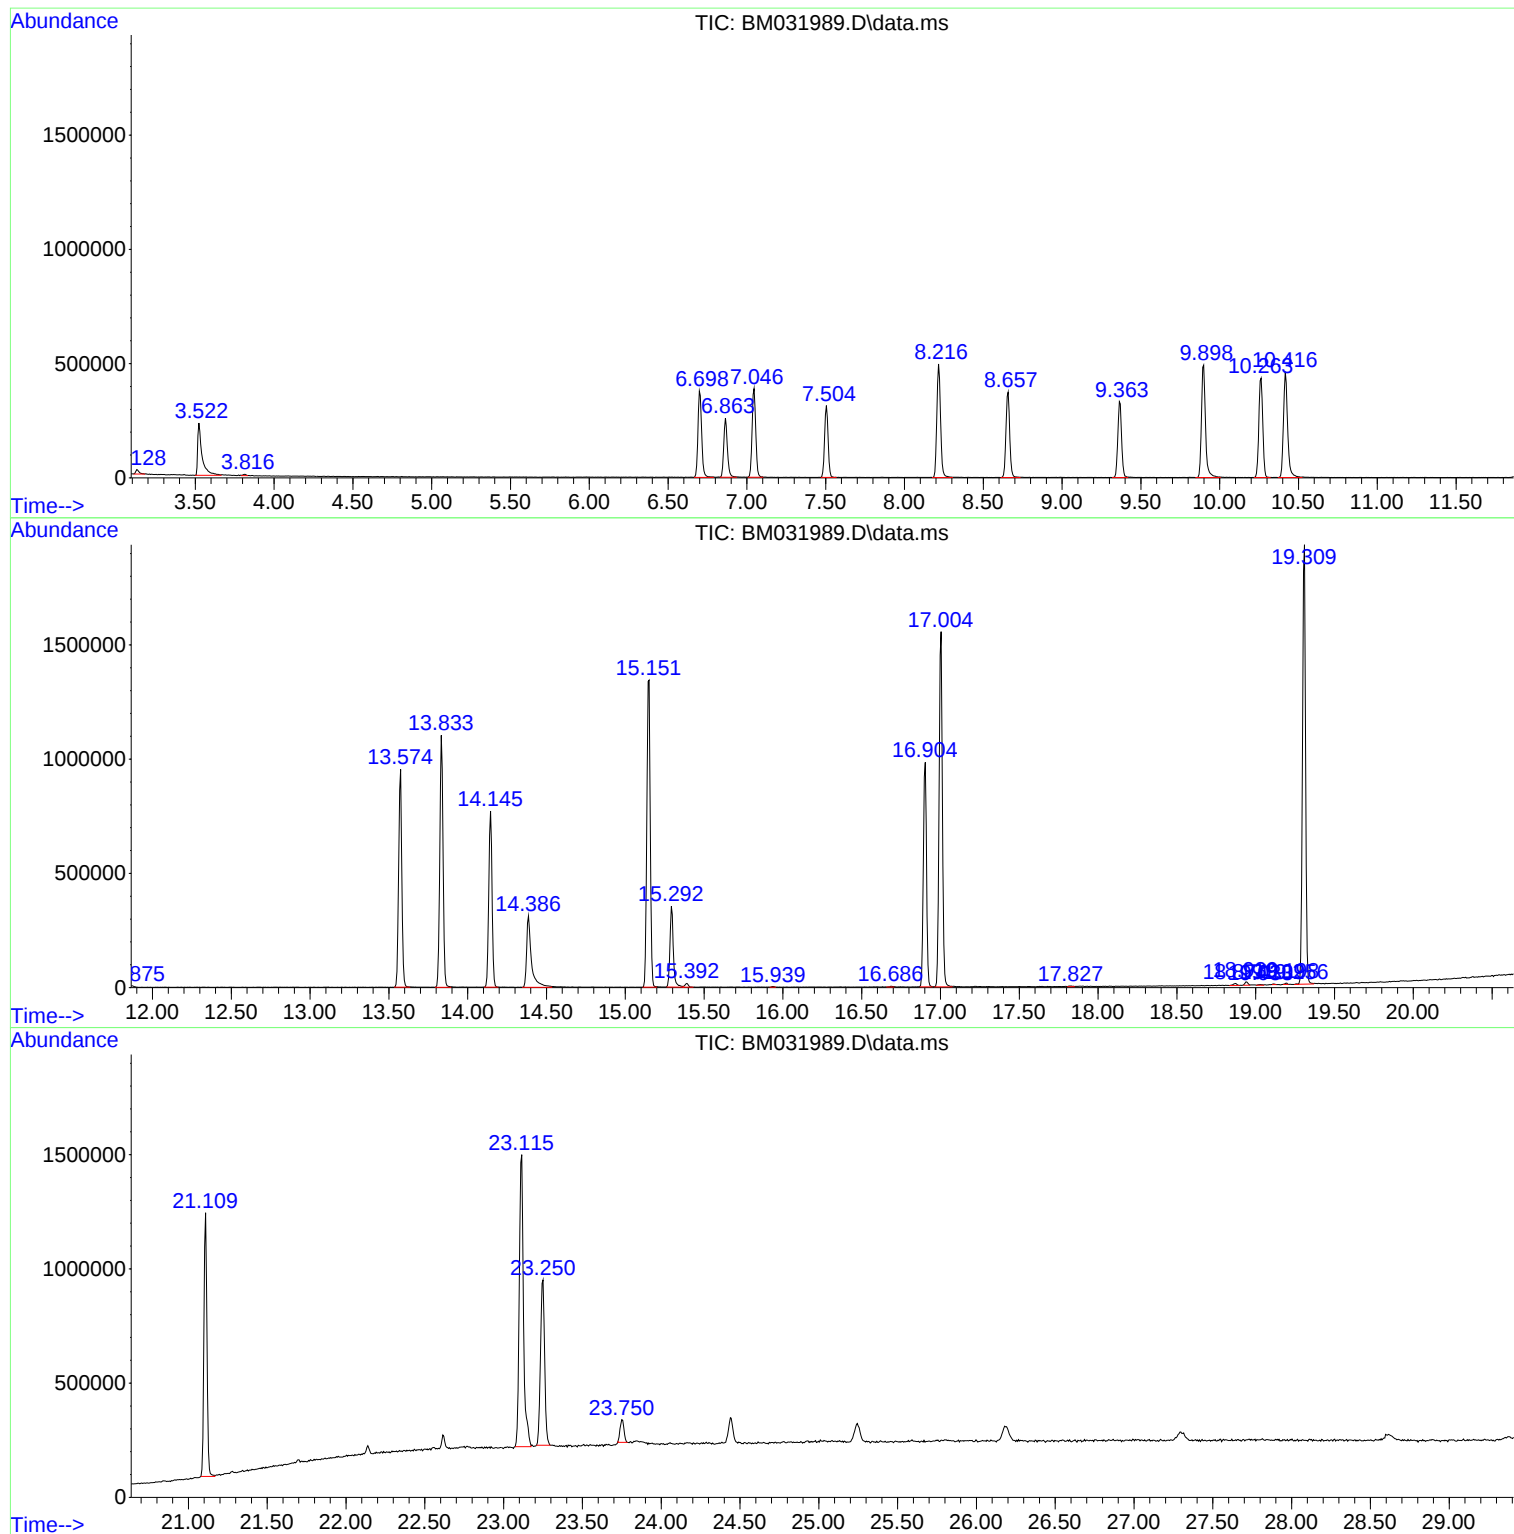

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031989.D
Acq On : 31 Aug 2021 17:47
Operator : CG/JU
Sample : PB138690BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK690










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.750	2.56 ng/ul	169938	Perylene-d12	23.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Decane, 3,8-dimethyl-	170	C12H26	017312-55-9	76
2			Hexacosane	366	C26H54	000630-01-3	76
3			Octacosane, 2-methyl-	408	C29H60	001560-98-1	76
4			Tetracosane	338	C24H50	000646-31-1	76
5			4-Methylheneicosane	310	C22H46	025117-29-7	68

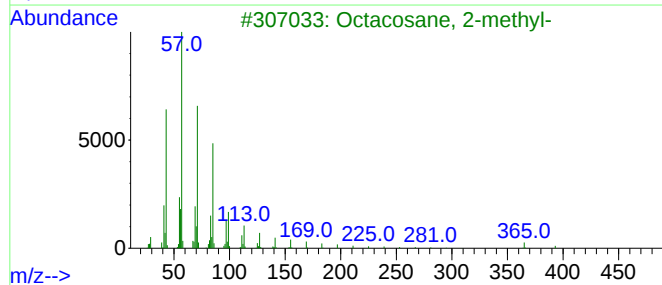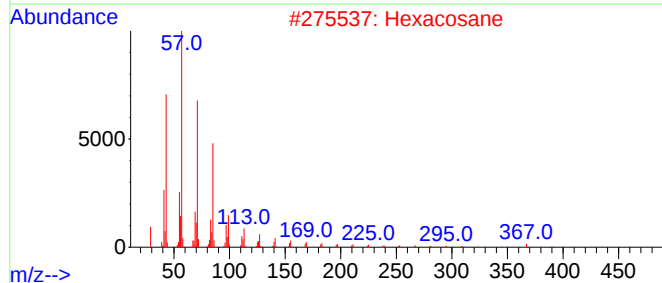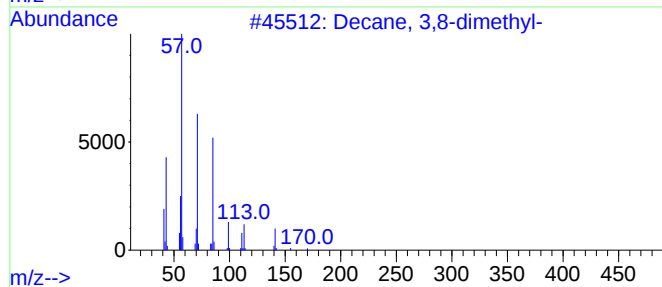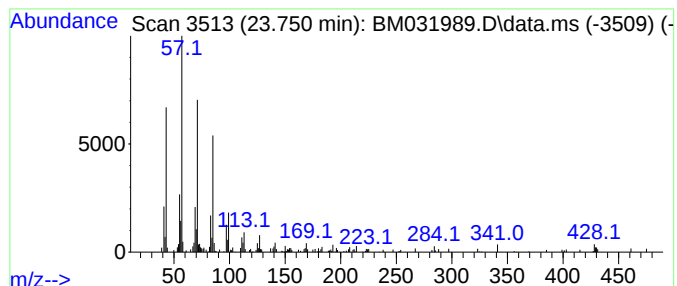

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM031989.D
Acq On : 31 Aug 2021 17:47
Operator : CG/JU
Sample : PB138690BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK690

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	23.750	2.6	ng/u1	169938	6	23.250	1325530	20.0