

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM032006.D
 Acq On : 01 Sep 2021 04:54
 Operator : CG/JU
 Sample : M3581-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.422	224	227	229	rVB3	1736	1969	0.18%	0.046%
2	4.504	238	241	243	rBV3	1957	1852	0.17%	0.043%
3	5.104	341	343	344	rBV2	1686	1166	0.11%	0.027%
4	5.292	372	375	379	rVB4	1606	1970	0.18%	0.046%
5	5.334	379	382	384	rVV3	991	1285	0.12%	0.030%
6	5.469	403	405	409	rVB3	1392	1509	0.14%	0.035%
7	5.557	418	420	425	rVB5	1476	1126	0.10%	0.026%
8	5.845	465	469	472	rBV3	1632	1379	0.13%	0.032%
9	5.892	475	477	479	rVB3	1399	1156	0.11%	0.027%
10	6.028	497	500	503	rBV4	1028	1614	0.15%	0.037%
11	6.292	541	545	548	rVB4	1278	1401	0.13%	0.032%
12	6.687	610	612	615	rBV3	1142	1257	0.12%	0.029%
13	6.875	639	644	649	rBV5	1348	3324	0.31%	0.077%
14	7.192	697	698	702	rVB3	1201	1205	0.11%	0.028%
15	7.504	745	751	762	rBV	149654	253587	23.31%	5.879%
16	7.716	784	787	792	rVB4	901	1388	0.13%	0.032%
17	7.839	805	808	811	rBV4	953	1134	0.10%	0.026%
18	8.769	963	966	971	rBV4	775	1400	0.13%	0.032%
19	8.916	989	991	996	rVB2	1036	1438	0.13%	0.033%
20	8.969	996	1000	1001	rBV	1506	1440	0.13%	0.033%
21	9.292	1050	1055	1057	rBV3	874	1270	0.12%	0.029%
22	9.539	1092	1097	1100	rBV4	647	1365	0.13%	0.032%
23	9.886	1153	1156	1159	rBV3	842	1348	0.12%	0.031%
24	10.263	1212	1220	1231	rBV	203043	386266	35.50%	8.956%
25	11.098	1357	1362	1365	rBV3	1014	1894	0.17%	0.044%
26	11.227	1381	1384	1389	rVV3	855	1523	0.14%	0.035%
27	12.010	1511	1517	1519	rBV3	889	1286	0.12%	0.030%
28	12.216	1549	1552	1555	rVB3	802	1094	0.10%	0.025%
29	12.410	1581	1585	1587	rBV2	864	1146	0.11%	0.027%
30	12.792	1645	1650	1654	rVB3	672	1294	0.12%	0.030%
31	14.145	1872	1880	1897	rBV	377900	617893	56.79%	14.326%
32	14.257	1897	1899	1904	rBV5	1037	1346	0.12%	0.031%
33	14.733	1977	1980	1982	rBV	944	1185	0.11%	0.027%
34	15.680	2138	2141	2146	rBV3	844	1243	0.11%	0.029%
35	16.298	2243	2246	2249	rVB3	1525	2148	0.20%	0.050%
36	16.327	2249	2251	2253	rBV2	1388	1503	0.14%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
 Data File : BM032006.D
 Acq On : 01 Sep 2021 04:54
 Operator : CG/JU
 Sample : M3581-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Title : SVOA CALIBRATION

37	16.480	2274	2277	2280	rBV3	897	1152	0.11%	0.027%
38	16.615	2296	2300	2305	rVB4	1132	2167	0.20%	0.050%
39	16.698	2311	2314	2316	rVB5	1501	1816	0.17%	0.042%
40	16.903	2342	2349	2368	rBV	465568	797580	73.30%	18.492%
41	17.021	2368	2369	2373	rVB3	1688	1524	0.14%	0.035%
42	17.198	2396	2399	2401	rVB4	1293	1211	0.11%	0.028%
43	17.333	2419	2422	2424	rBV2	1076	1211	0.11%	0.028%
44	17.380	2427	2430	2432	rBV3	959	1136	0.10%	0.026%
45	17.462	2441	2444	2449	rBV5	1242	1990	0.18%	0.046%
46	17.509	2449	2452	2454	rVV4	919	1145	0.11%	0.027%
47	17.745	2490	2492	2495	rVB3	2366	2158	0.20%	0.050%
48	17.921	2521	2522	2526	rVB3	1513	1170	0.11%	0.027%
49	17.950	2526	2527	2531	rVB2	1269	1480	0.14%	0.034%
50	18.003	2531	2536	2537	rBV4	2426	2588	0.24%	0.060%
51	18.198	2567	2569	2572	rBV3	1186	1616	0.15%	0.037%
52	18.221	2572	2573	2577	rVV4	1518	1227	0.11%	0.028%
53	18.321	2589	2590	2593	rVB2	1285	1236	0.11%	0.029%
54	18.398	2601	2603	2608	rBV4	857	1290	0.12%	0.030%
55	18.697	2651	2654	2656	rBV4	1537	1969	0.18%	0.046%
56	18.762	2662	2665	2667	rBV4	1563	1864	0.17%	0.043%
57	18.839	2677	2678	2683	rBV4	1639	2393	0.22%	0.055%
58	19.139	2727	2729	2731	rBV3	1828	1646	0.15%	0.038%
59	19.292	2753	2755	2757	rBV2	3328	2288	0.21%	0.053%
60	19.568	2800	2802	2805	rBV4	3042	3697	0.34%	0.086%
61	21.109	3058	3064	3074	rBV	789832	1081117	99.36%	25.066%
62	23.244	3421	3427	3439	rVB	602312	1088084	100.00%	25.227%




Sum of corrected areas: 4313159

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032006.D
Acq On : 01 Sep 2021 04:54
Operator : CG/JU
Sample : M3581-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

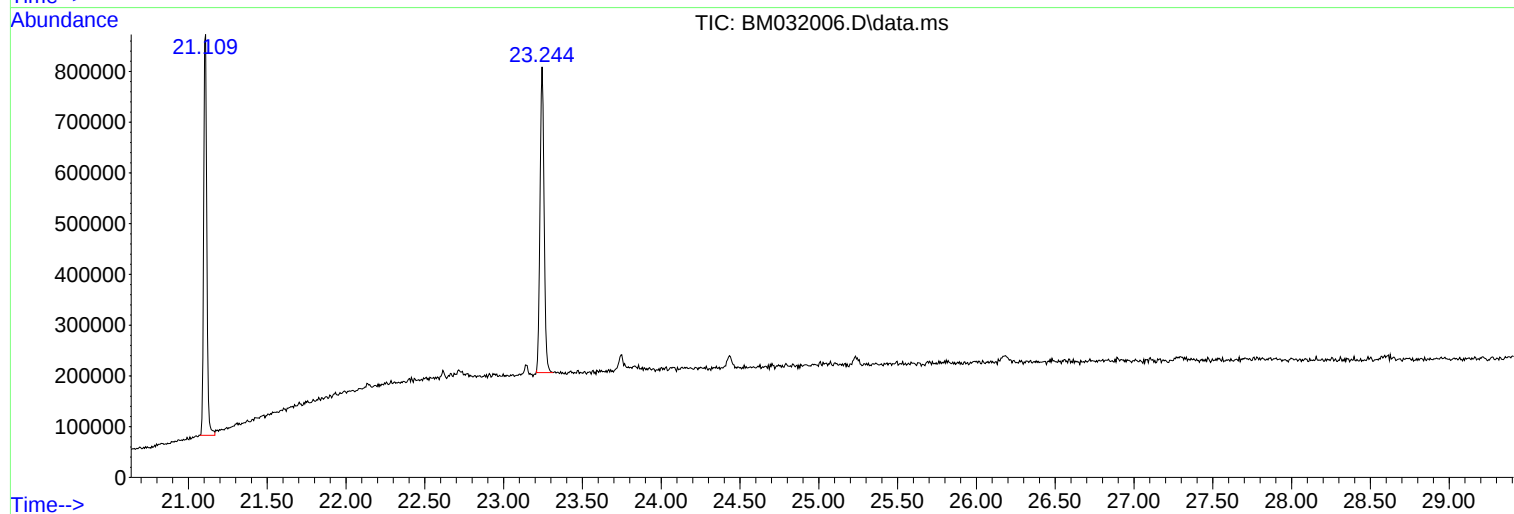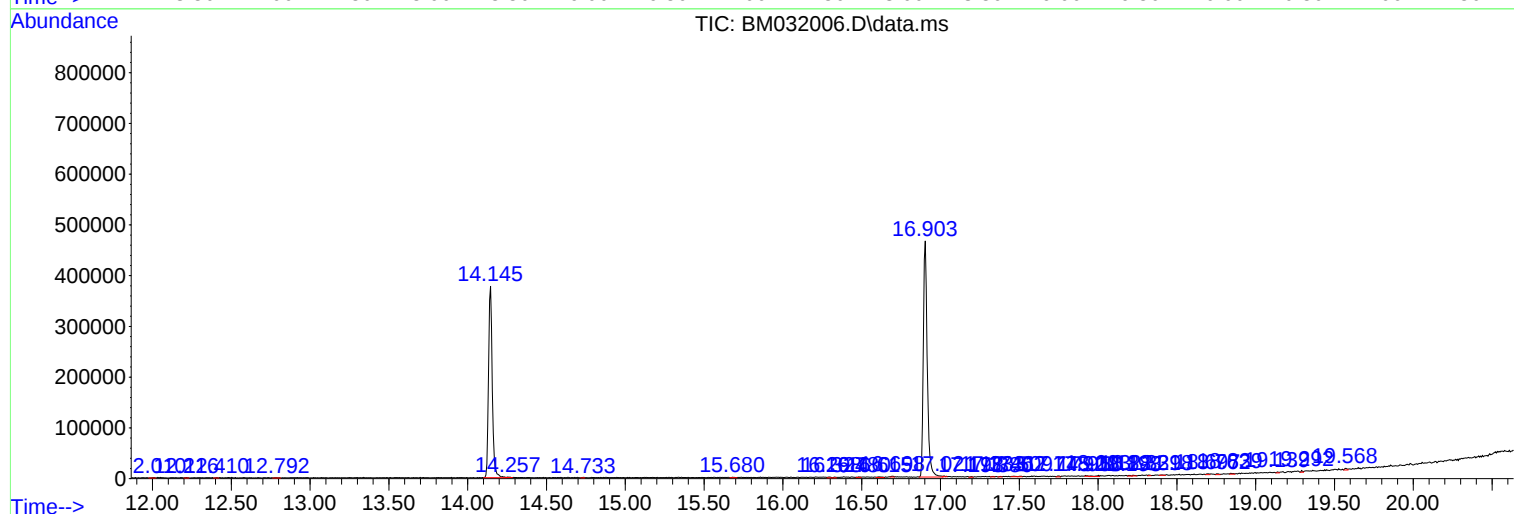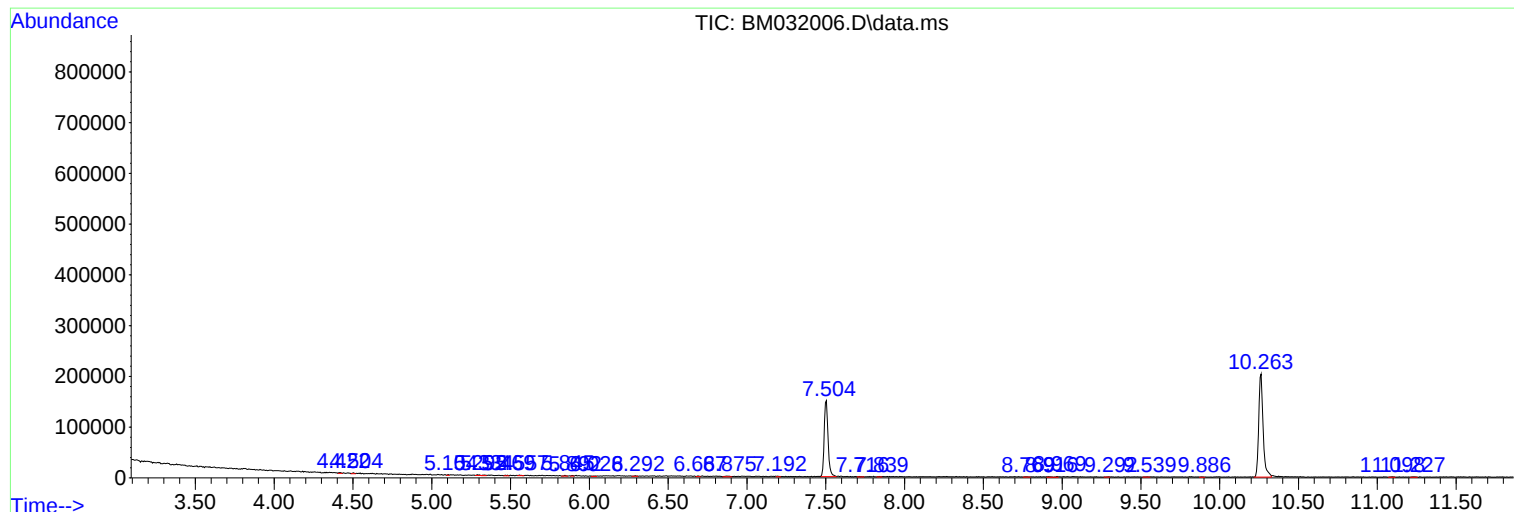

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032006.D
Acq On : 01 Sep 2021 04:54
Operator : CG/JU
Sample : M3581-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032006.D
Acq On : 01 Sep 2021 04:54
Operator : CG/JU
Sample : M3581-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
