

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
 Data File : BM047405.D
 Acq On : 30 Aug 2024 14:21
 Operator : RC/JU
 Sample : P3751-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-CMC-ESLAG-1

Quant Time: Aug 30 14:57:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 26 18:11:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.346	152	241169	20.000	ng	0.00
21) Naphthalene-d8	10.098	136	861937	20.000	ng	0.00
39) Acenaphthene-d10	14.004	164	569536	20.000	ng	0.00
64) Phenanthrene-d10	16.774	188	1188579	20.000	ng	0.00
76) Chrysene-d12	21.021	240	975990	20.000	ng	0.00
86) Perylene-d12	23.721	264	987006	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.010	112	1494673	118.905	ng	0.00
7) Phenol-d6	6.569	99	1851239	108.107	ng	0.00
23) Nitrobenzene-d5	8.493	82	1424468	91.698	ng	0.00
42) 2,4,6-Tribromophenol	15.522	330	1060015	154.266	ng	0.00
45) 2-Fluorobiphenyl	12.610	172	3281415	88.526	ng	0.00
79) Terphenyl-d14	19.445	244	5499345	100.294	ng	0.00
Target Compounds						
						Qvalue
50) Dimethylphthalate	13.486	163	83776	2.135	ng	98
70) Pentachlorophenol	16.457	266	26368	2.816	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047405.D
Acq On : 30 Aug 2024 14:21
Operator : RC/JU
Sample : P3751-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-CMC-ESLAG-1

Quant Time: Aug 30 14:57:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

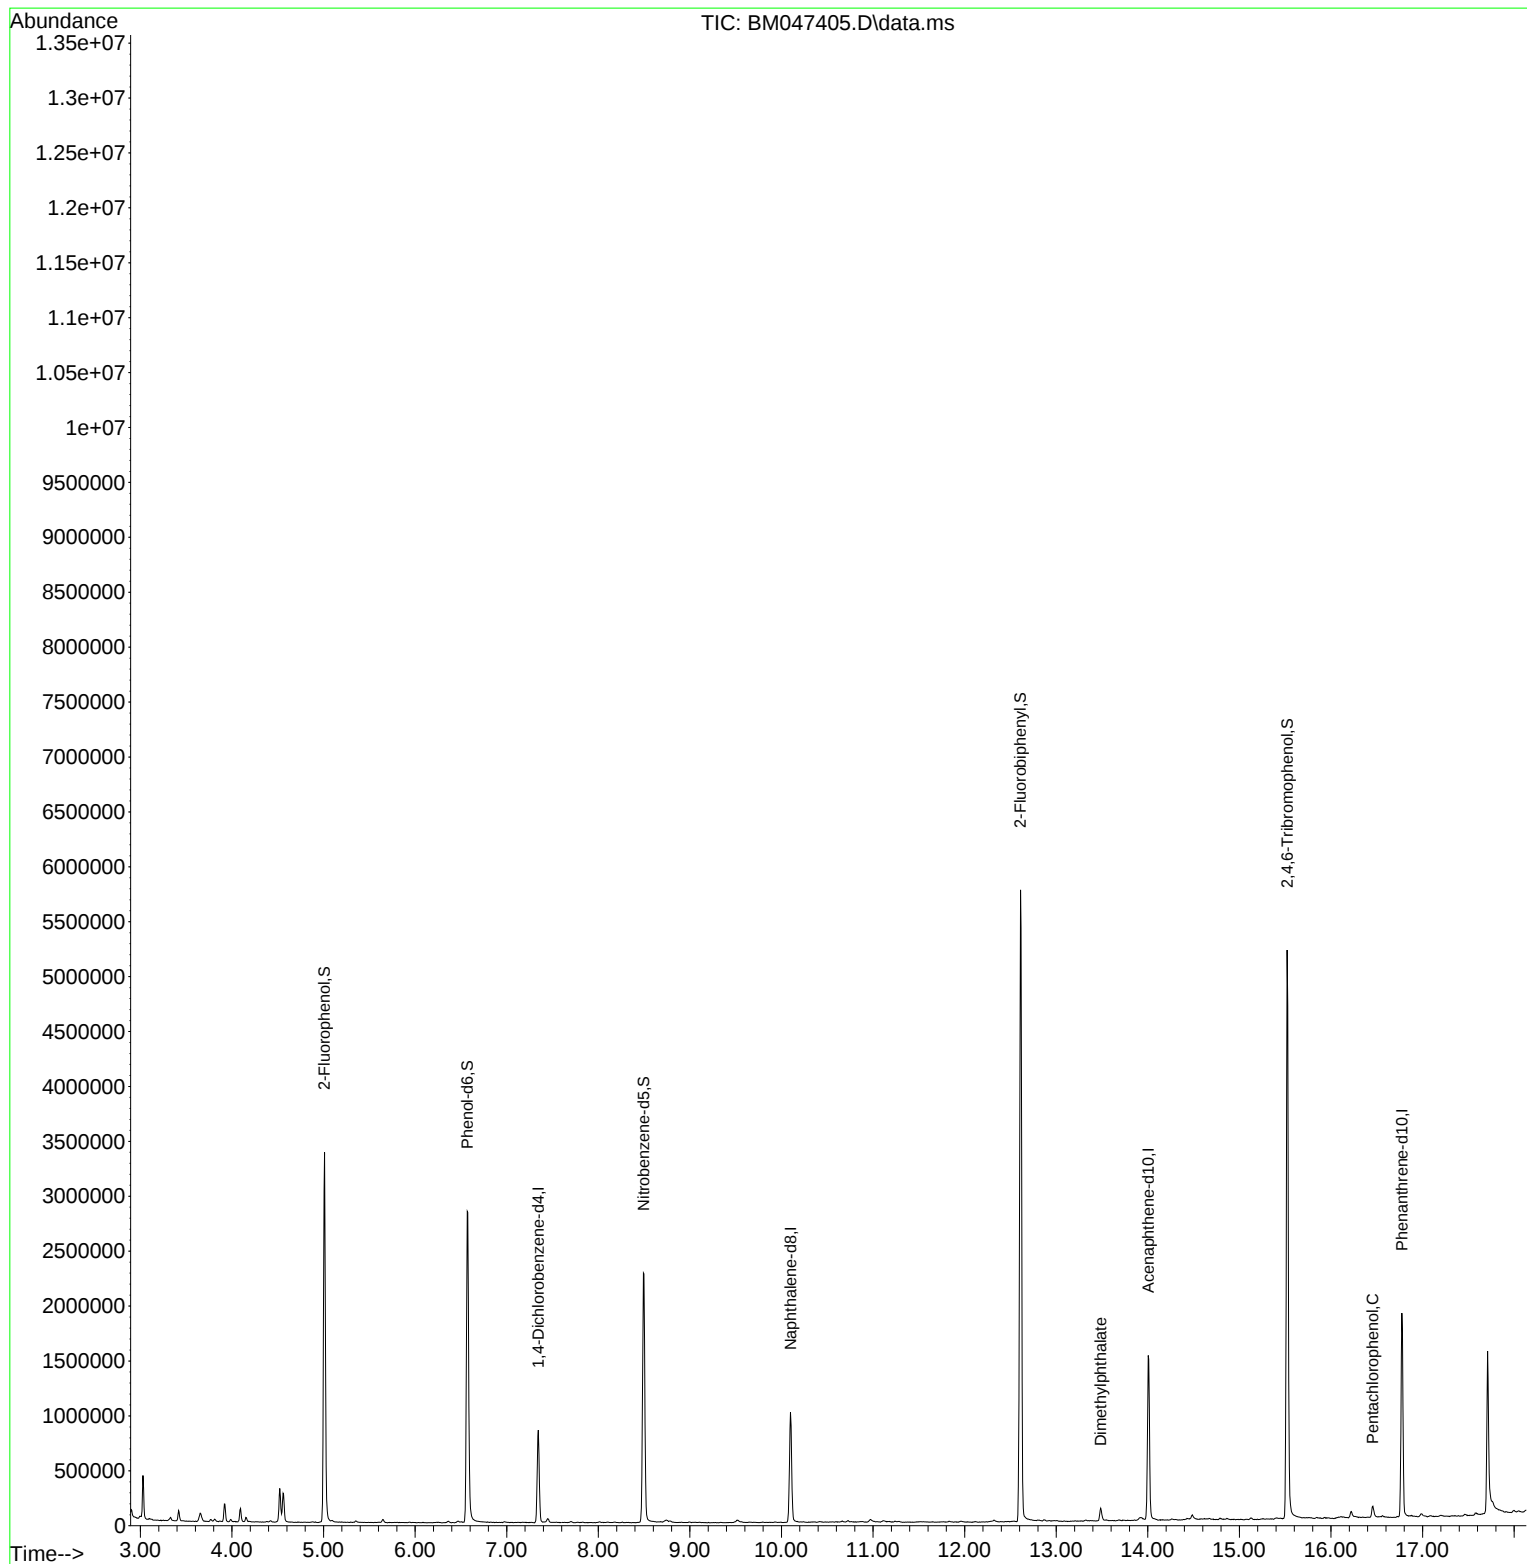

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047405.D
Acq On : 30 Aug 2024 14:21
Operator : RC/JU
Sample : P3751-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-CMC-ESLAG-1

Quant Time: Aug 30 14:57:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

