
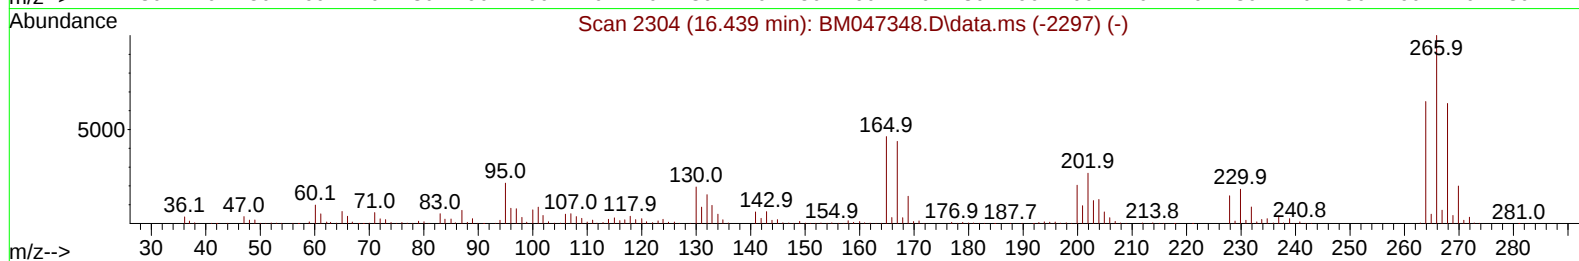
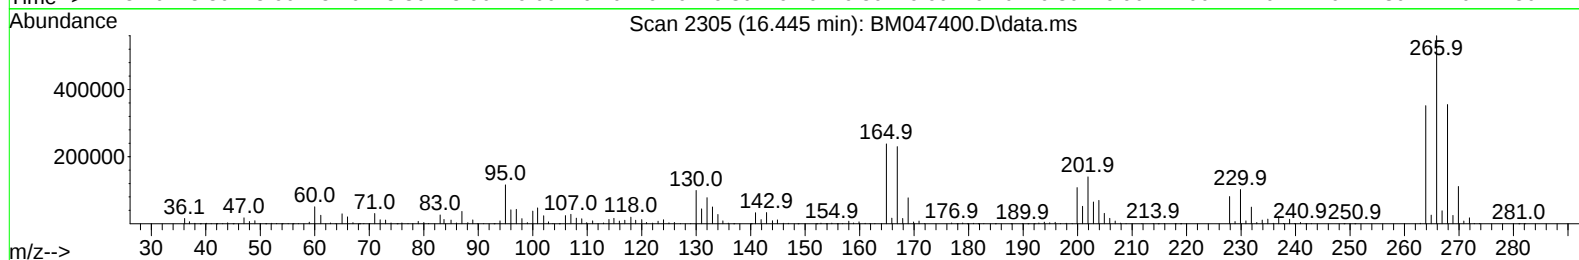


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM083024\  
Data File : BM047400.D  
Acq On : 30 Aug 2024 10:48  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 11:41:44 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM082624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 26 18:11:40 2024  
Response via : Initial Calibration

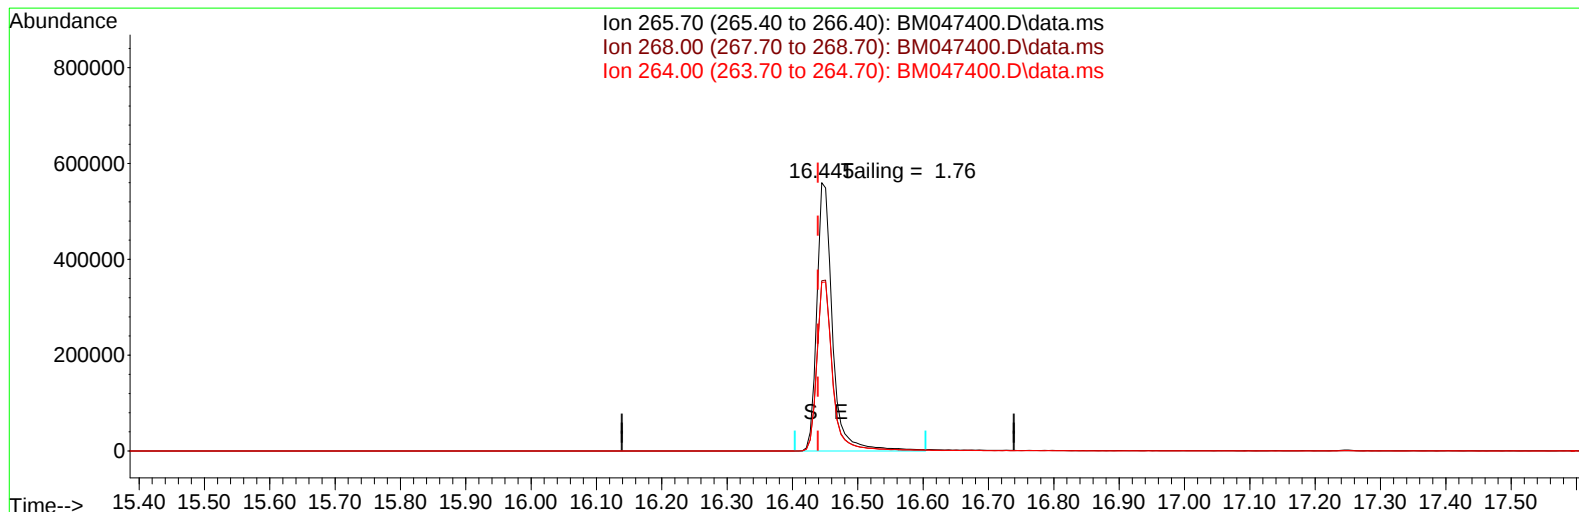

TIC: BM047400.D\data.ms

**(70) Pentachlorophenol (C)**




**16.445min (+ 0.006) 233397.58 ng**

**response 934029**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.42  |
| 264.00 | 64.90  | 62.82  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM083024\  
Data File : BM047400.D  
Acq On : 30 Aug 2024 10:48  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 11:41:44 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM082624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 26 18:11:40 2024  
Response via : Initial Calibration

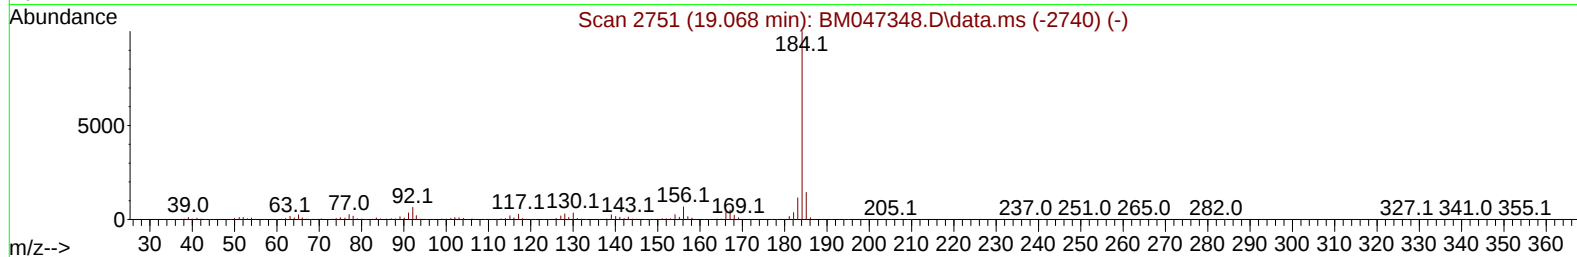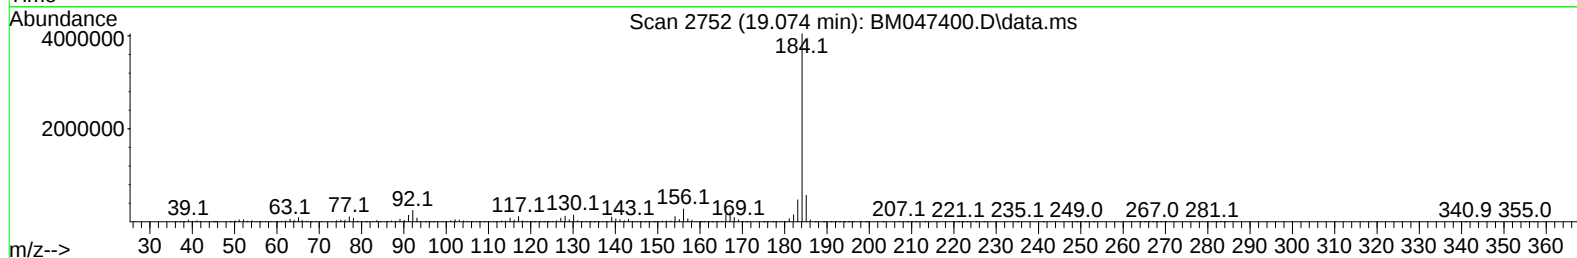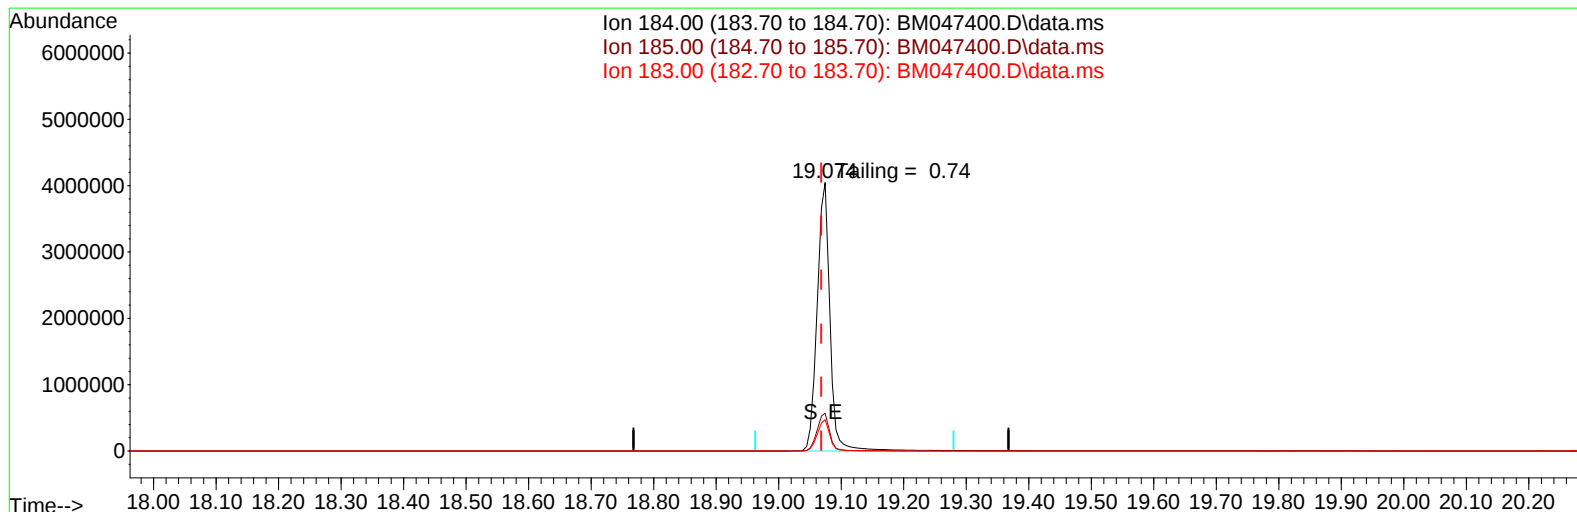

TIC: BM047400.D\data.ms

**(77) Benzidine****19.074min (+ 0.006) 86573.98 ng****response 5776142**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.06  |
| 183.00 | 11.50  | 11.70  |
| 0.00   | 0.00   | 0.00   |