

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
 Data File : BM047410.D
 Acq On : 30 Aug 2024 17:39
 Operator : RC/JU
 Sample : P3800-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RBR20046

Quant Time: Aug 30 23:29:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 26 18:11:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.345	152	342605	20.000	ng	0.00
21) Naphthalene-d8	10.098	136	1215652	20.000	ng	0.00
39) Acenaphthene-d10	14.016	164	596231	20.000	ng	0.00
64) Phenanthrene-d10	16.845	188	633330	20.000	ng	# 0.07
76) Chrysene-d12	21.050	240	1001003	20.000	ng	0.03
86) Perylene-d12	23.733	264	1281328	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.016	112	95324	5.338	ng	0.01
7) Phenol-d6	6.569	99	632049	25.982	ng	0.00
23) Nitrobenzene-d5	8.492	82	1172304	53.507	ng	0.00
42) 2,4,6-Tribromophenol	15.563	330	2132	0.296	ng	0.04
45) 2-Fluorobiphenyl	12.610	172	2575113	66.361	ng	0.00
79) Terphenyl-d14	19.492	244	2199911	39.118	ng	0.05
Target Compounds						
71) Phenanthrene	16.892	178	609077	19.803	ng	# 1
74) Di-n-butylphthalate	17.809	149	451145	12.877	ng	# 30

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047410.D
Acq On : 30 Aug 2024 17:39
Operator : RC/JU
Sample : P3800-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBR20046


Quant Time: Aug 30 23:29:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

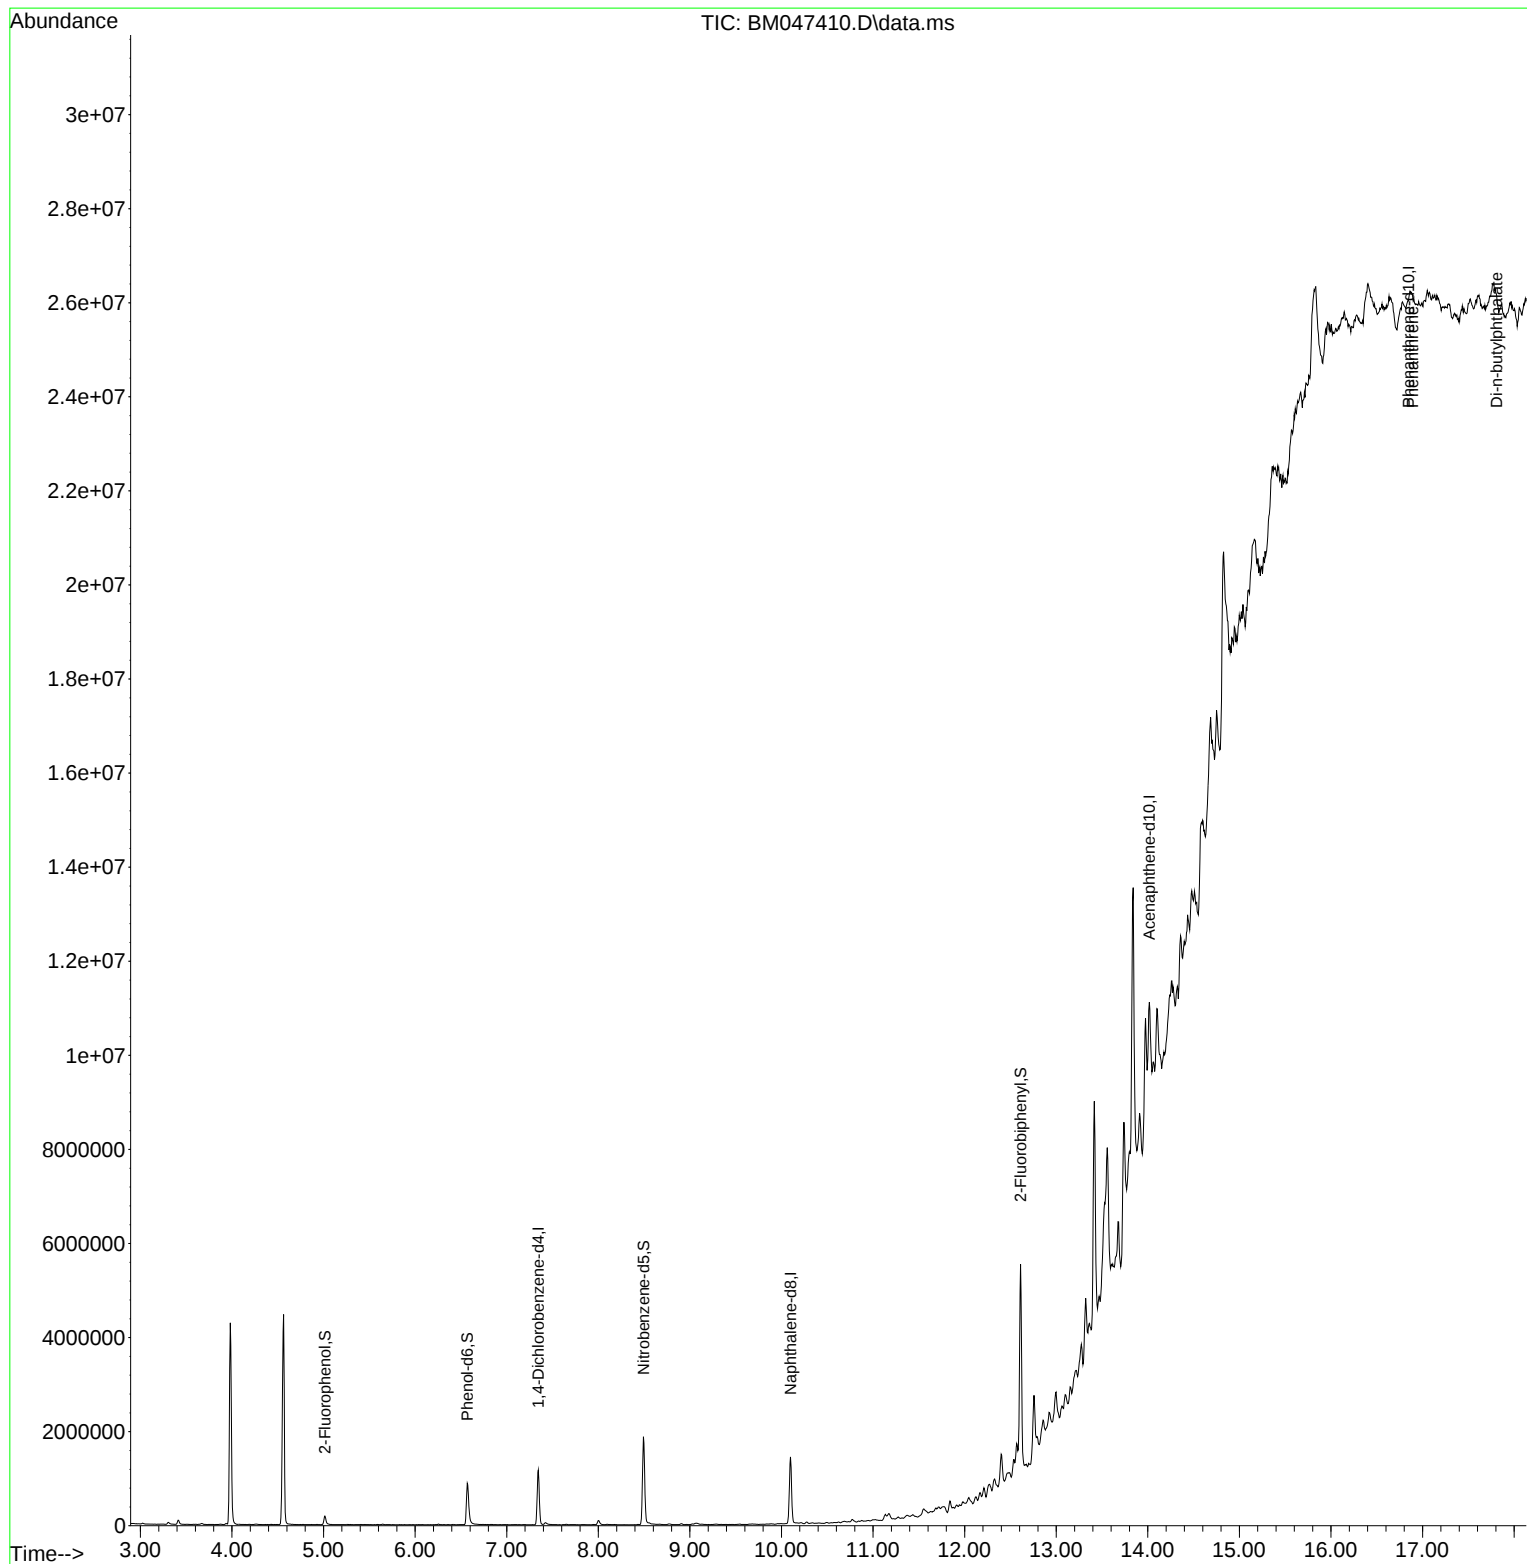


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047410.D
Acq On : 30 Aug 2024 17:39
Operator : RC/JU
Sample : P3800-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBR20046

Quant Time: Aug 30 23:29:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration




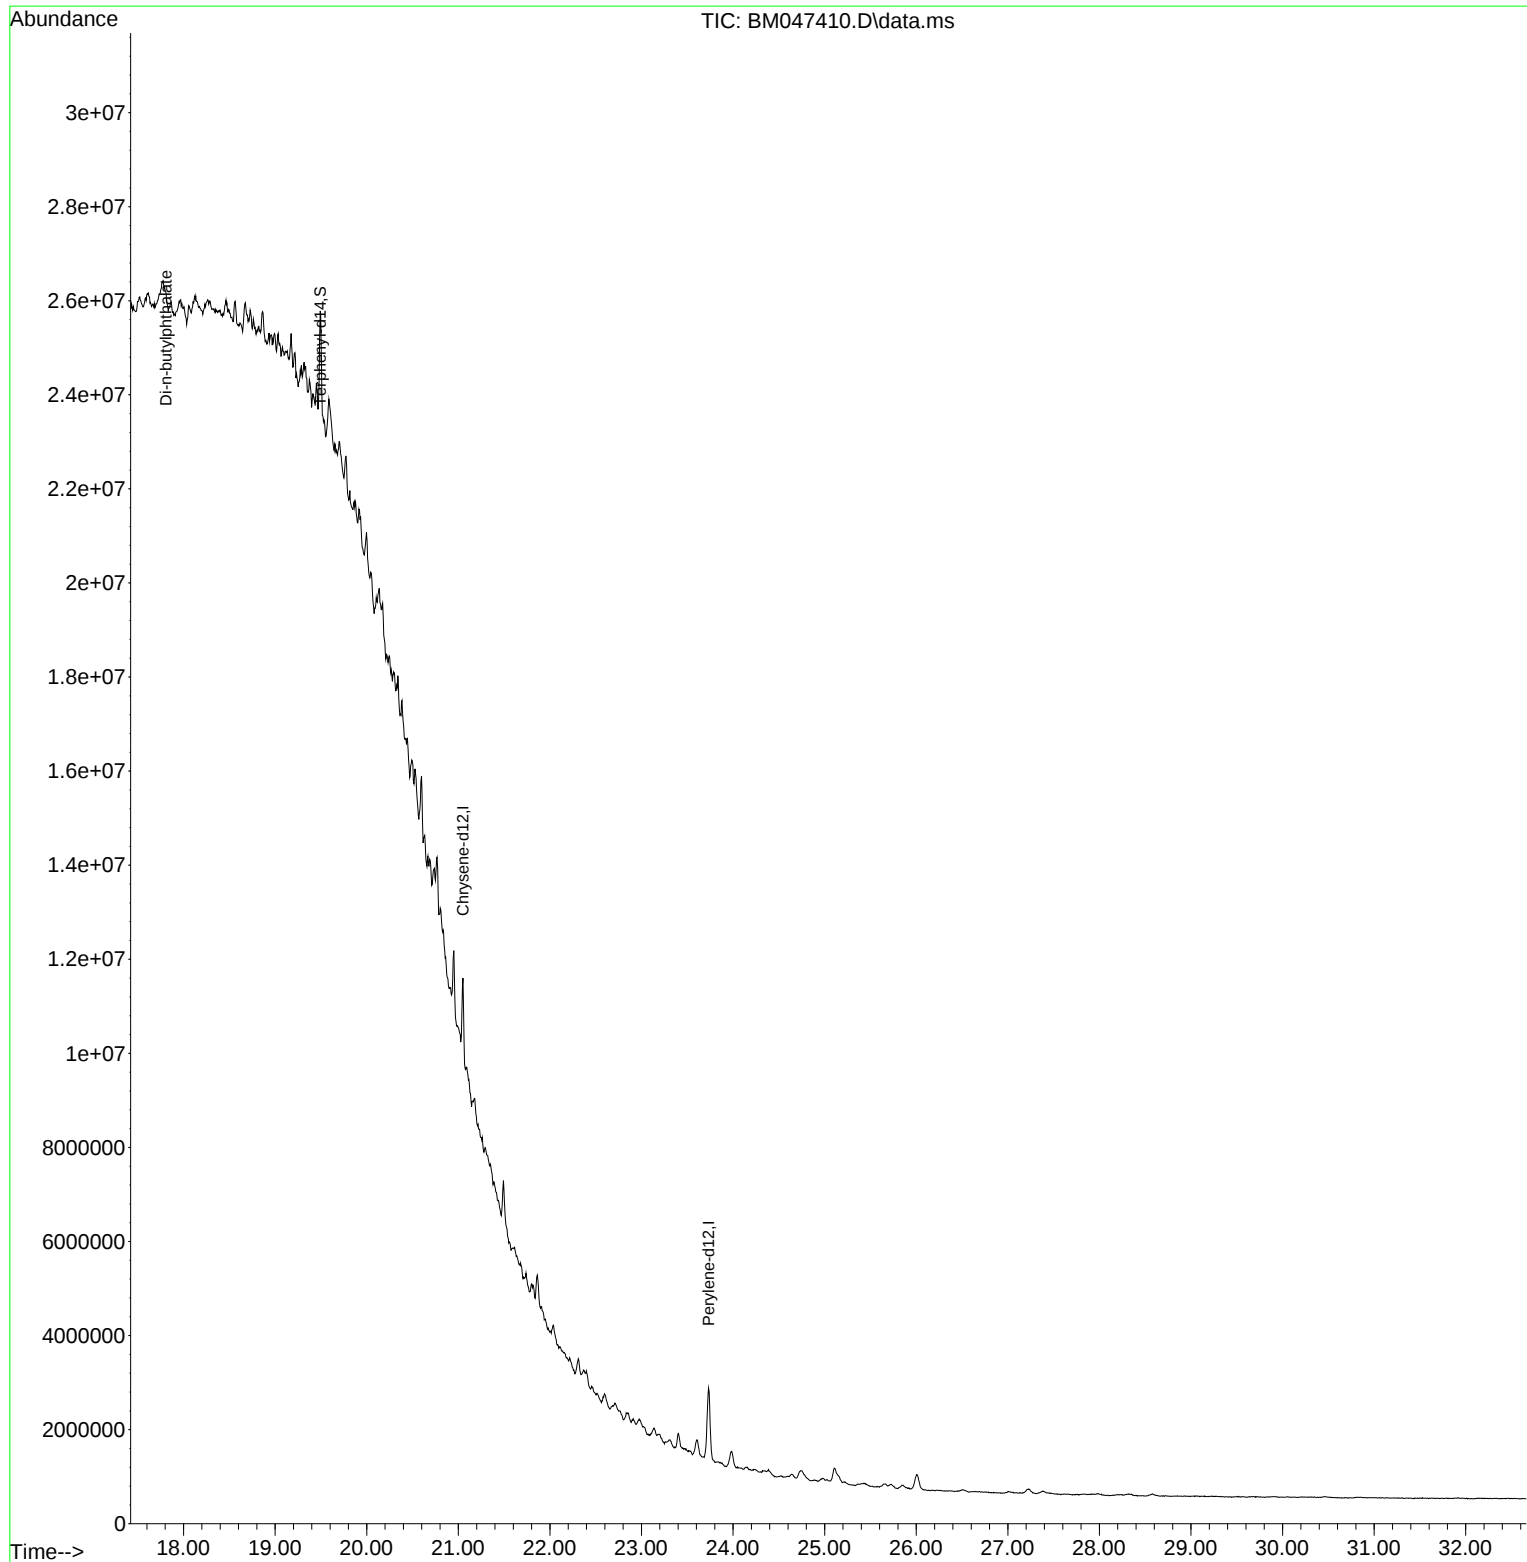


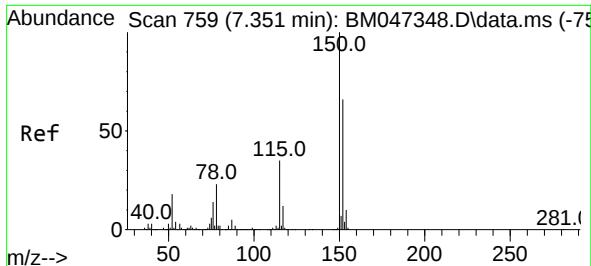

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.345 min Scan# 71
Delta R.T. -0.006 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39




Instrument :
BNA_M
ClientSampleId :
RBR20046


Tgt Ion:152 Resp: 342605
Ion Ratio Lower Upper
152 100
150 157.6 121.3 181.9
115 54.1 42.6 64.0

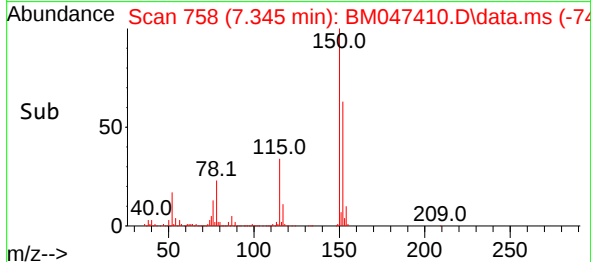

#5
2-Fluorophenol
Concen: 5.338 ng
RT: 5.016 min Scan# 362
Delta R.T. 0.012 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39

Tgt Ion:112 Resp: 95324
Ion Ratio Lower Upper
112 100
64 55.0 45.7 68.5
63 28.7 23.8 35.8


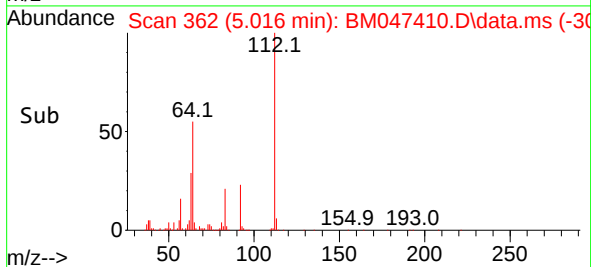

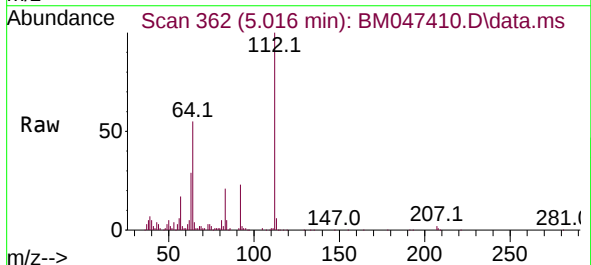


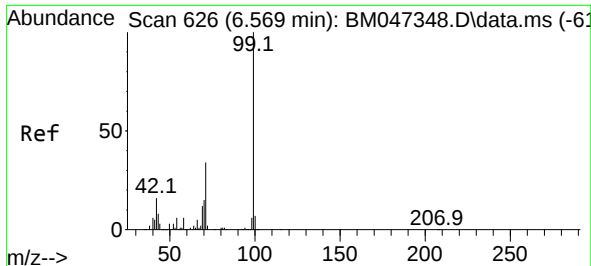

#7
Phenol-d6
Concen: 25.982 ng
RT: 6.569 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39




Instrument :
BNA_M
ClientSampleId :
RBR20046


Tgt Ion: 99 Resp: 632049
Ion Ratio Lower Upper
99 100
42 15.5 13.0 19.4
71 33.9 27.5 41.3

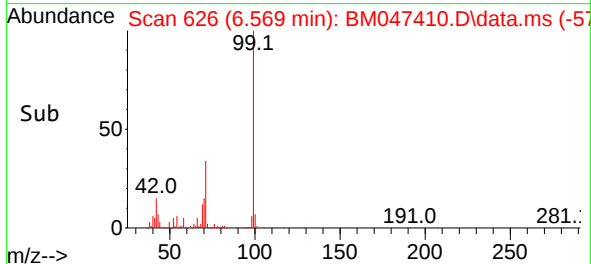

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.098 min Scan# 1226
Delta R.T. -0.006 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39

Tgt Ion: 136 Resp: 1215652
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 6.6 5.2 7.8
68 5.8 4.6 6.8


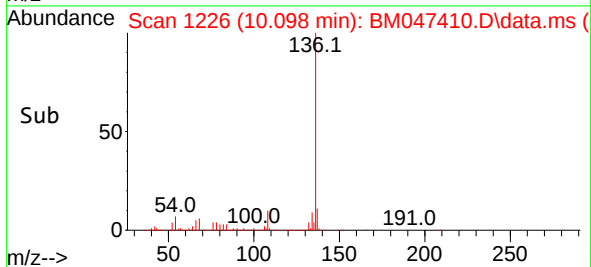

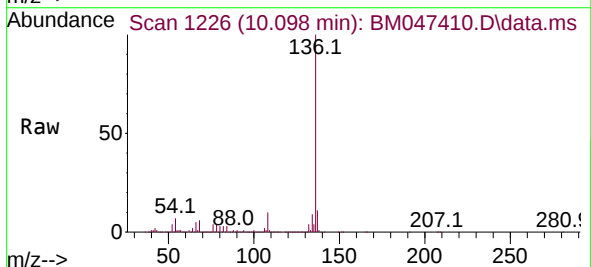


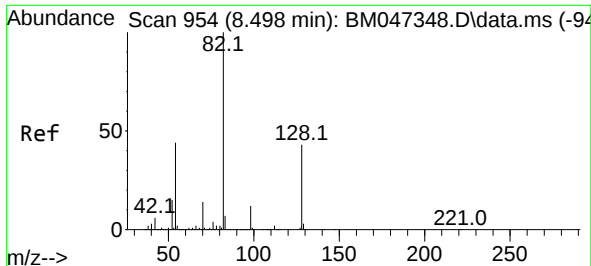

#23
Nitrobenzene-d5
Concen: 53.507 ng
RT: 8.492 min Scan# 91
Delta R.T. -0.006 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39




Instrument :
BNA_M
ClientSampleId :
RBR20046


Tgt Ion: 82 Resp: 1172304
Ion Ratio Lower Upper
82 100
128 44.2 34.6 51.8
54 43.9 35.5 53.3

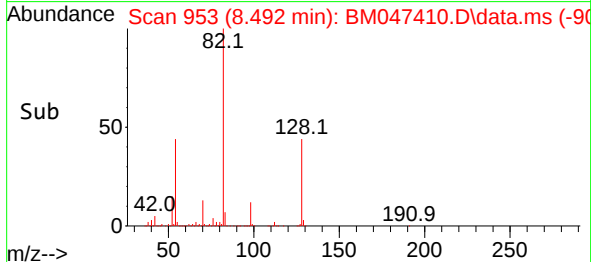

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.016 min Scan# 1892
Delta R.T. 0.006 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39

Tgt Ion:164 Resp: 596231
Ion Ratio Lower Upper
164 100
162 95.7 79.7 119.5
160 43.0 34.9 52.3


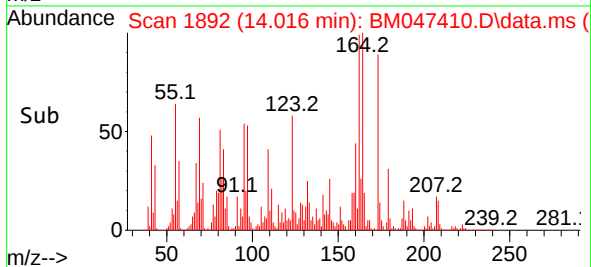

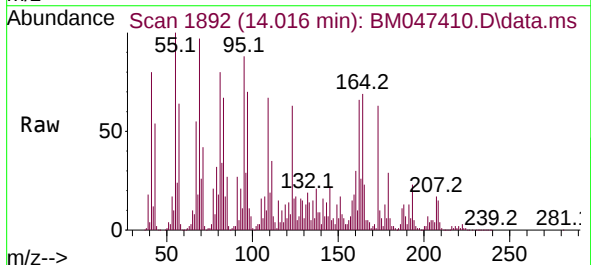


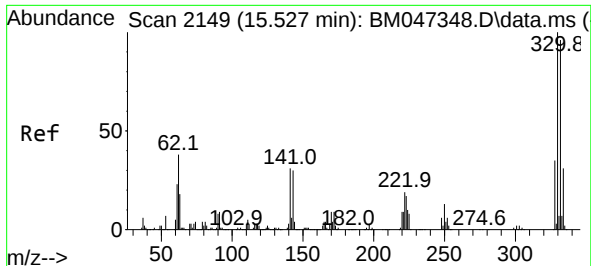

#42
2,4,6-Tribromophenol
Concen: 0.296 ng
RT: 15.563 min Scan# 2149
Delta R.T. 0.035 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39




Instrument :
BNA_M
ClientSampleId :
RBR20046


Tgt Ion:330 Resp: 2132
Ion Ratio Lower Upper
330 100
332 211.7 77.2 115.8#
141 0.0 27.6 41.4#

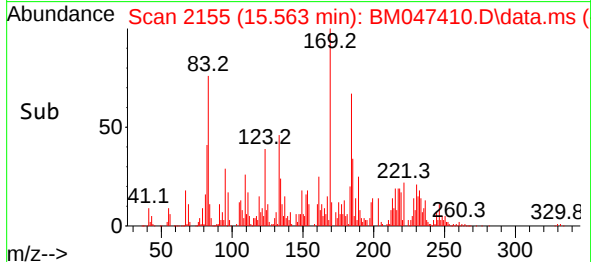

#45
2-Fluorobiphenyl
Concen: 66.361 ng
RT: 12.610 min Scan# 1653
Delta R.T. -0.006 min
Lab File: BM047410.D
Acq: 30 Aug 2024 17:39

Tgt Ion:172 Resp: 2575113
Ion Ratio Lower Upper
172 100
171 35.0 27.8 41.6
170 23.3 18.5 27.7

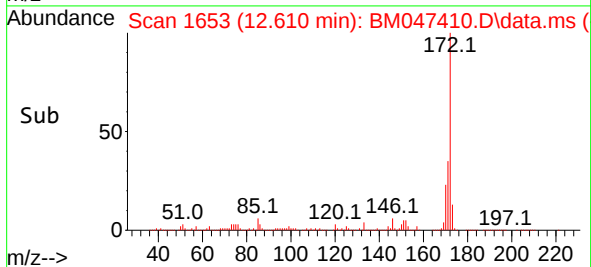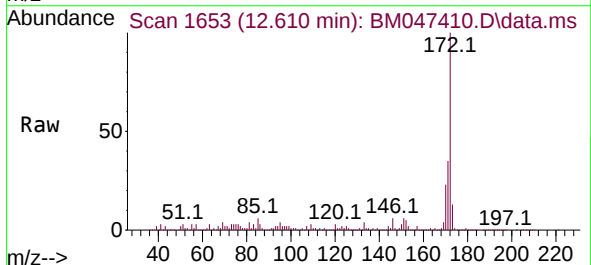



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.845 min Scan# 21

Delta R.T. 0.071 min

Lab File: BM047410.D

Acq: 30 Aug 2024 17:39

Instrument :

BNA_M

ClientSampleId :

RBR20046





Tgt Ion:188 Resp: 633330

Ion Ratio Lower Upper

188 100

94 46.6 6.4 9.6#

80 39.1 7.4 11.2#

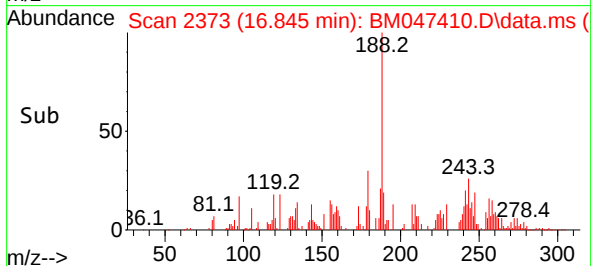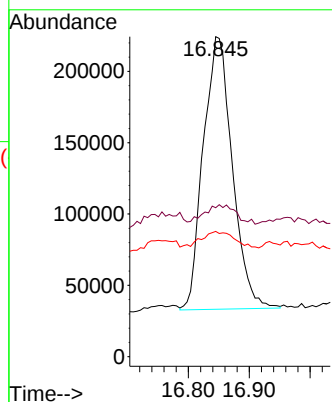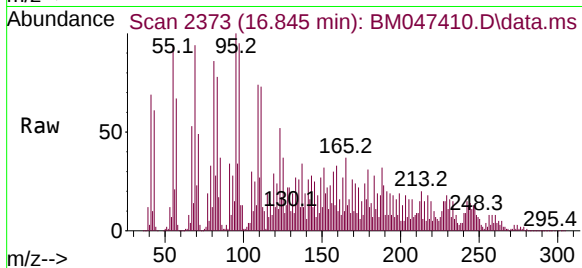

#71

Phenanthrene

Concen: 19.803 ng

RT: 16.892 min Scan# 2381

Delta R.T. 0.071 min

Lab File: BM047410.D

Acq: 30 Aug 2024 17:39




Tgt Ion:178 Resp: 609077


Ion Ratio Lower Upper

178 100

176 29.9 15.2 22.8#

179 114.0 12.2 18.4#

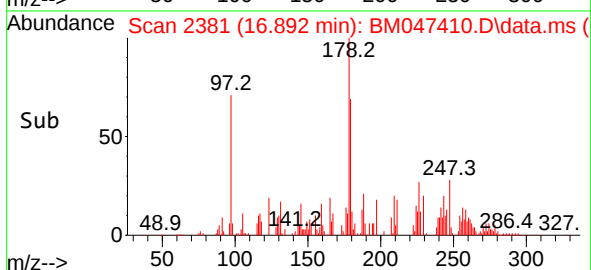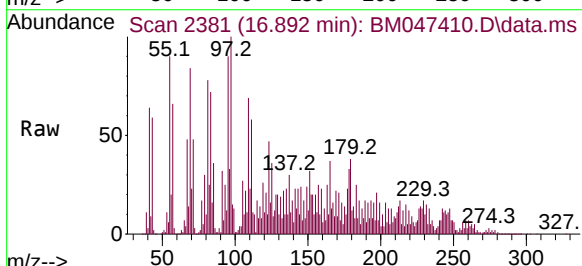



#74

Di-n-butylphthalate

Concen: 12.877 ng

RT: 17.809 min Scan# 2

Delta R.T. 0.035 min

Lab File: BM047410.D

Acq: 30 Aug 2024 17:39

Instrument :

BNA_M

ClientSampleId :

RBR20046





Tgt Ion:149 Resp: 451145

Ion Ratio Lower Upper

149 100

150 44.9 7.4 11.0#

104 9.8 3.8 5.6#

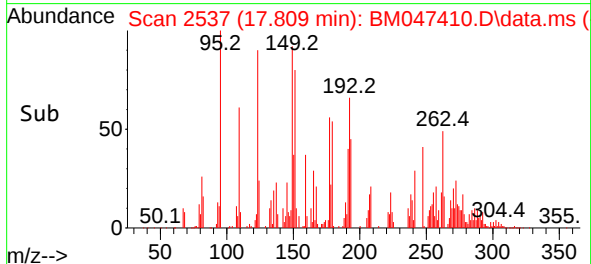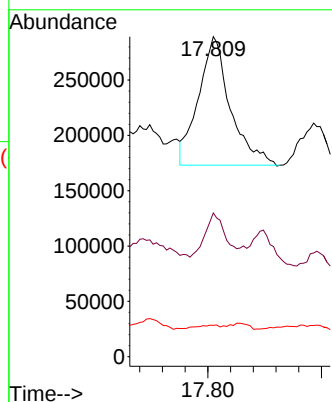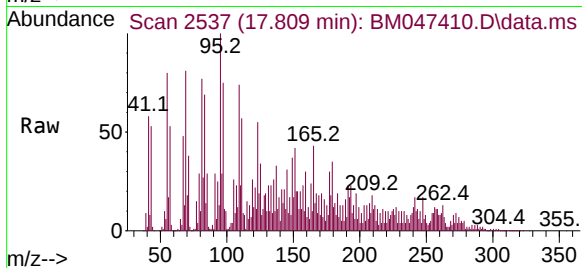

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.050 min Scan# 3088

Delta R.T. 0.029 min

Lab File: BM047410.D

Acq: 30 Aug 2024 17:39




Tgt Ion:240 Resp: 1001003


Ion Ratio Lower Upper

240 100

120 10.1 7.4 11.0

236 26.9 20.8 31.2


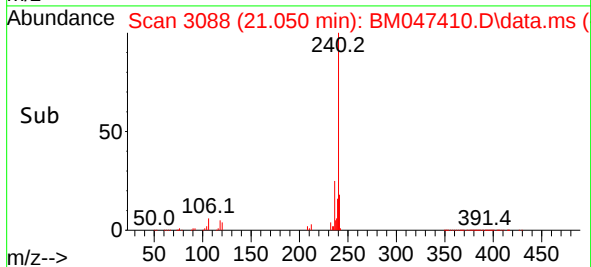
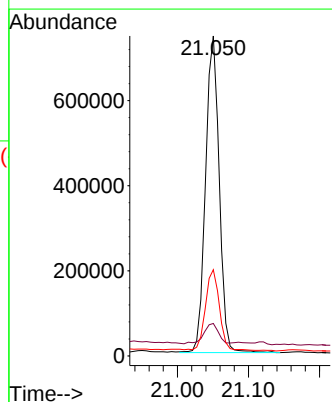
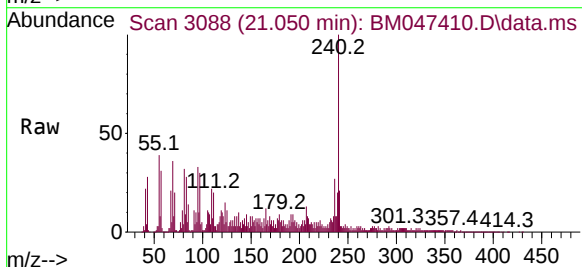


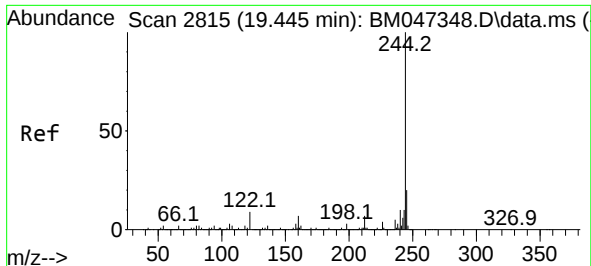

#79
 Terphenyl-d14
 Concen: 39.118 ng
 RT: 19.492 min Scan# 21
 Delta R.T. 0.047 min
 Lab File: BM047410.D
 Acq: 30 Aug 2024 17:39

Instrument :
 BNA_M
 ClientSampleId :
 RBR20046

Tgt Ion:244 Resp: 2199911
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 9.3 7.0 10.4

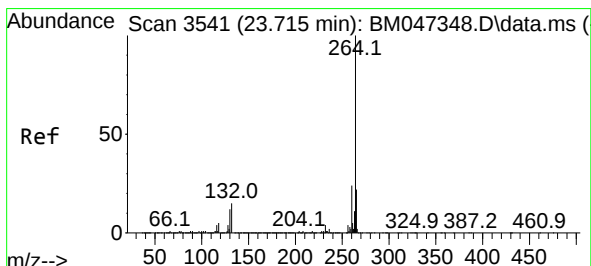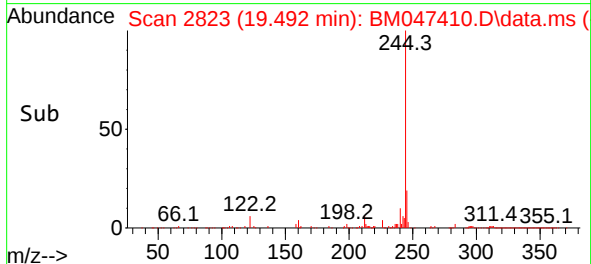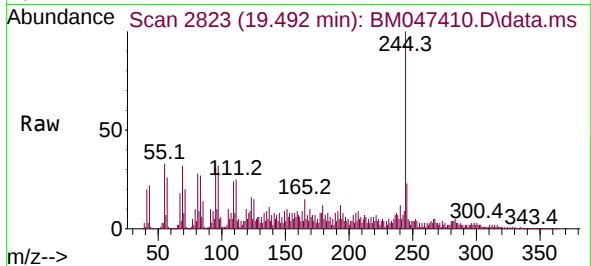

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.733 min Scan# 3544
 Delta R.T. 0.018 min
 Lab File: BM047410.D
 Acq: 30 Aug 2024 17:39

Tgt Ion:264 Resp: 1281328
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.0 28.4
 265 21.7 17.8 26.6

