
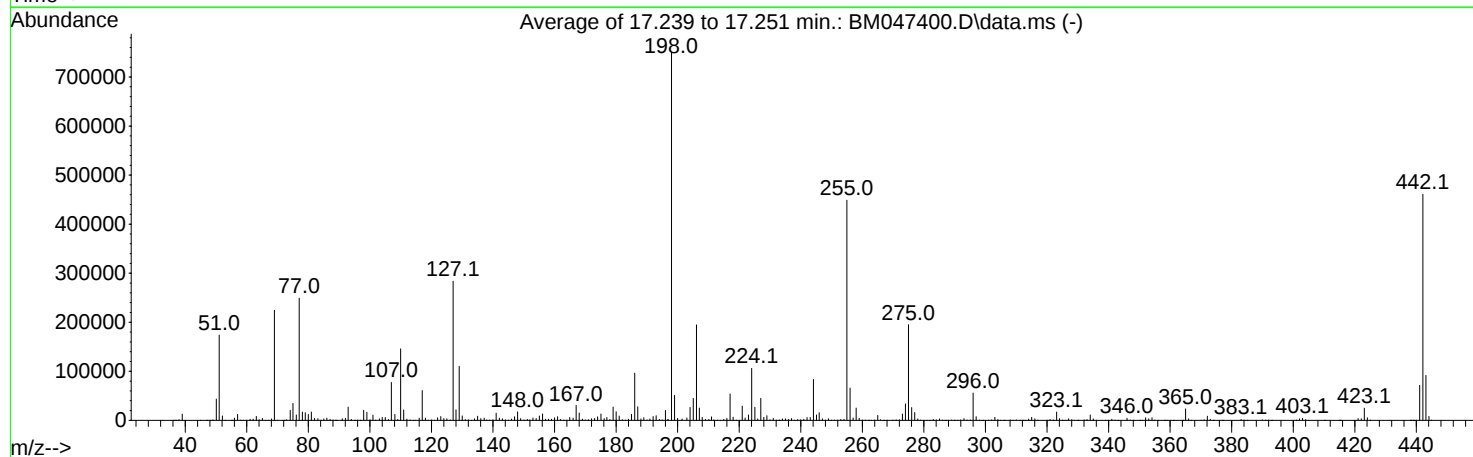


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047400.D
Acq On : 30 Aug 2024 10:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

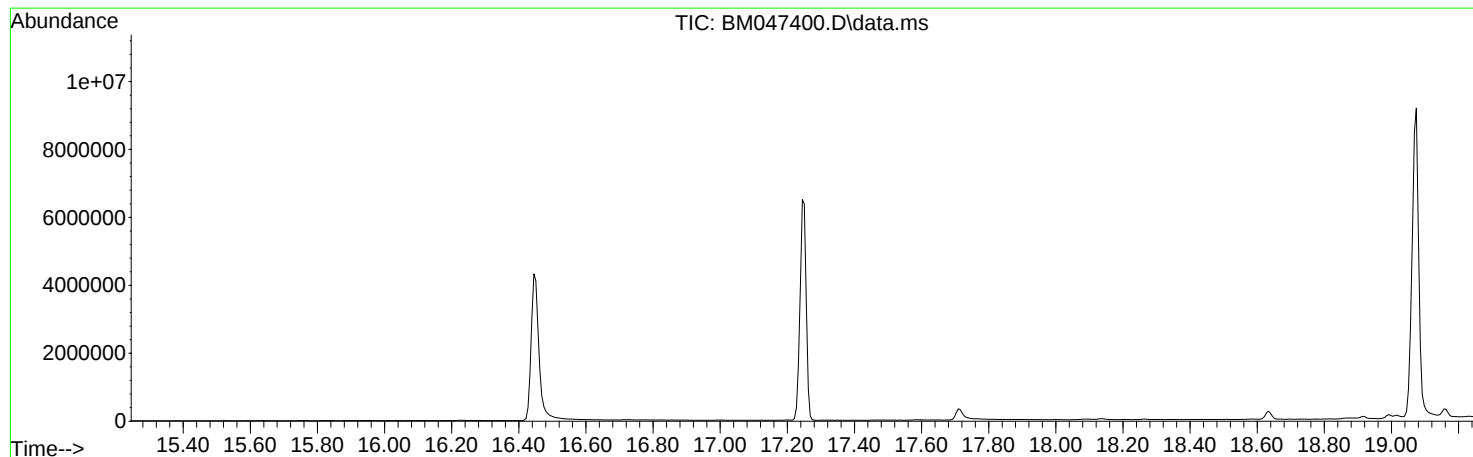

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	173969	PASS
68	69	0.00	2	1.3	2936	PASS
69	198	0.00	100	29.9	224390	PASS
70	69	0.00	2	0.2	422	PASS
127	198	10	80	37.8	283712	PASS
197	198	0.00	2	0.3	2014	PASS
198	198	100	100	100.0	749952	PASS
199	198	5	9	6.8	51120	PASS
275	198	10	60	26.0	195029	PASS
365	198	1	100	3.1	23381	PASS
441	198	0.01	100	9.5	71363	PASS
442	442	50	100	100.0	461013	PASS
443	442	15	24	19.9	91605	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/30/2024	BNA_M	<u>BM047400.D</u>
Compound Name	Response	Retention Time
DDT	2897034	20.309
DDD	55494	19.909
DDE	5717	19.35
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61211	2958245	2.07

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047400.D
Acq On : 30 Aug 2024 10:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 30 11:41:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

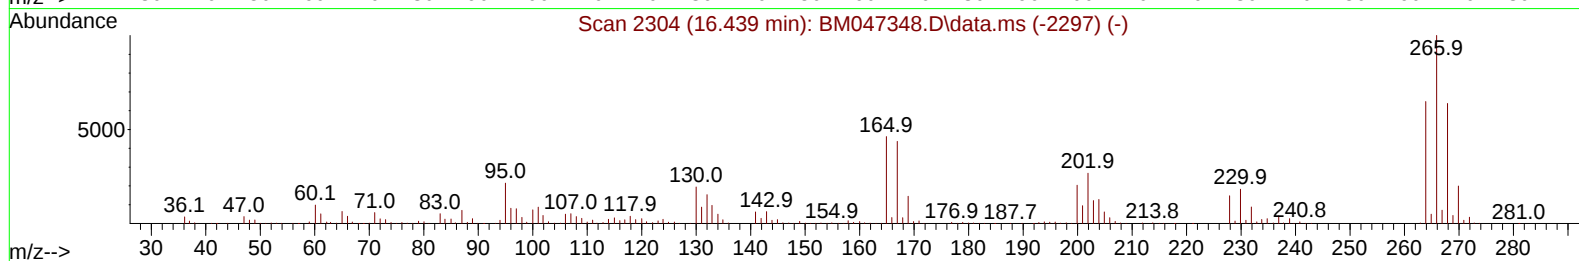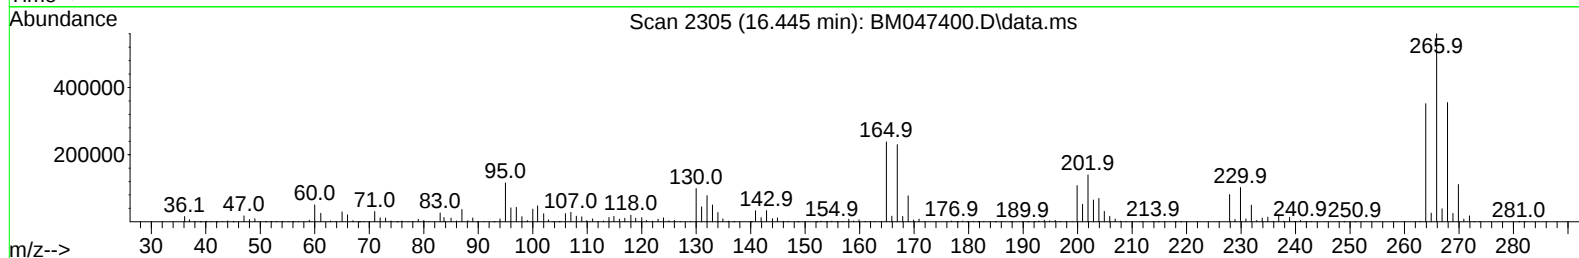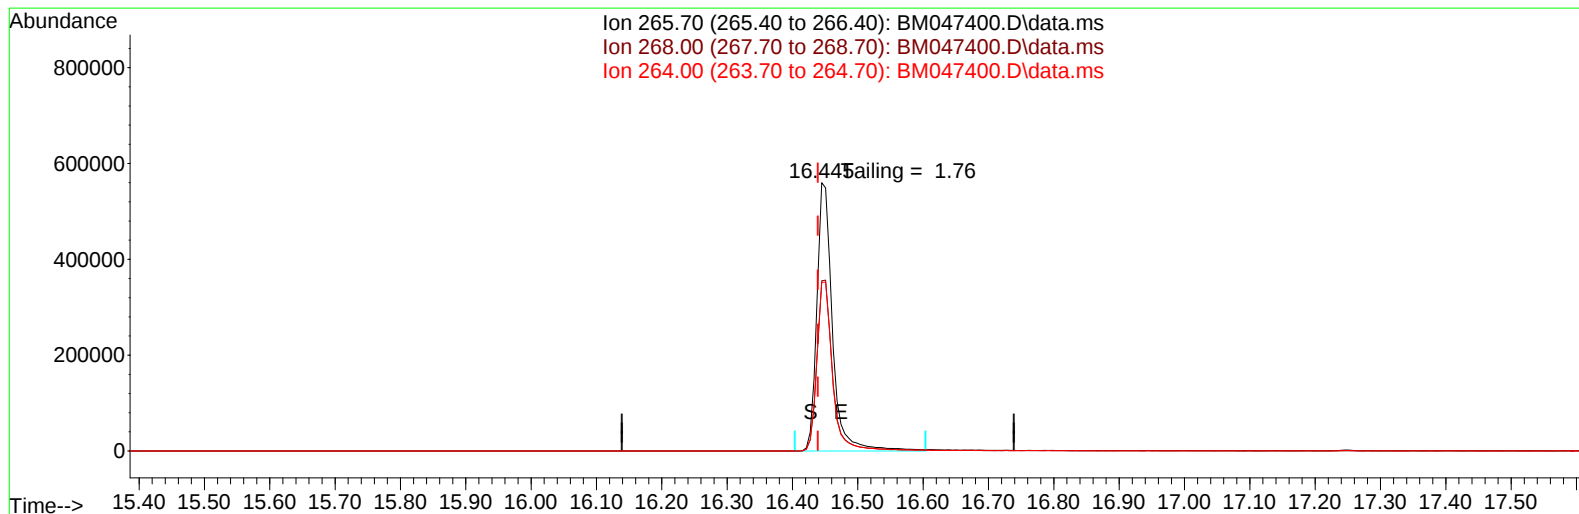

TIC: BM047400.D\data.ms

(70) Pentachlorophenol (C)

16.445min (+ 0.006) 233397.58 ng




response 934029

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.42
264.00	64.90	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083024\
Data File : BM047400.D
Acq On : 30 Aug 2024 10:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 30 11:41:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

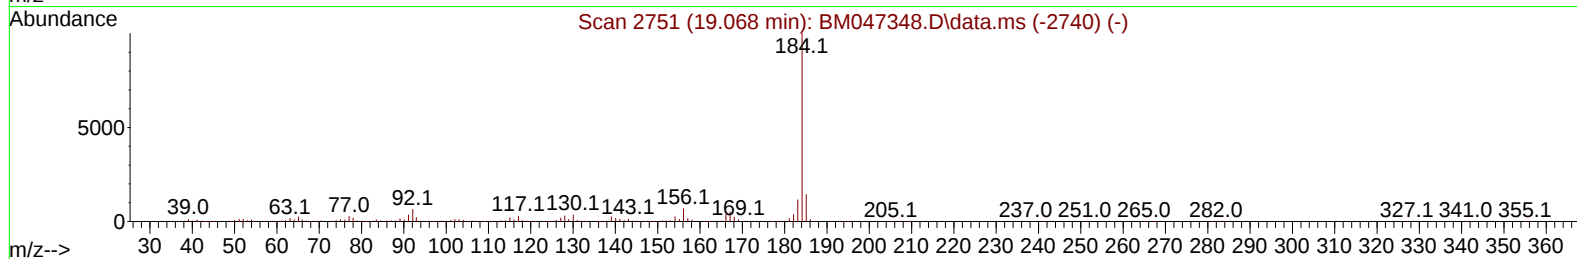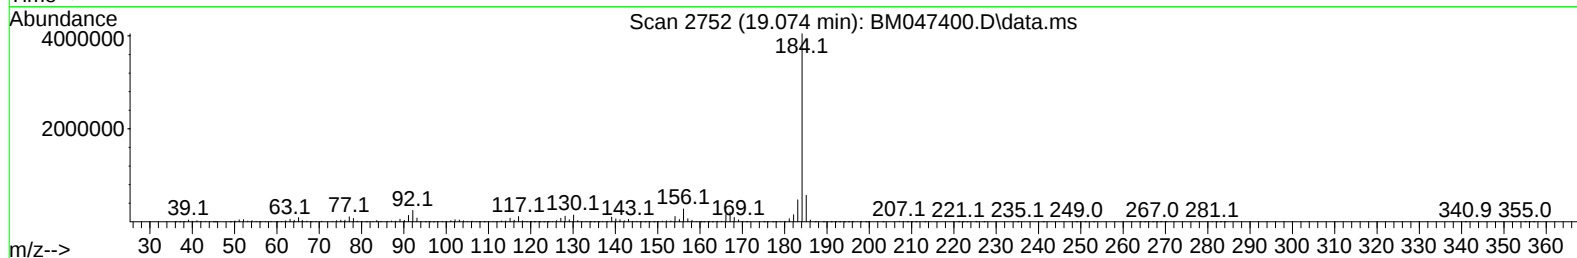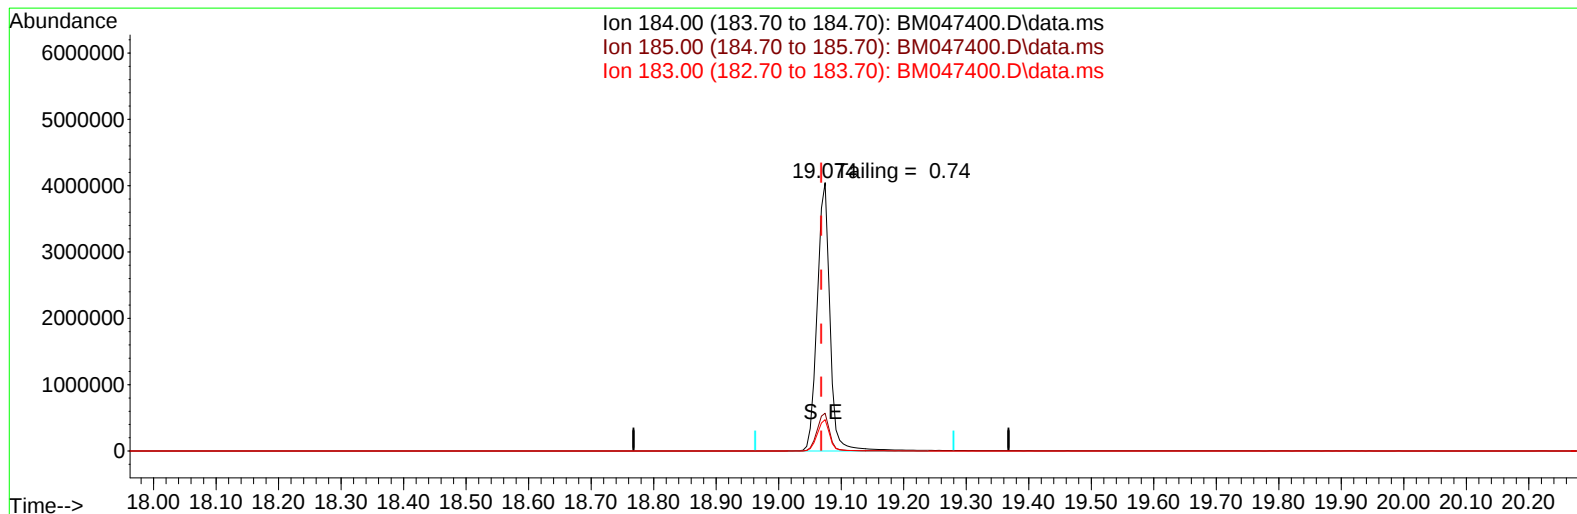

TIC: BM047400.D\data.ms

(77) Benzidine

19.074min (+ 0.006) 86573.98 ng

response 5776142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	11.50	11.70
0.00	0.00	0.00