

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM083115\
 Data File : BM002593.D
 Acq On : 31 Aug 2015 17:33
 Operator : UM/IZ
 Sample : G3456-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9E87

Quant Time: Sep 01 01:42:01 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 01 01:38:52 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	138934	20.00	ng/ul	0.00
2) Naphthalene-d8	11.65	136	606349	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.37	164	285408	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.08	188	480521	20.00	ng/ul	0.00
17) Chrysene-d12	22.16	240	398292	20.00	ng/ul	0.00
22) Perylene-d12	24.79	264	413692	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.07	160	672314	23.04	ng/ul	0.00
10) Fluorene-d10	16.34	176	411157	20.06	ng/ul	0.00
14) Anthracene-d10	18.17	188	529569	22.85	ng/ul	0.00
18) Pyrene-d10	20.40	212	398066	22.55	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.62	264	405317	18.65	ng/ul	0.00
Target Compounds						
19) Pyrene	20.43	202	27876	1.19	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM083115\
Data File : BM002593.D
Acq On : 31 Aug 2015 17:33
Operator : UM/IZ
Sample : G3456-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9E87

Quant Time: Sep 01 01:42:01 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 01 01:38:52 2015
Response via : Initial Calibration

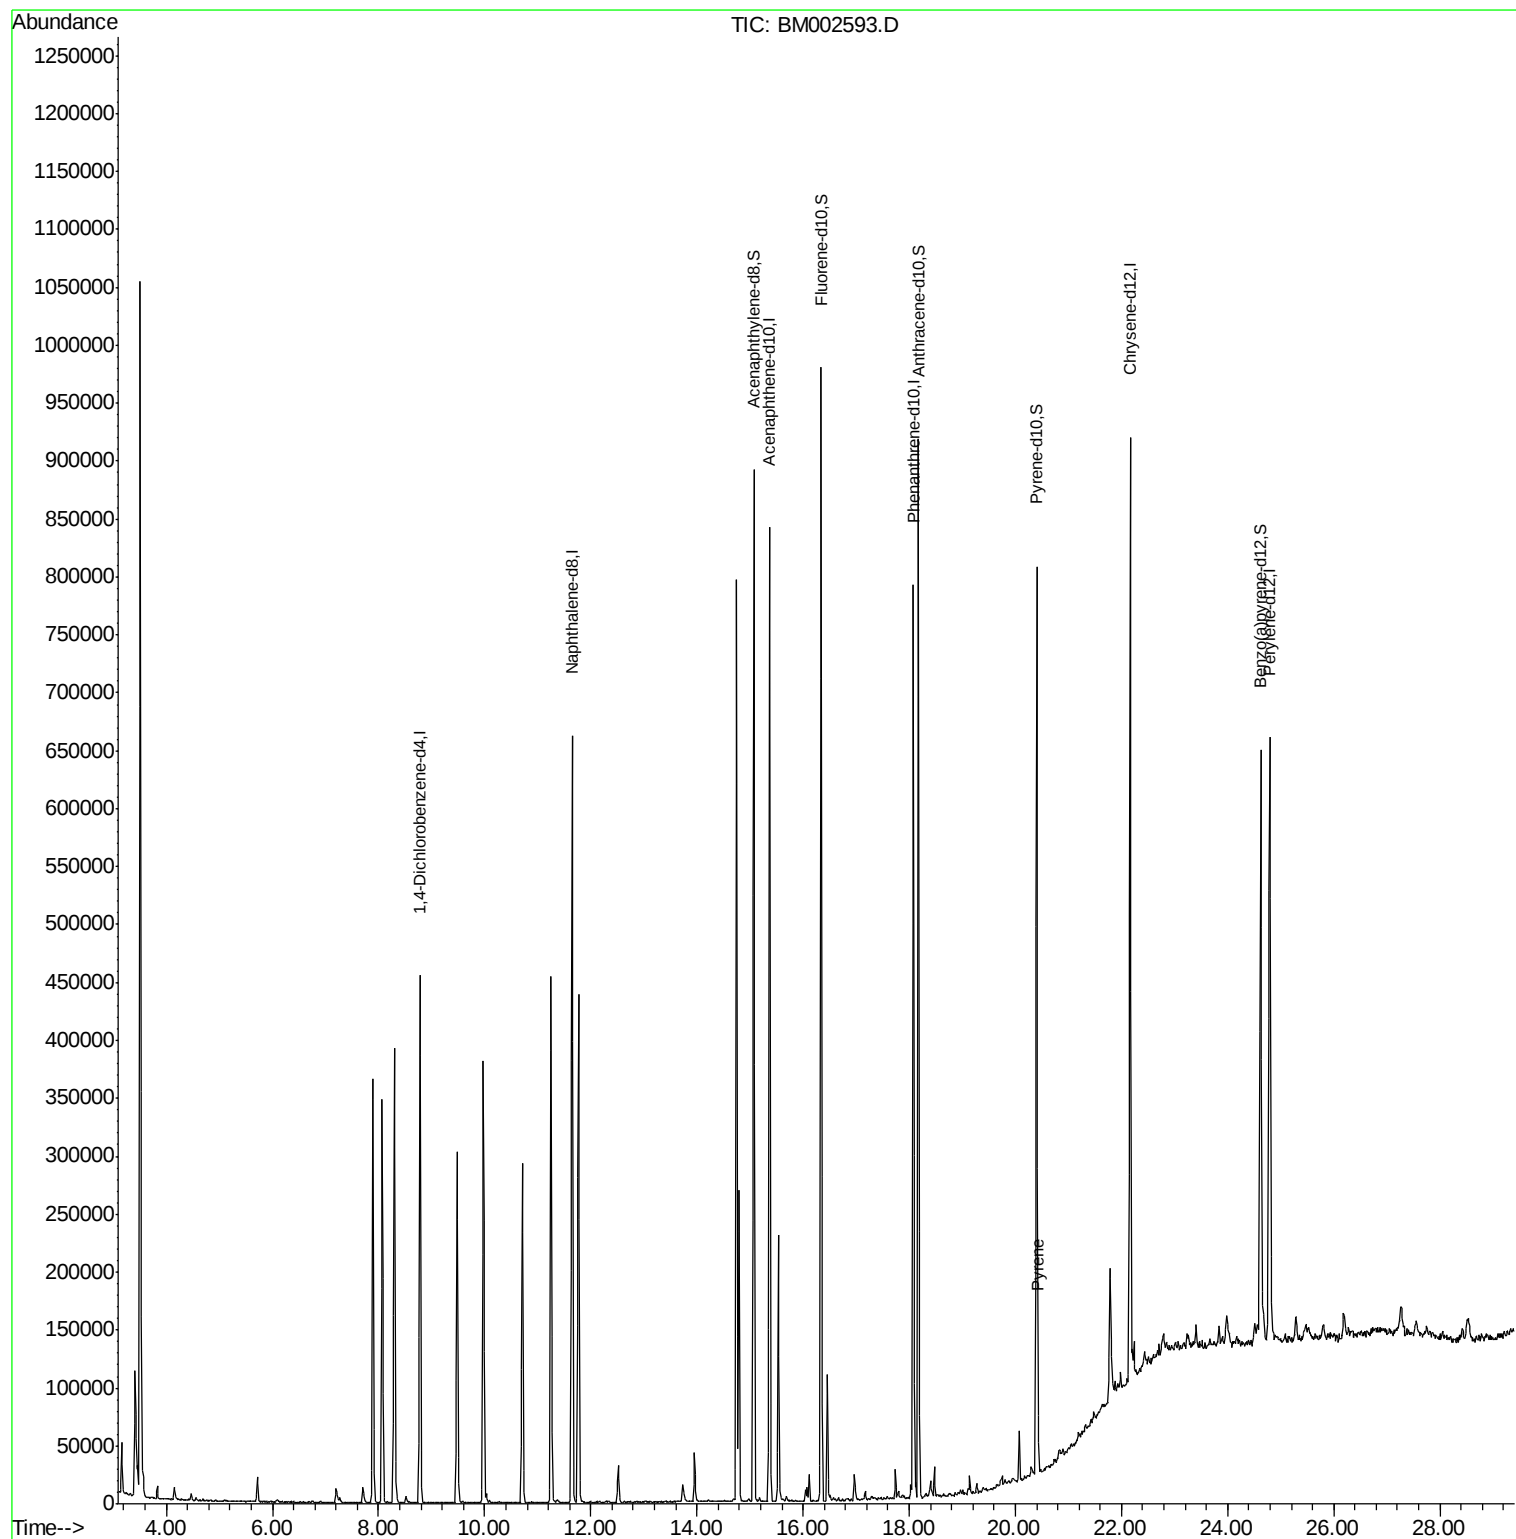

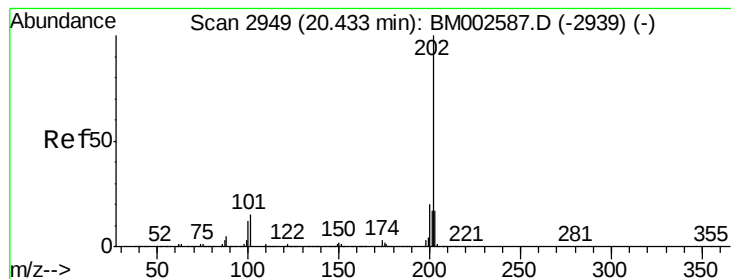

#19

Pyrene

Concen: 1.19 ng/ul

RT: 20.43 min Scan# 2948

Delta R.T. -0.01 min

Lab File: BM002593.D

Acq: 31 Aug 2015 17:33

Instrument :

BNA_M

ClientSampleId :

D9E87


Tgt Ion: 202 Resp: 27876

Ion Ratio Lower Upper

202 100

101 15.8 12.0 18.0

100 13.2 9.7 14.5

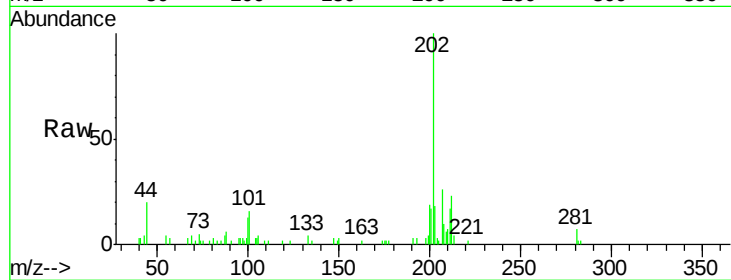

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

