

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM083115\
 Data File : BM002636.D
 Acq On : 01 Sep 2015 19:46
 Operator : UM/IZ
 Sample : G3456-08RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9E92RE

Quant Time: Sep 02 00:46:15 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 00:45:29 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	62432	20.00	ng/ul	0.00
2) Naphthalene-d8	11.65	136	255707	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.37	164	139273	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.08	188	285603	20.00	ng/ul	0.00
17) Chrysene-d12	22.16	240	299045	20.00	ng/ul	0.00
22) Perylene-d12	24.79	264	298525	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.07	160	586646	41.20	ng/ul	0.00
10) Fluorene-d10	16.34	176	346577	34.65	ng/ul	0.00
14) Anthracene-d10	18.17	188	599842	43.54	ng/ul	0.00
18) Pyrene-d10	20.40	212	401749	30.31	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.62	264	527154	33.62	ng/ul	0.00
Target Compounds						
16) Fluoranthene	20.07	202	21260	1.14	ng/ul	Qvalue 99
19) Pyrene	20.43	202	18596	1.06	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM083115\
Data File : BM002636.D
Acq On : 01 Sep 2015 19:46
Operator : UM/IZ
Sample : G3456-08RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9E92RE

Quant Time: Sep 02 00:46:15 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 00:45:29 2015
Response via : Initial Calibration




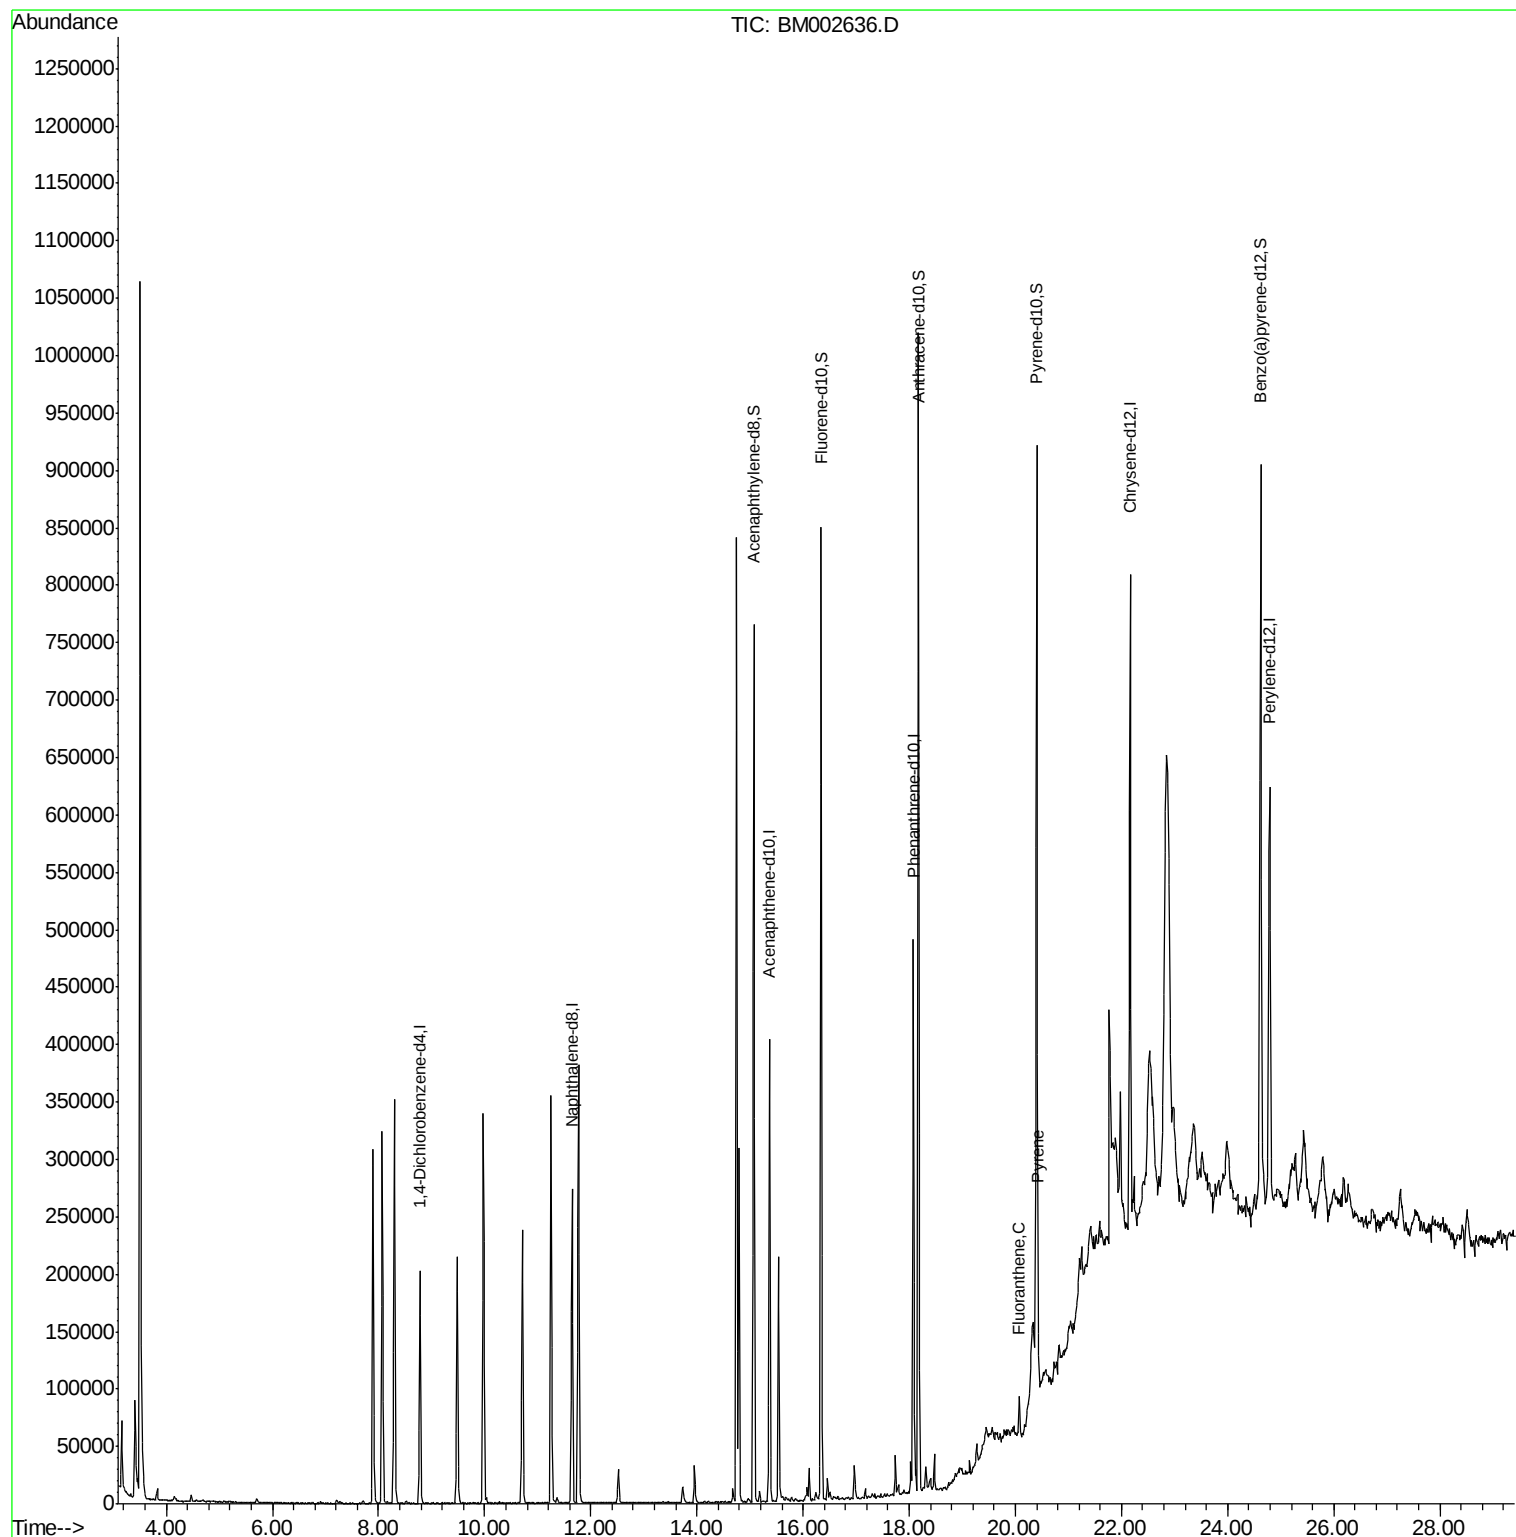


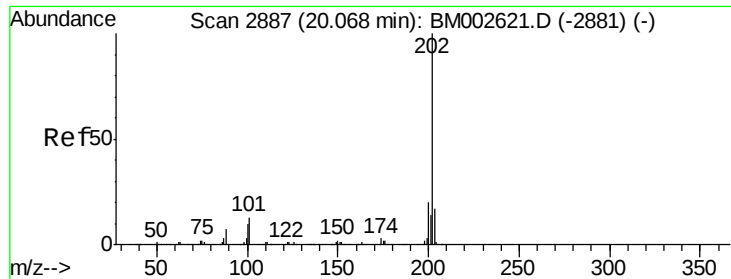

#16
Fluoranthene
Concen: 1.14 ng/ul
RT: 20.07 min Scan# 2887
Delta R.T. 0.00 min
Lab File: BM002636.D
Acq: 01 Sep 2015 19:46

Instrument :
BNA_M
ClientSampleId :
D9E92RE

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.4	9.7	14.5
100	9.8	7.4	11.2

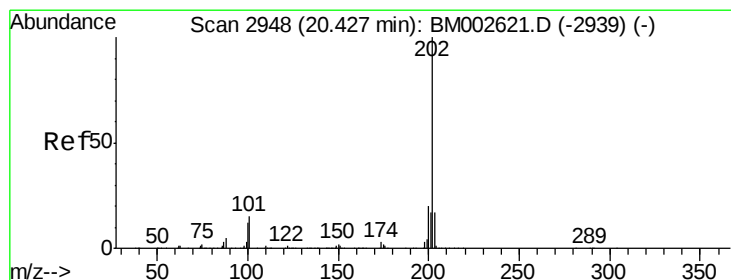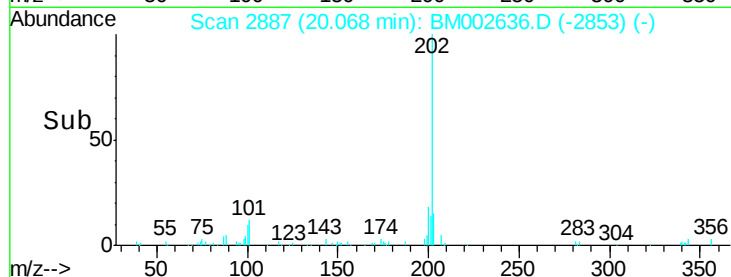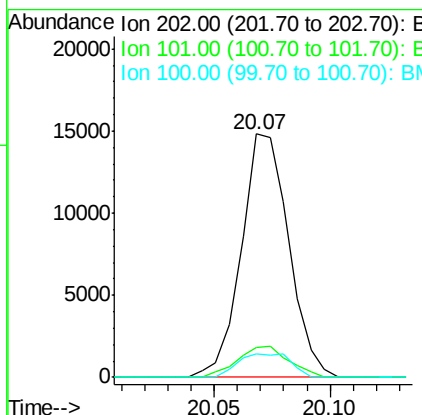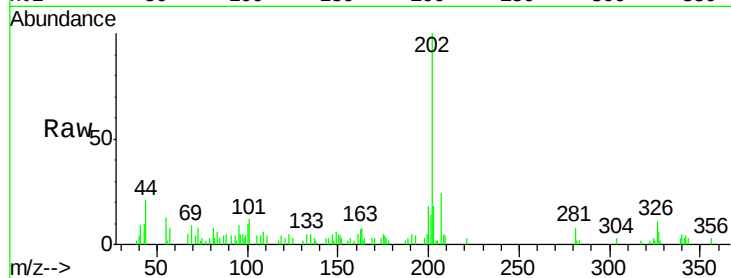

#19
Pyrene
Concen: 1.06 ng/ul
RT: 20.43 min Scan# 2948
Delta R.T. 0.00 min
Lab File: BM002636.D
Acq: 01 Sep 2015 19:46

Tgt Ion	Ratio	Lower	Upper
202	100		
101	18.5	12.0	18.0#
100	13.9	9.7	14.5

