




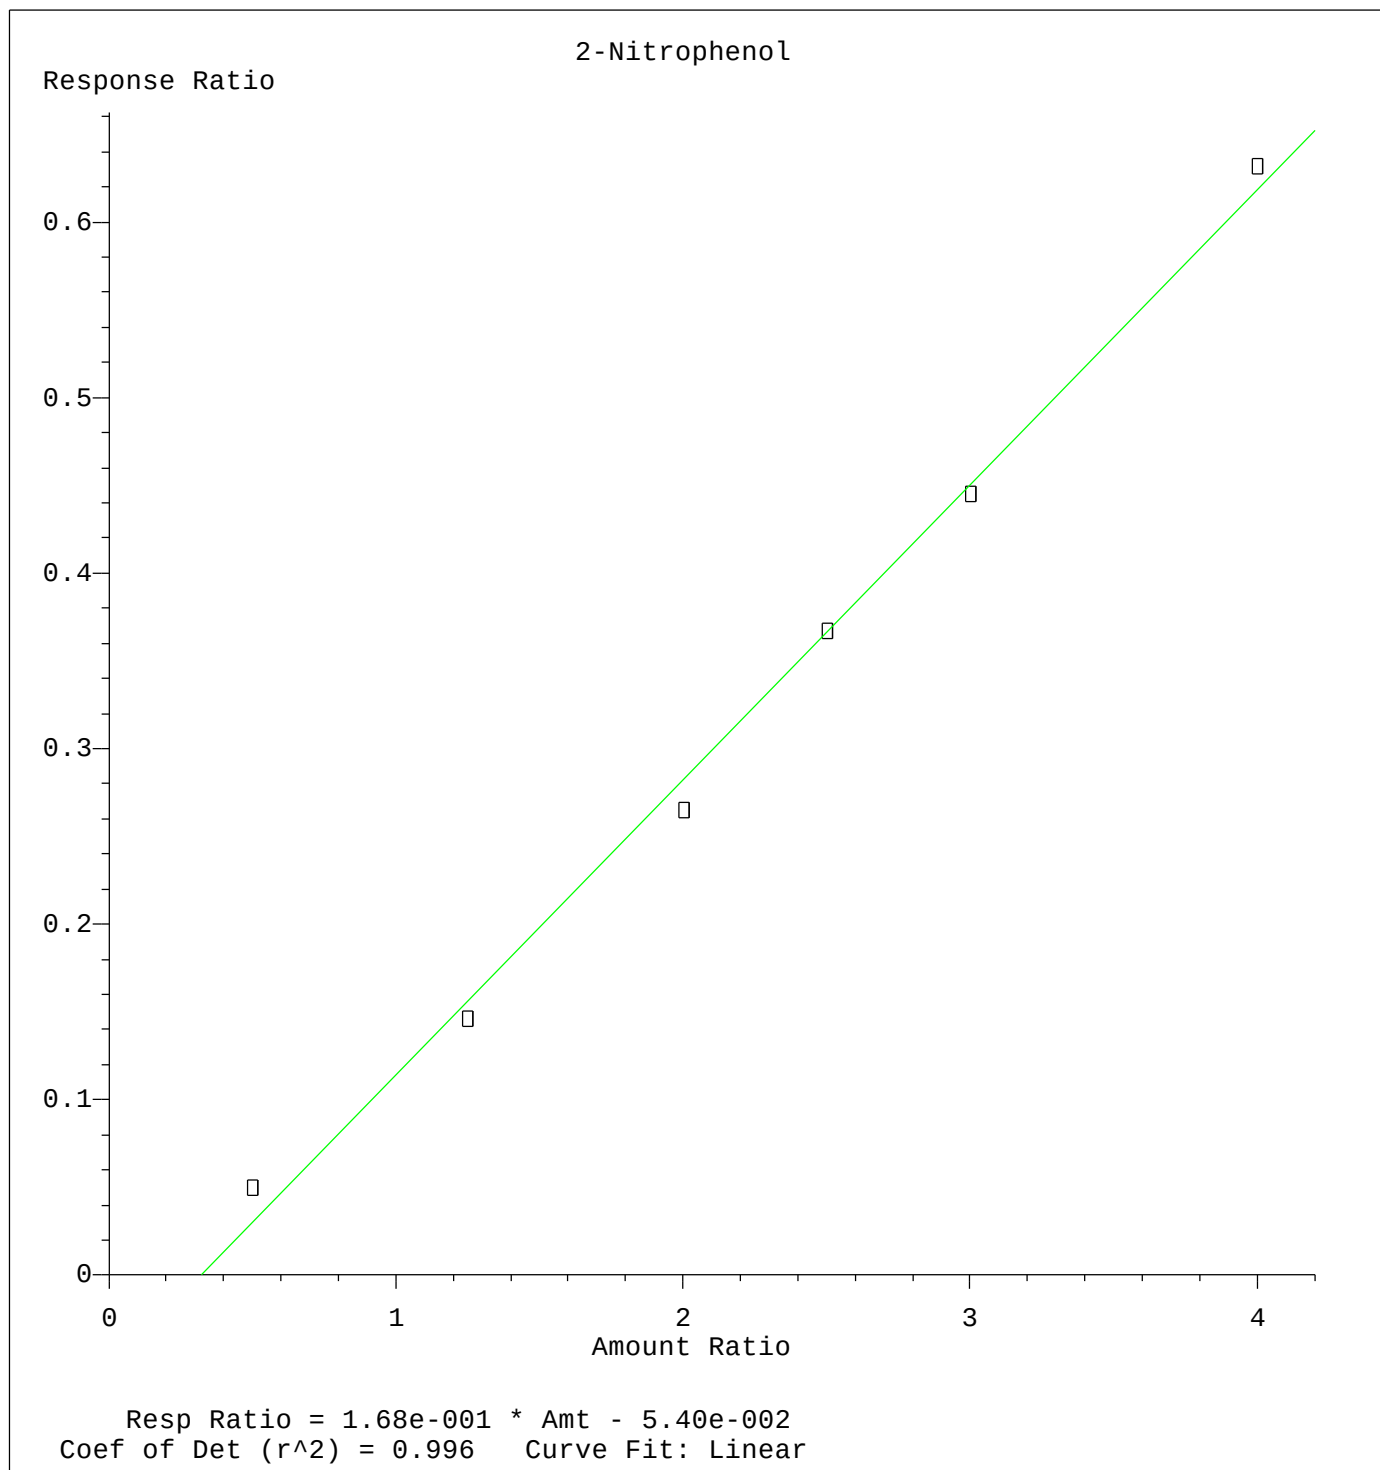

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017

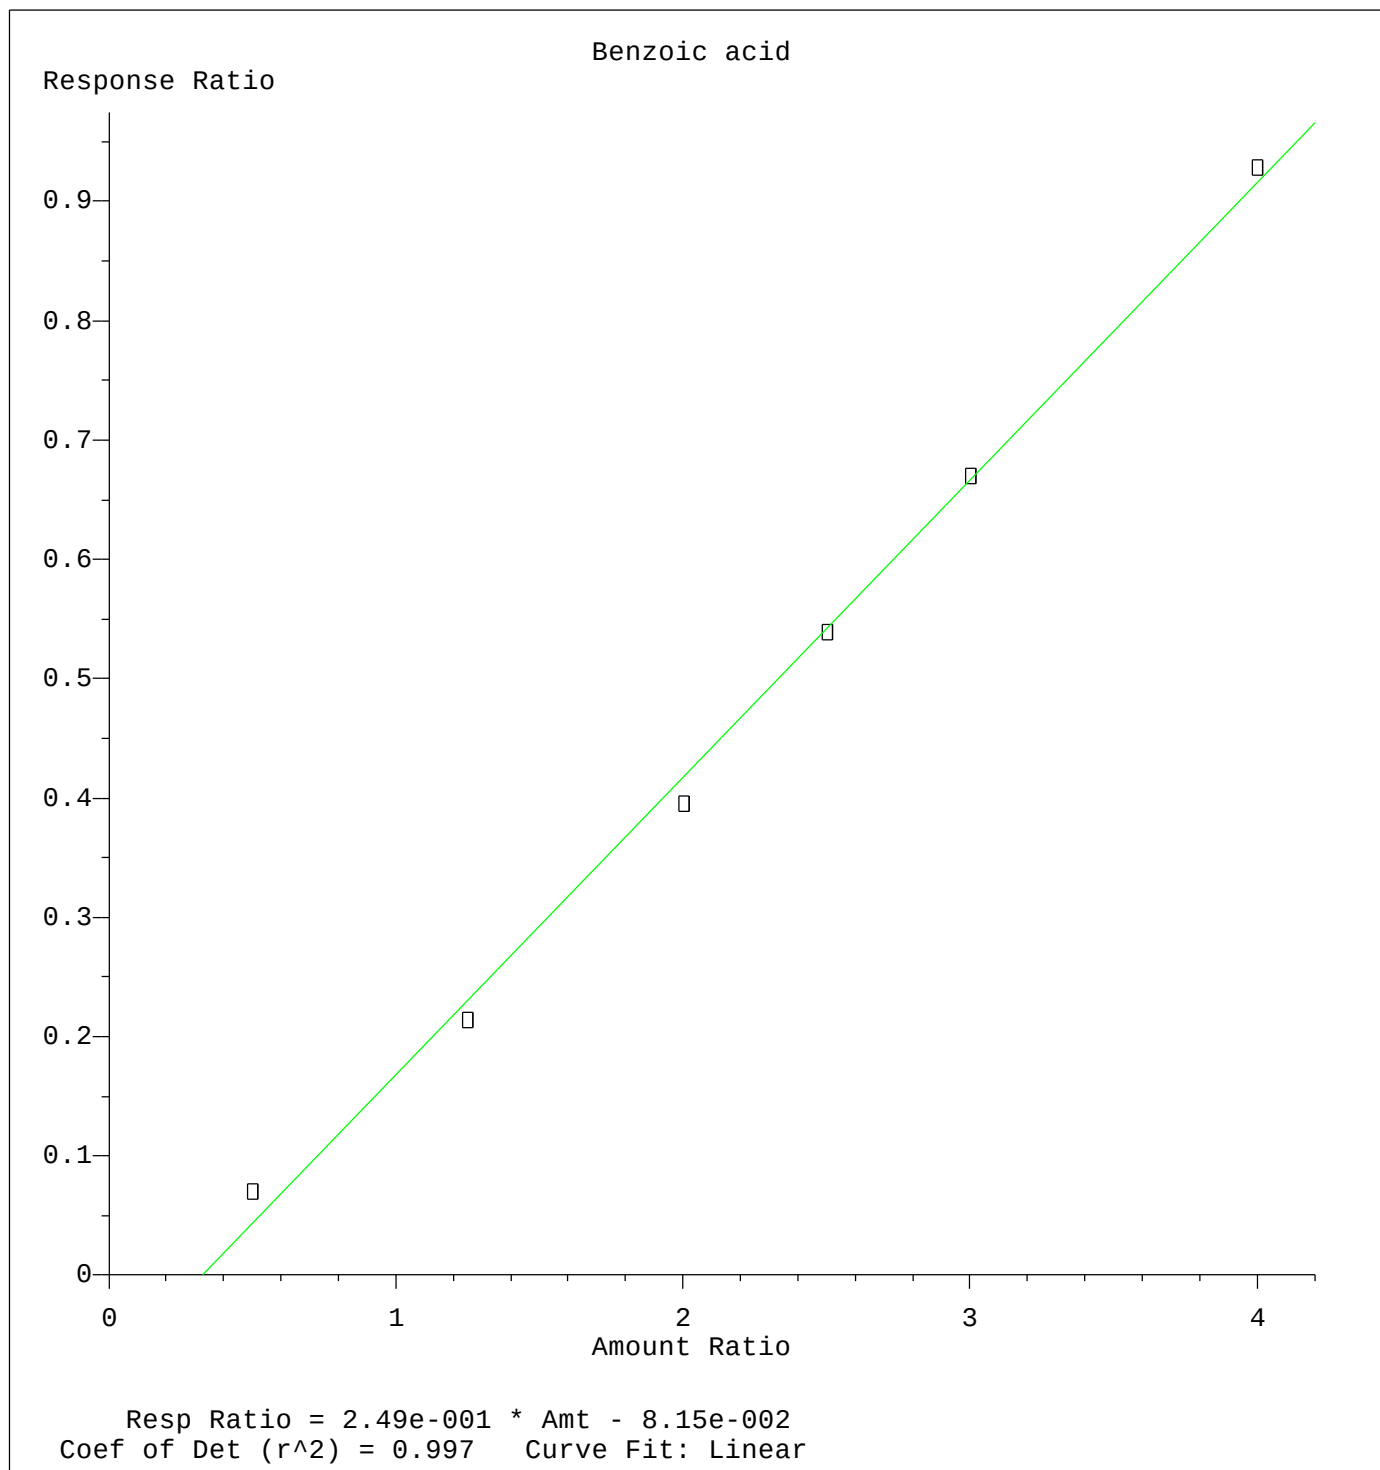


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017

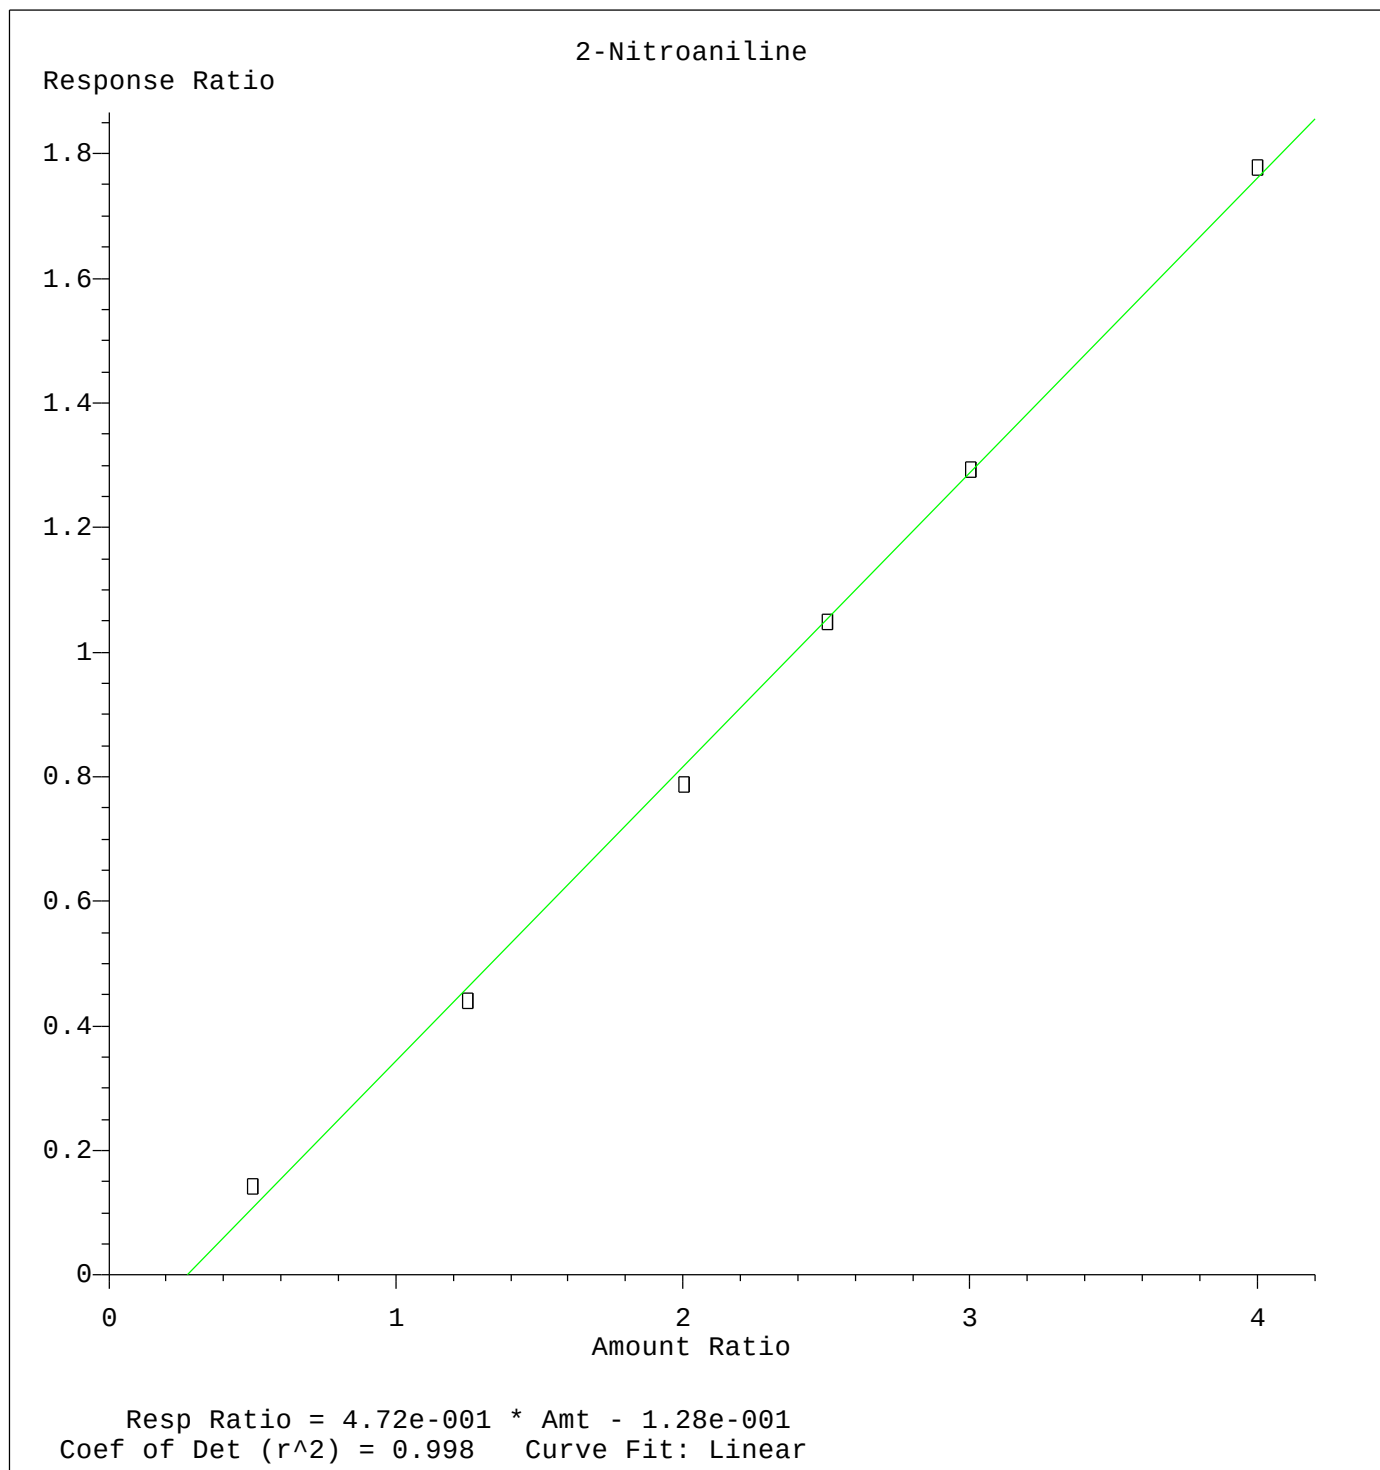

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017

2,4-Dinitrotoluene


Response Ratio

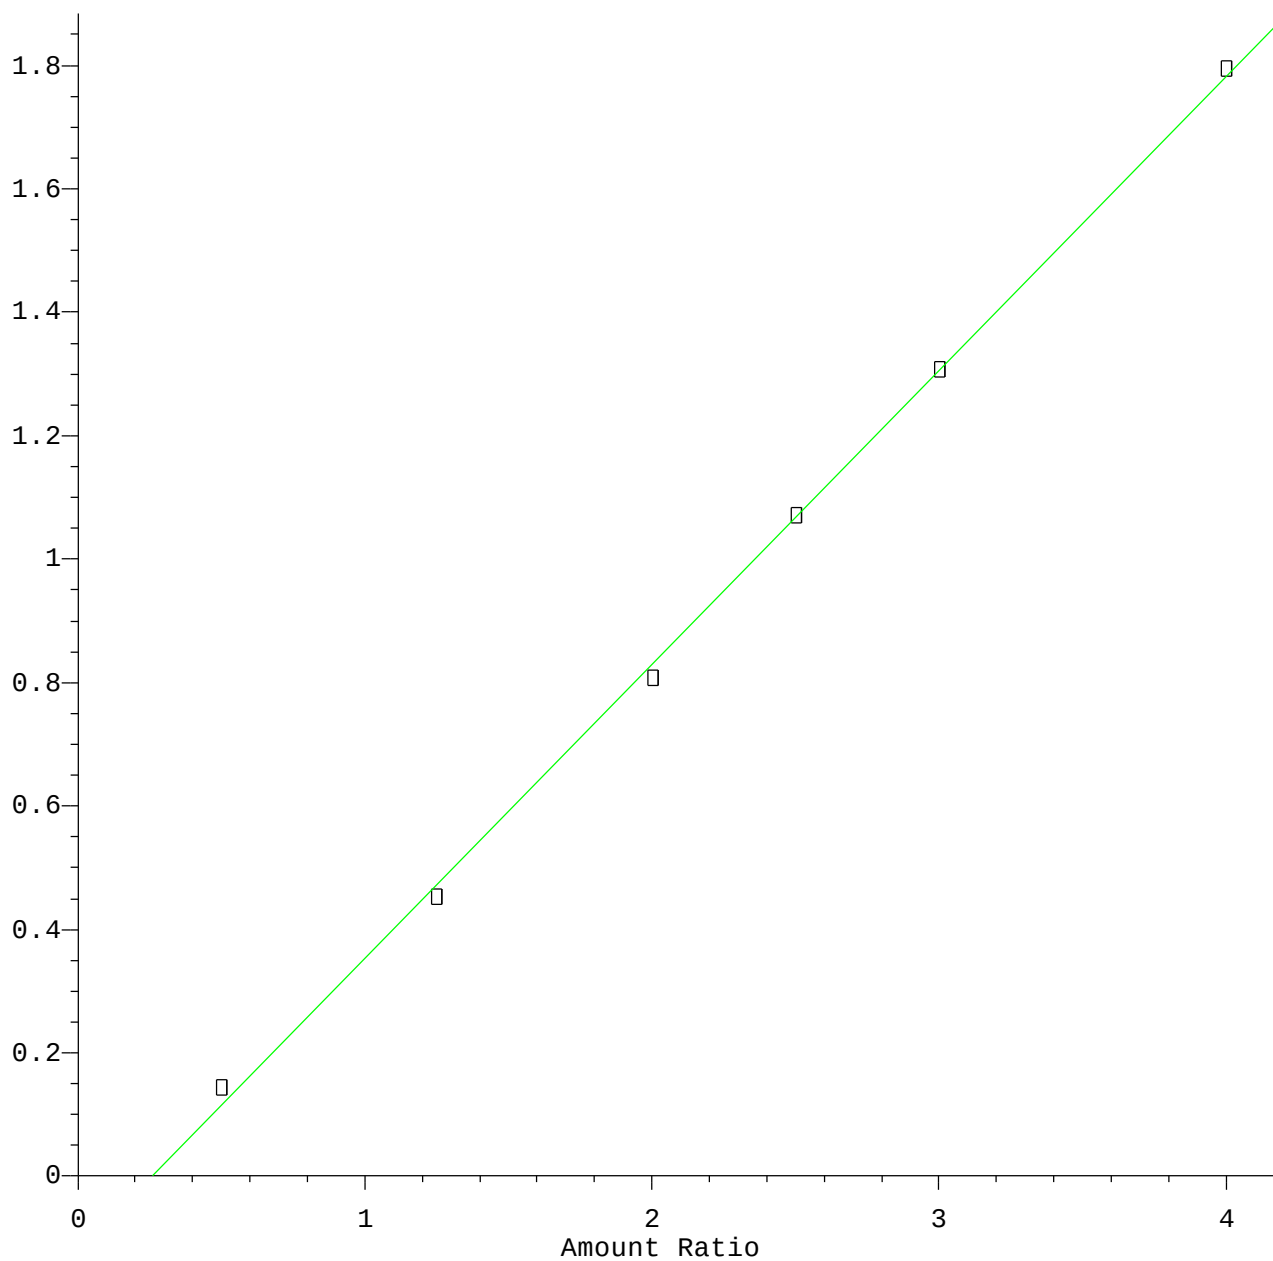

Resp Ratio = $4.76 \times 10^{-1} \times \text{Amt} - 1.22 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017


2,4-Dinitrophenol

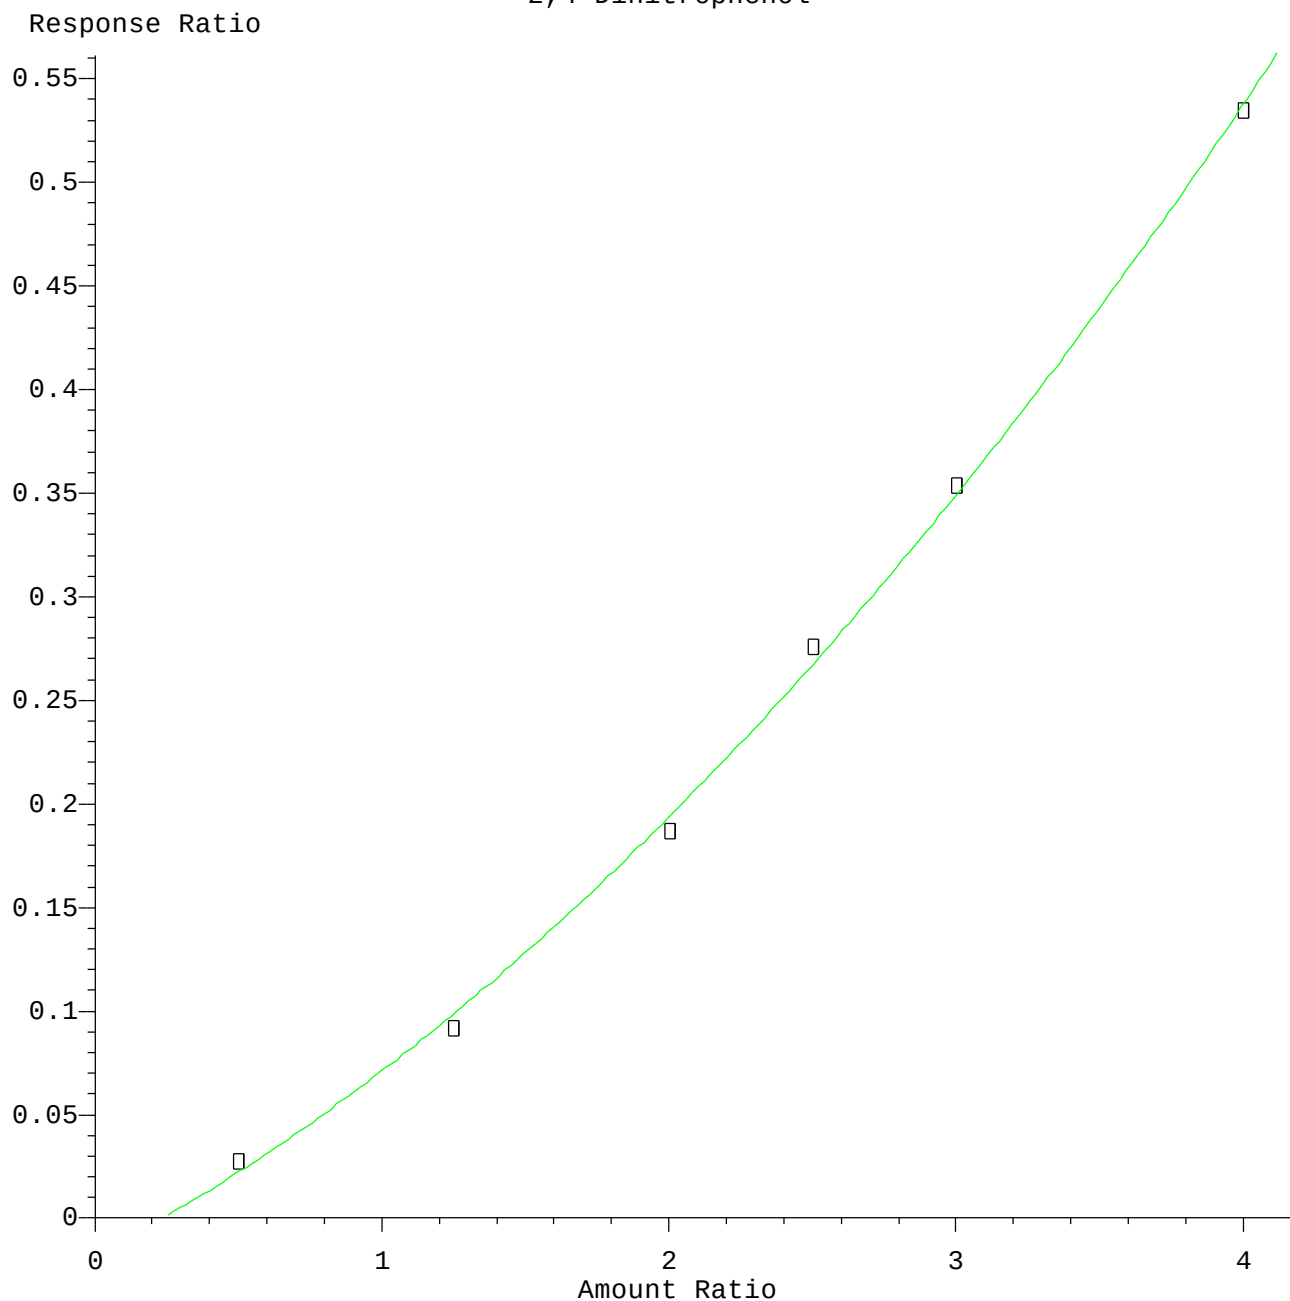

$R = 1.65e-002 A^2 + 7.30e-002 A - 1.84e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017

4,6-Dinitro-2-methylphenol

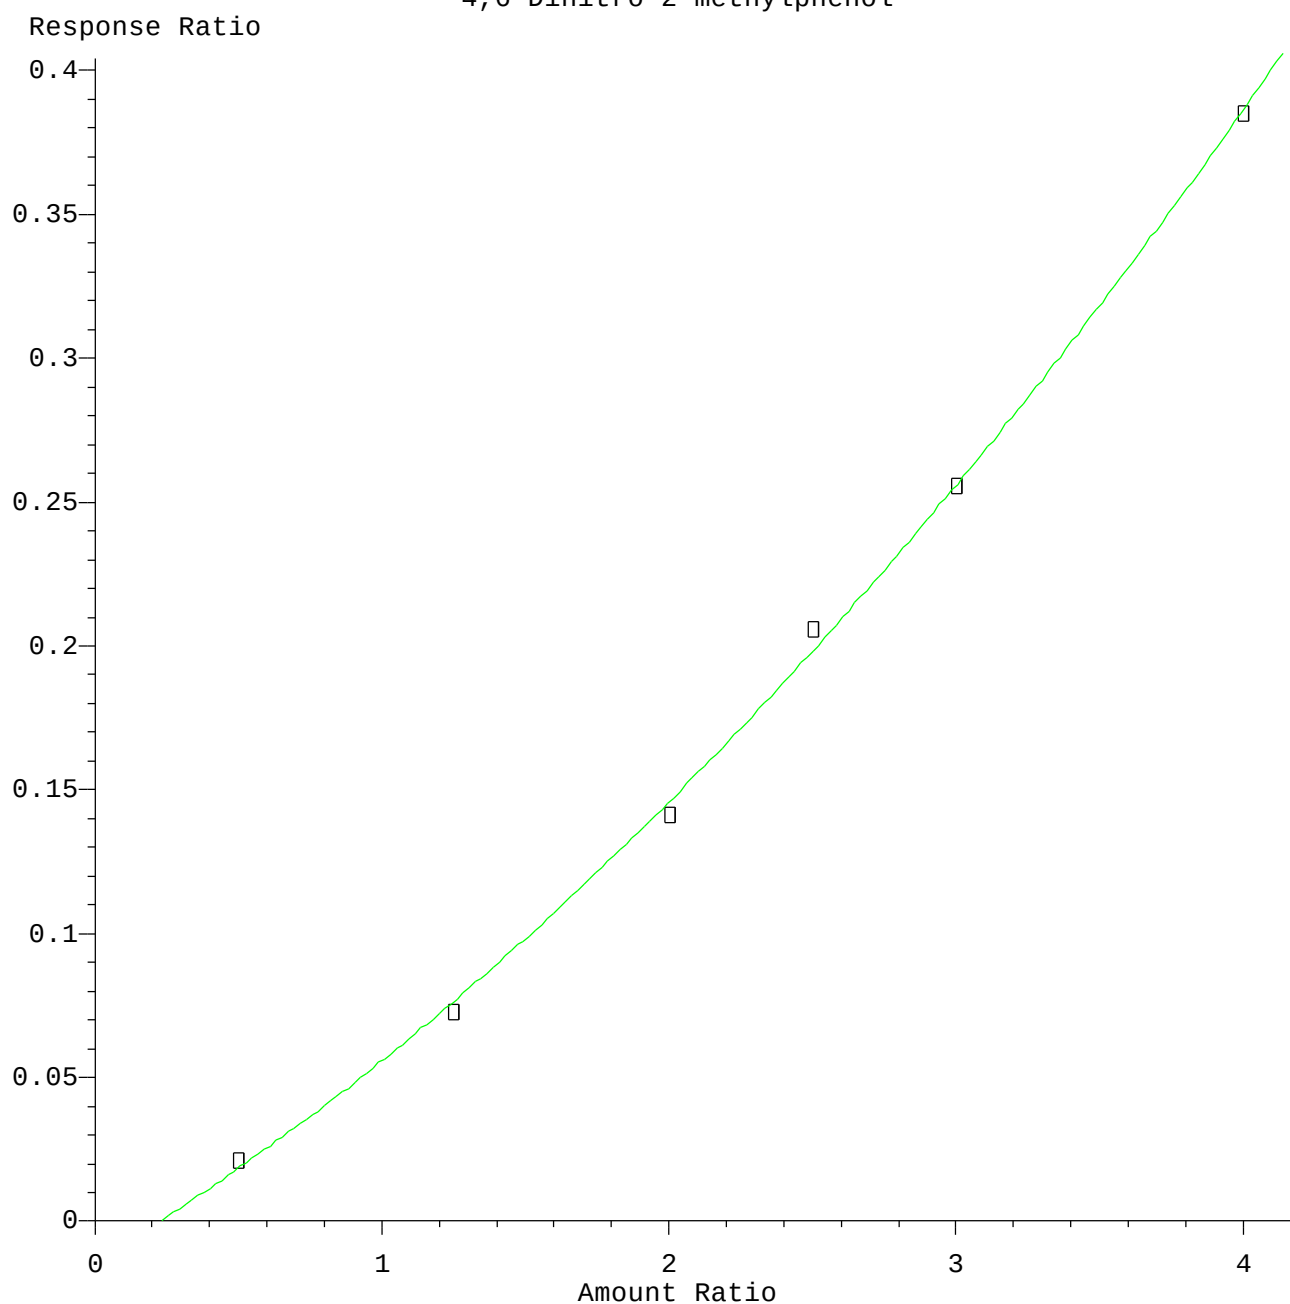

$R = 1.01e-002 A^2 + 5.96e-002 A - 1.40e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
Calibration Table Last Updated: Thu Aug 31 18:39:59 2017