
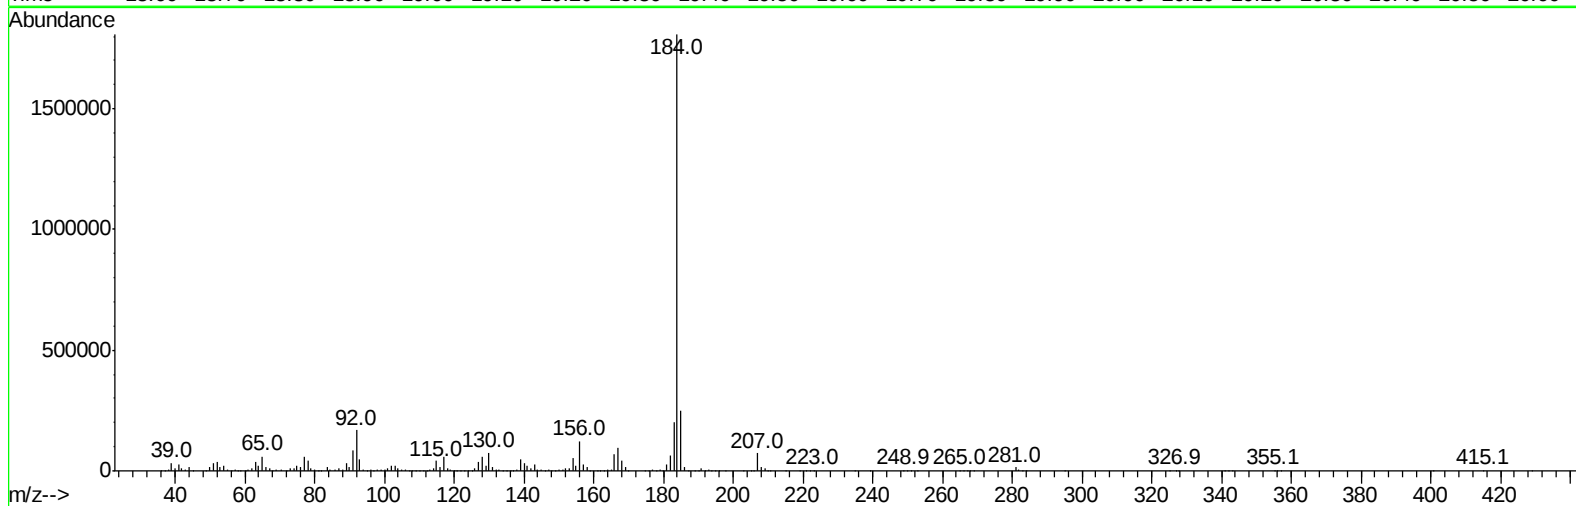


Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011366.D
Acq On : 31 Aug 2017 11:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:14:29 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

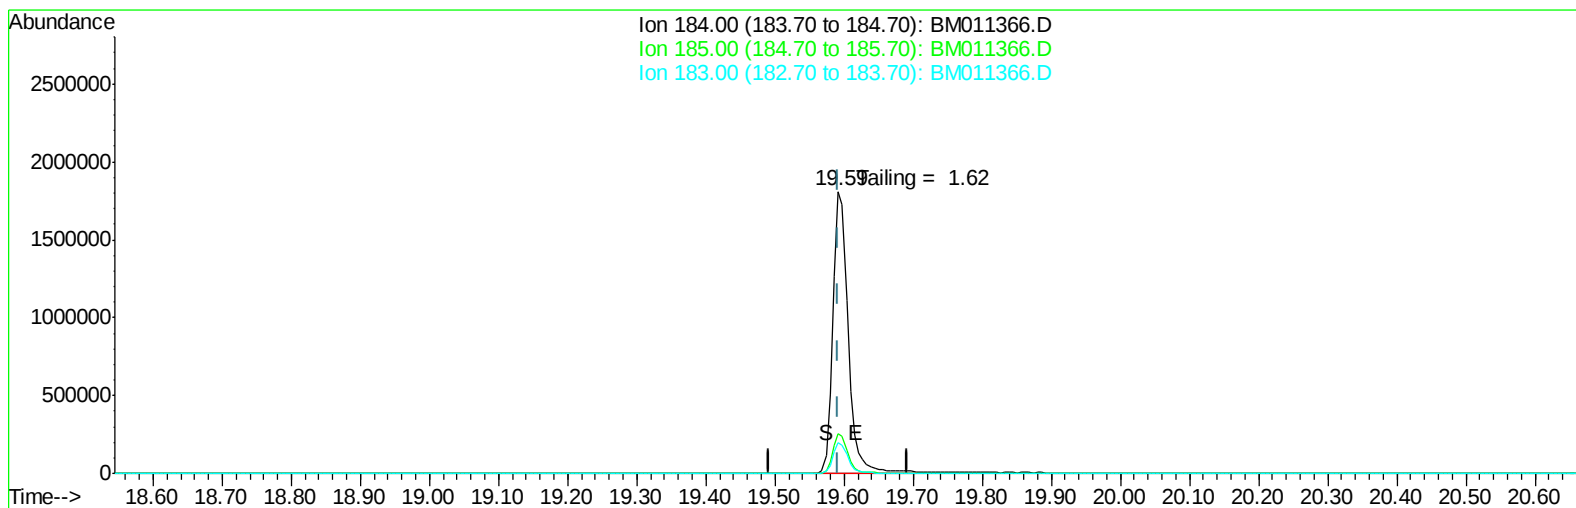

TIC: BM011366.D

(76) Benzidine



19.592min (-0.000) 29939.79ng

response 2740034

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.92
183.00	11.10	11.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011366.D
Acq On : 31 Aug 2017 11:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:14:29 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

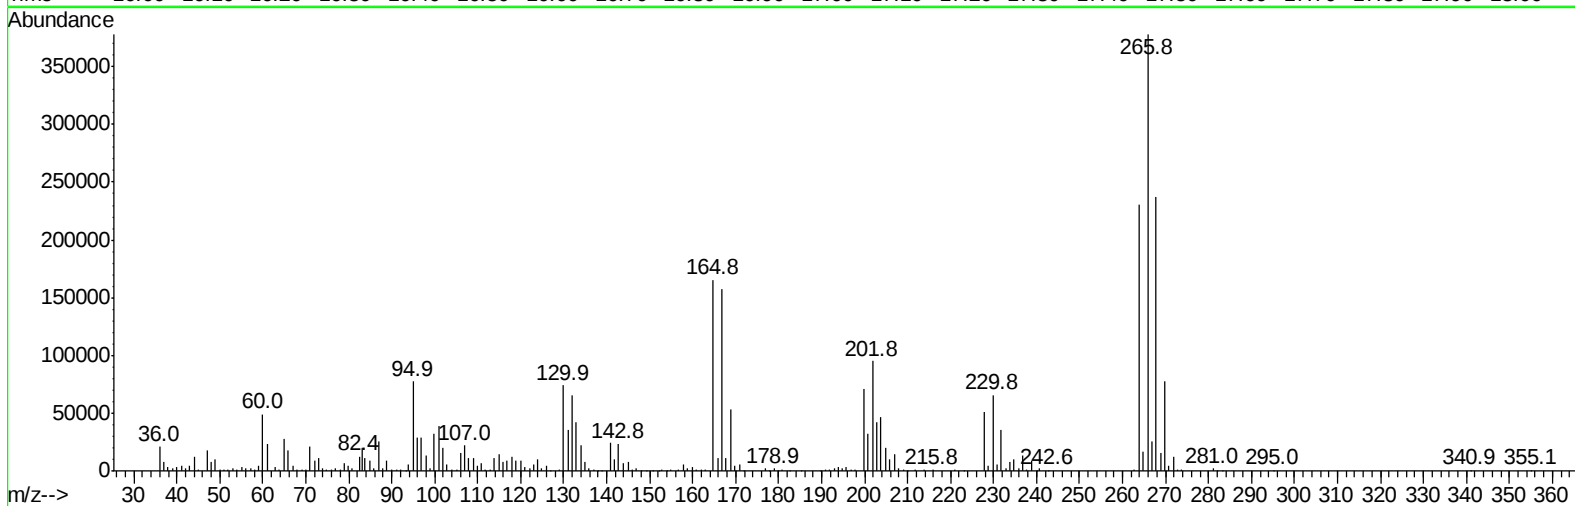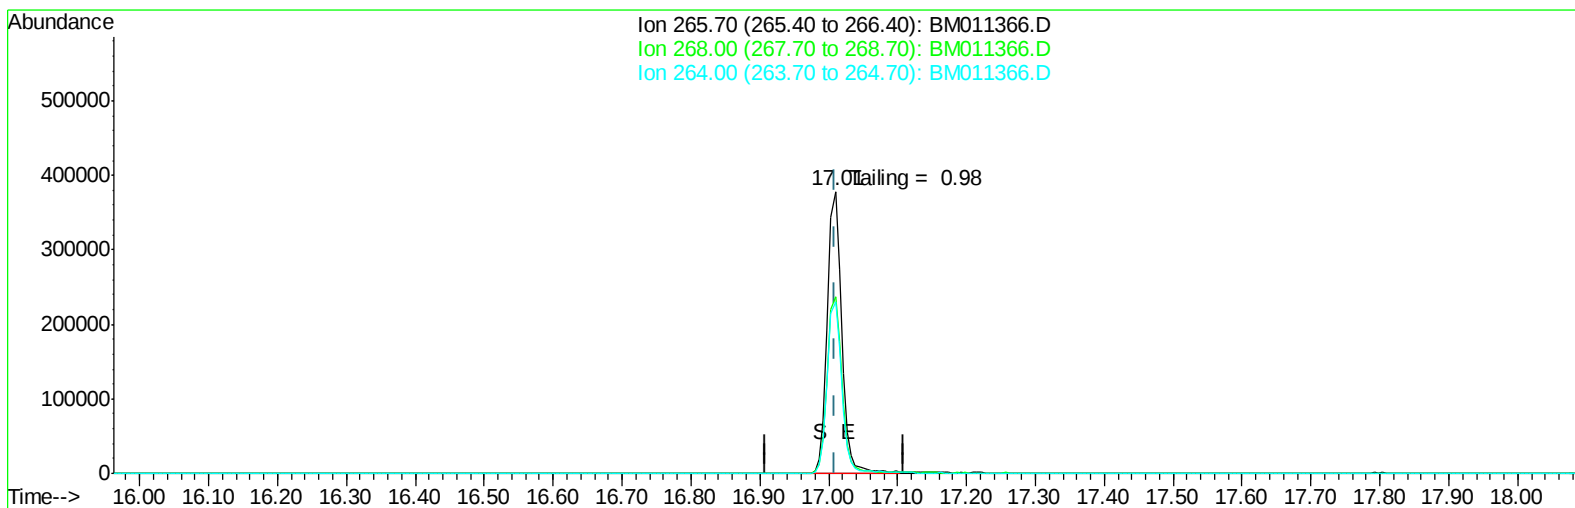

TIC: BM011366.D

(69) Pentachlorophenol (C)

17.009min (-0.000) 69805.59ng

response 544003

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.90
264.00	61.20	60.97
0.00	0.00	0.00