
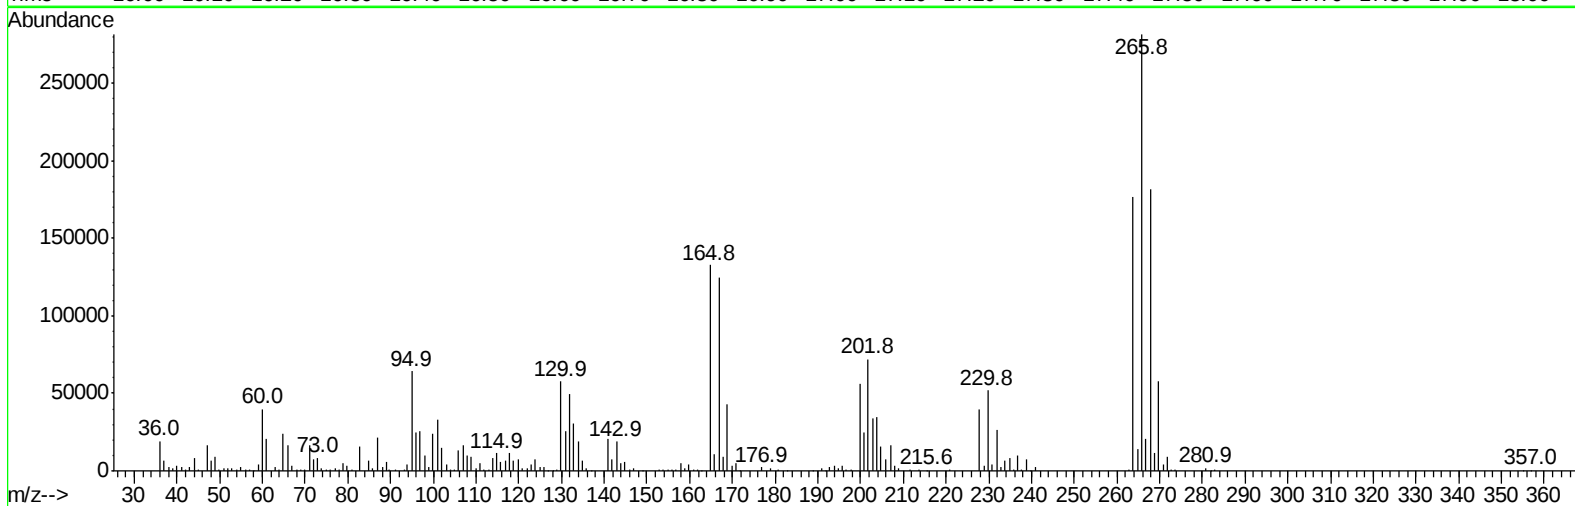


Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011375.D
Acq On : 31 Aug 2017 17:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:15:30 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

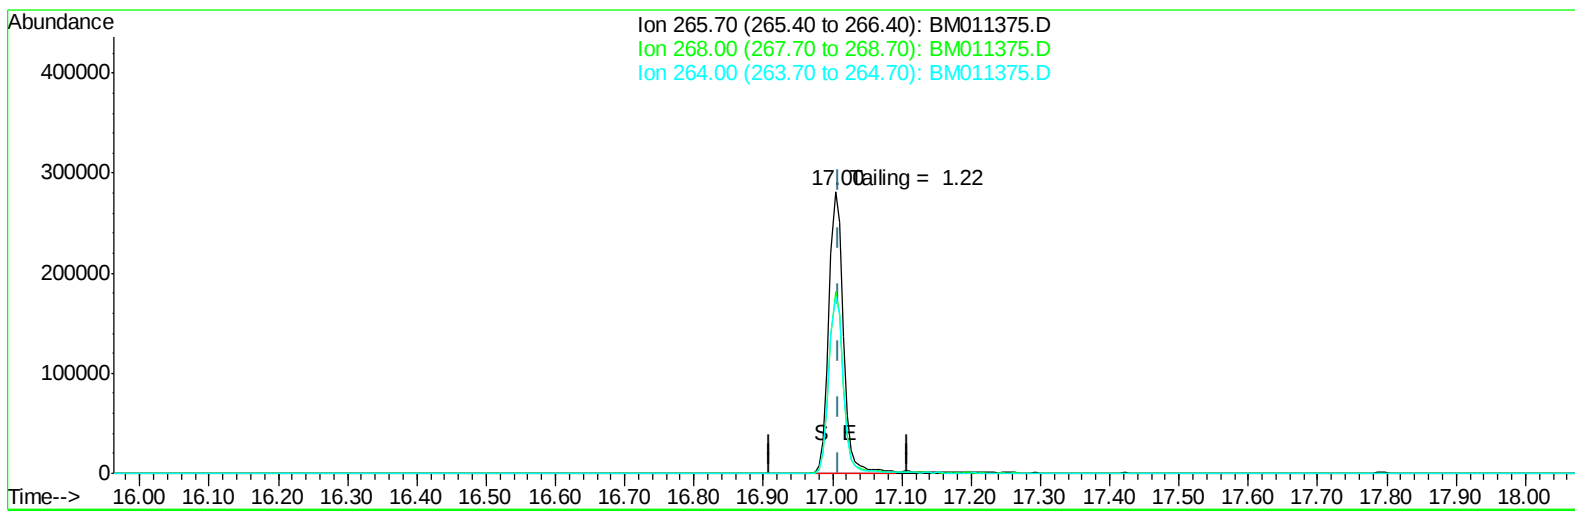

TIC: BM011375.D

(69) Pentachlorophenol (C)



17.004min (-0.006) 151927.93ng

response 407705

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.66
264.00	61.20	62.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
 Data File : BM011375.D
 Acq On : 31 Aug 2017 17:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:15:30 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 18:39:59 2017
 Response via : Initial Calibration

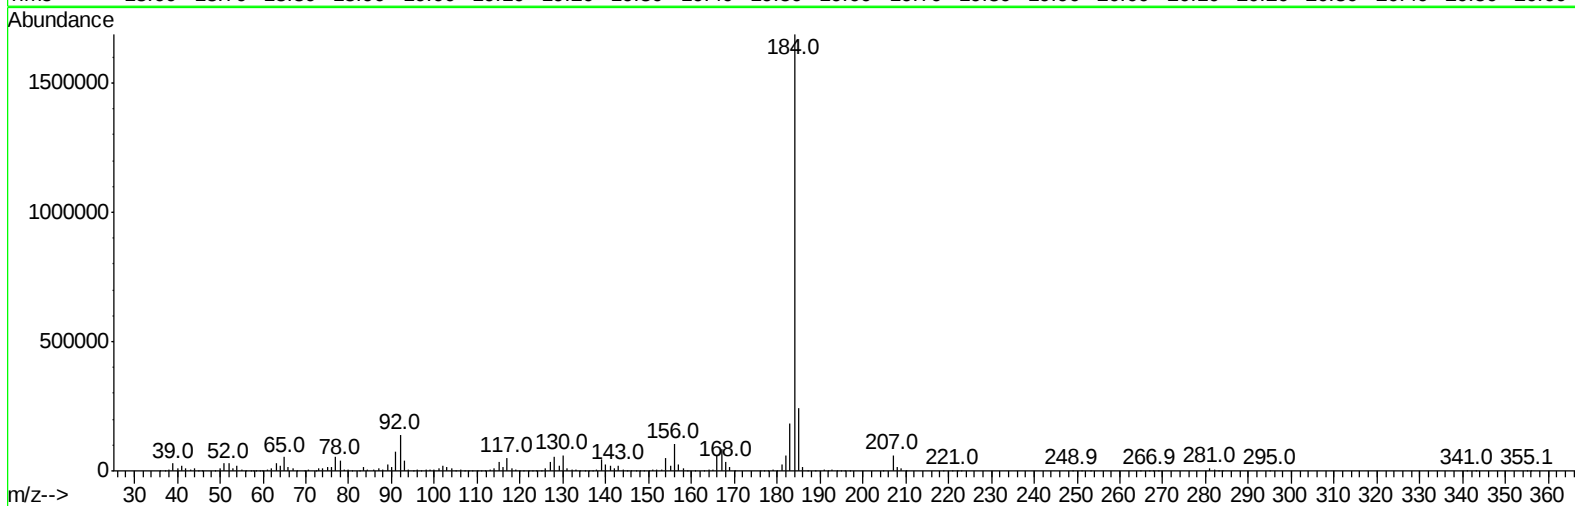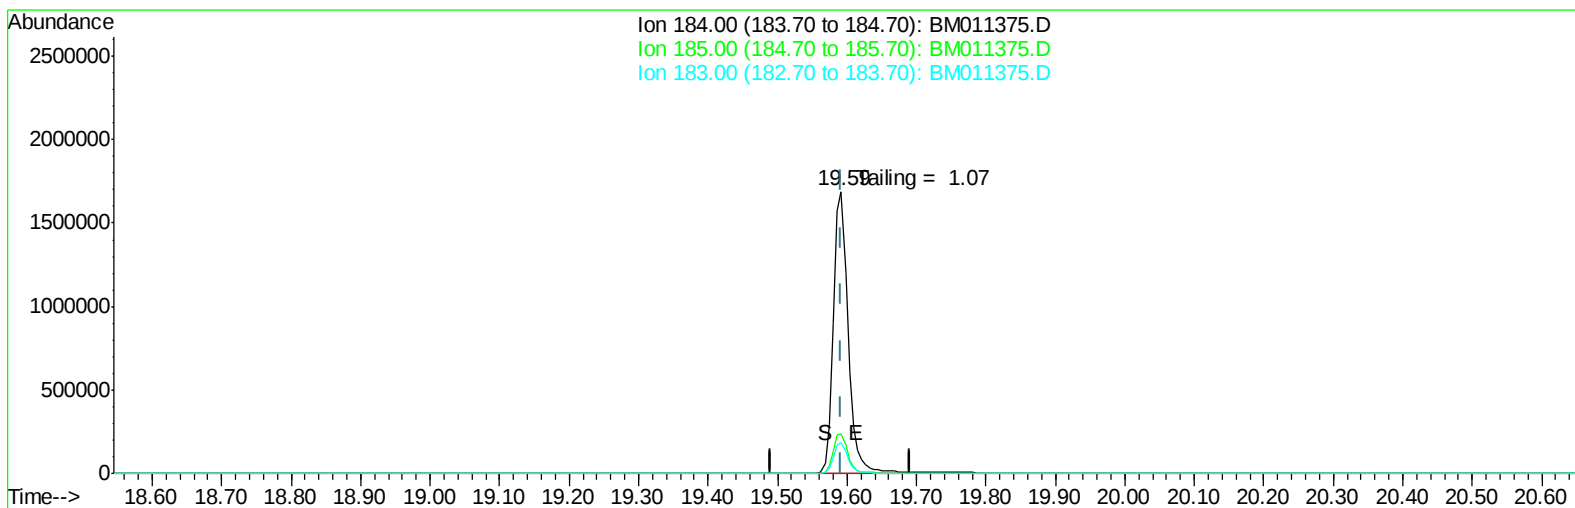

TIC: BM011375.D

(76) Benzidine

19.592min (+0.000) 115170.02ng

response 2466262

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.31
183.00	11.10	10.77
0.00	0.00	0.00