
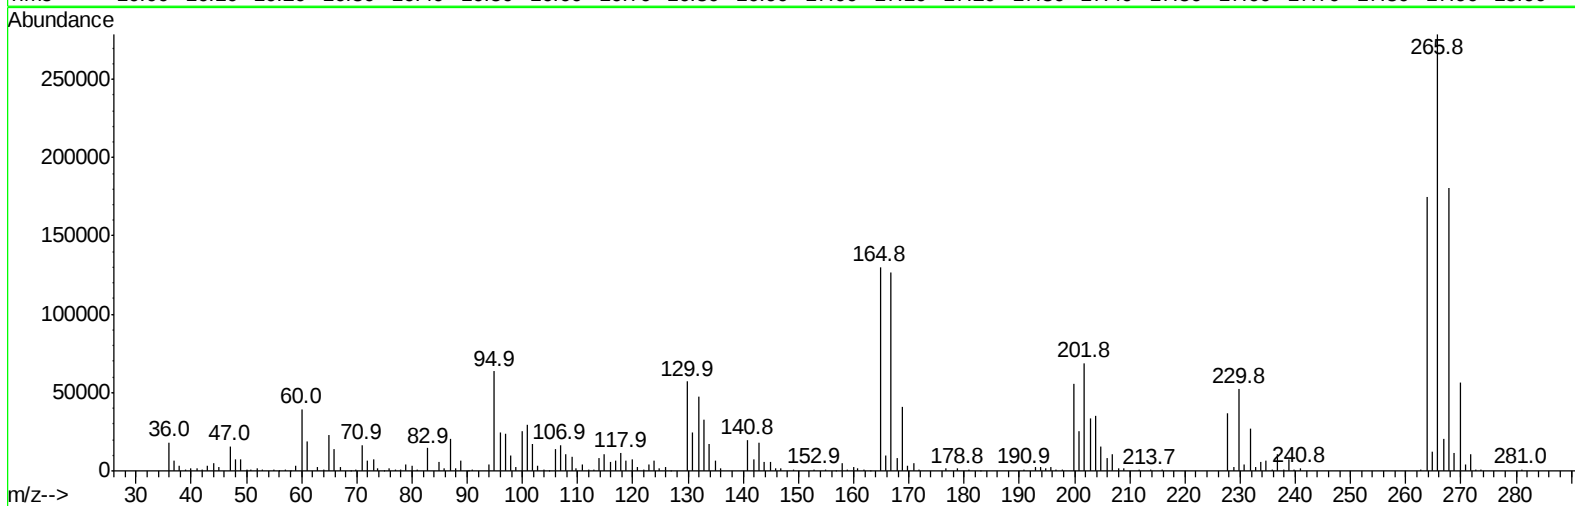


Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011395.D
Acq On : 01 Sep 2017 05:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:16:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

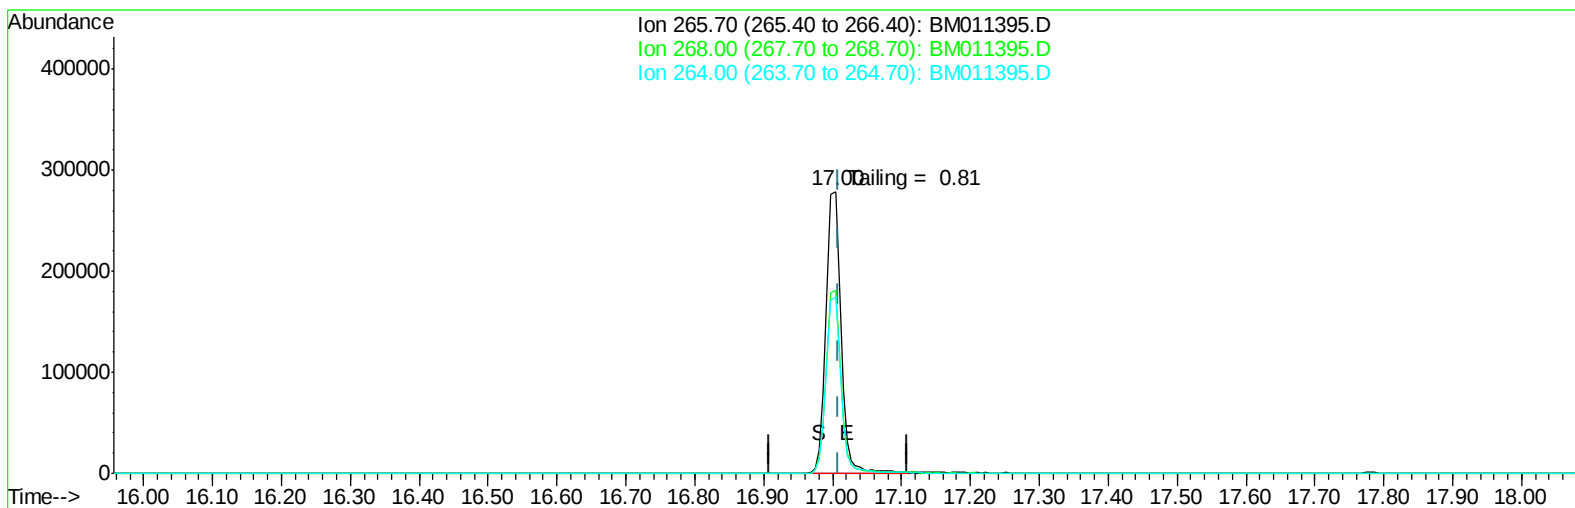

TIC: BM011395.D

(69) Pentachlorophenol (C)



17.004min (-0.006) 454796.73ng

response 419150

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.93
264.00	61.20	62.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011395.D
Acq On : 01 Sep 2017 05:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 09:16:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

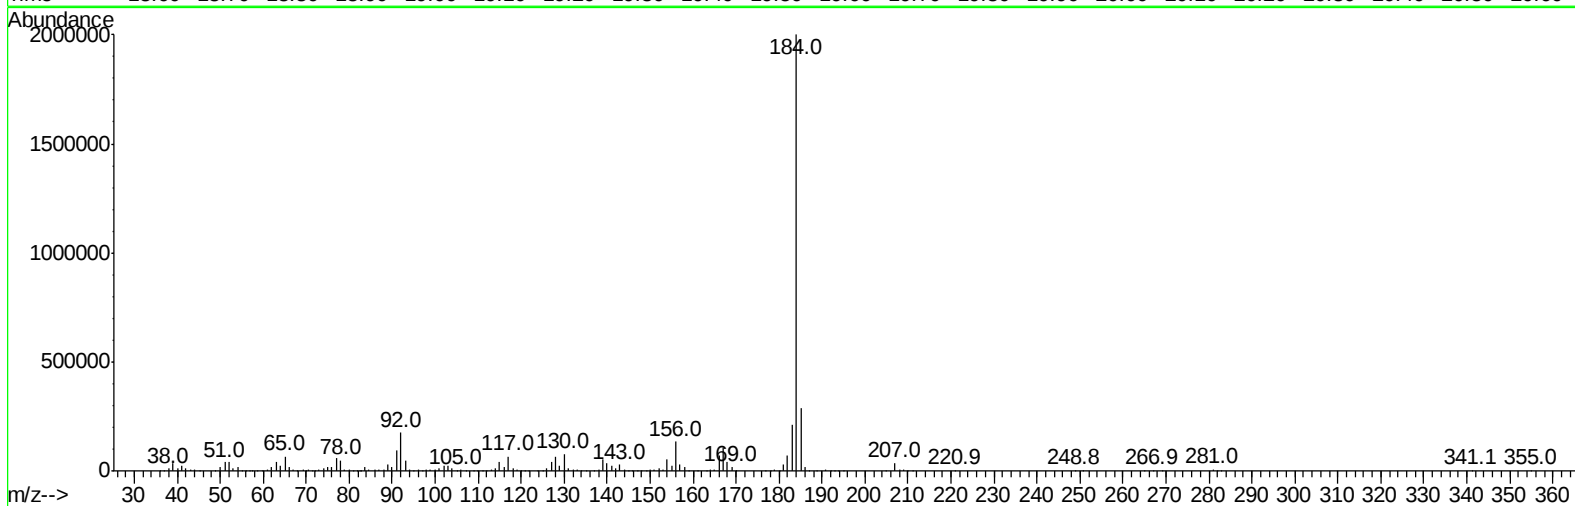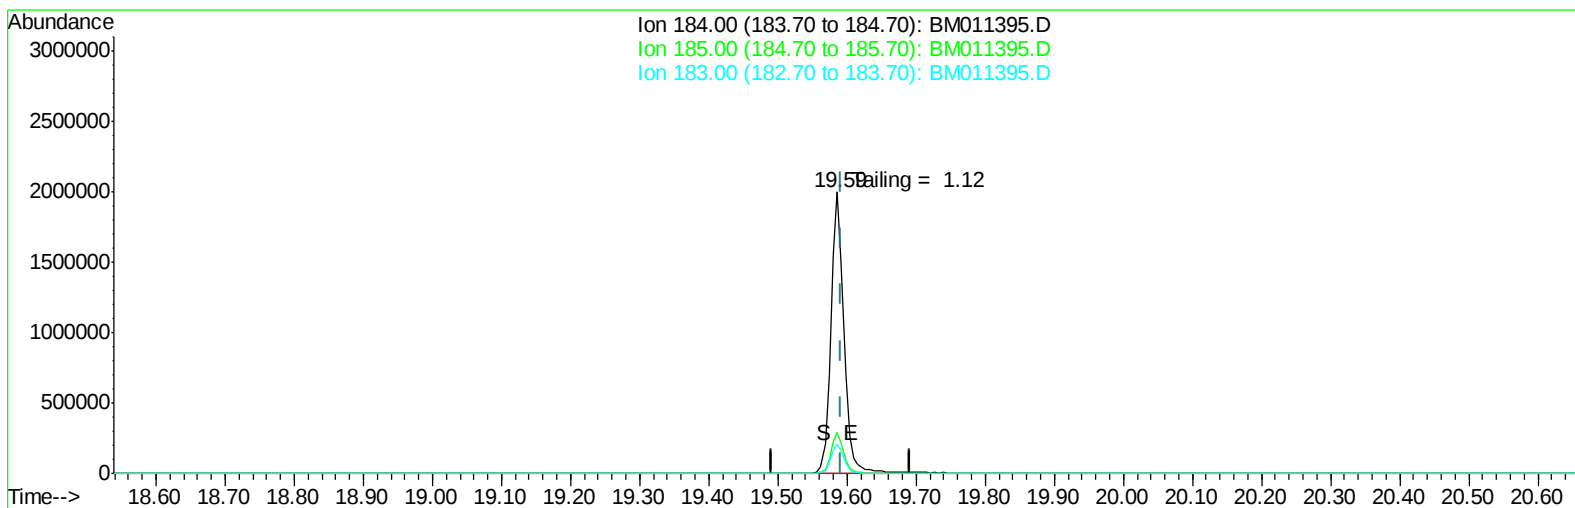

TIC: BM011395.D

(76) Benzidine

19.586min (-0.006) 116430.08ng

response 2582864

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.45
183.00	11.10	10.65
0.00	0.00	0.00