

Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
 Data File : BM011389.D
 Acq On : 01 Sep 2017 01:33
 Operator : SJ/JU
 Sample : I4963-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 3834-CC5

Quant Time: Sep 01 07:57:26 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 18:39:59 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	502379	20.00	ng	0.00
21) Naphthalene-d8	10.80	136	2208489	20.00	ng	0.00
38) Acenaphthene-d10	14.62	164	1253702	20.00	ng	0.00
63) Phenanthrene-d10	17.36	188	2828421	20.00	ng	0.00
75) Chrysene-d12	21.52	240	3266644	20.00	ng	-0.01
86) Perylene-d12	23.90	264	2984706	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	1609693	53.93	ng	0.00
7) Phenol-d6	7.13	99	1306692	31.57	ng	0.00
23) Nitrobenzene-d5	9.15	82	2962590	88.40	ng	0.00
41) 2,4,6-Tribromophenol	16.10	330	1772255	122.18	ng	0.00
44) 2-Fluorobiphenyl	13.25	172	7550250	86.81	ng	0.00
78) Terphenyl-d14	19.97	244	10213443	77.58	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM083117\
Data File : BM011389.D
Acq On : 01 Sep 2017 01:33
Operator : SJ/JU
Sample : I4963-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
3834-CC5

Quant Time: Sep 01 07:57:26 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

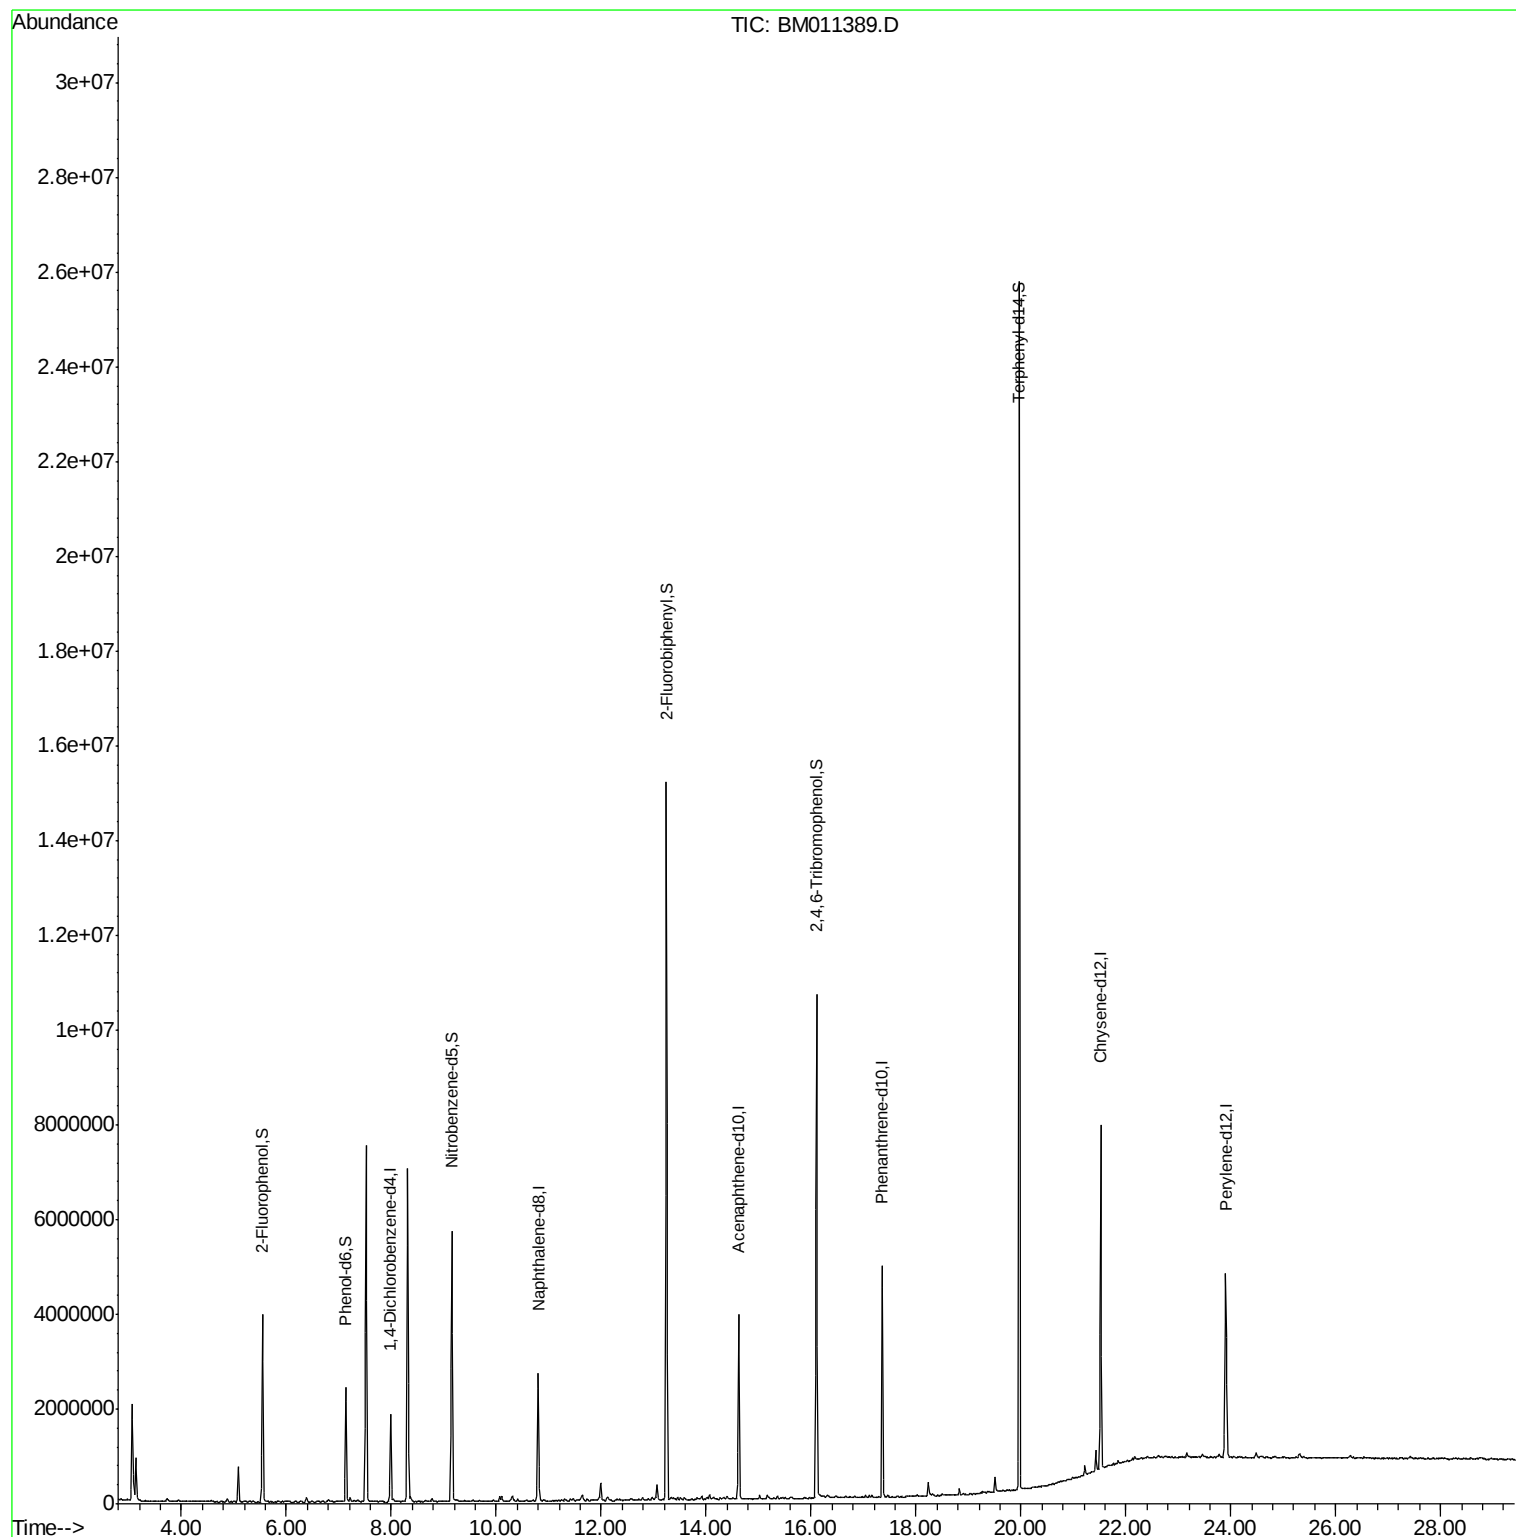




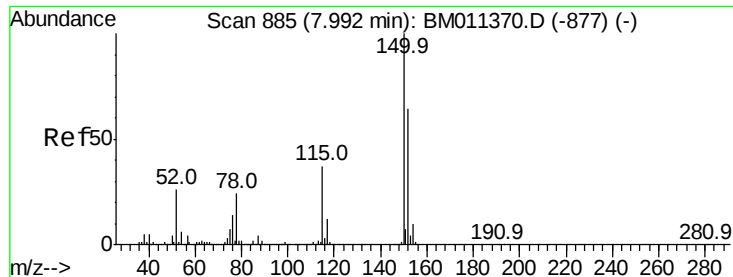


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 884
Delta R.T. -0.01 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33

Instrument :
BNA_M
ClientSampleId :
3834-CC5




Tot Ion:152 Resp: 502379
Ion Ratio Lower Upper
152 100
150 156.8 119.5 179.3
115 58.3 43.0 64.4

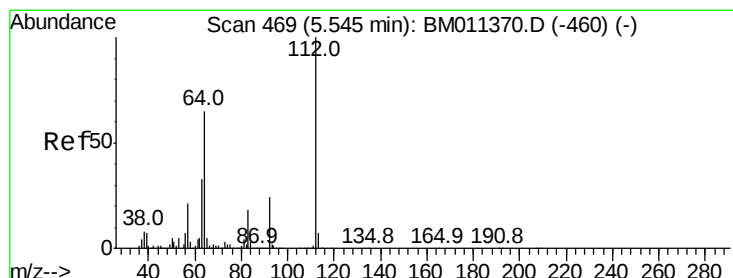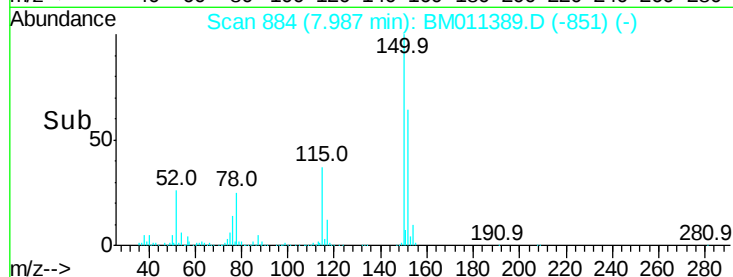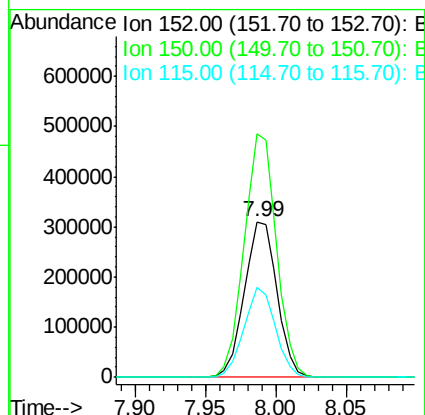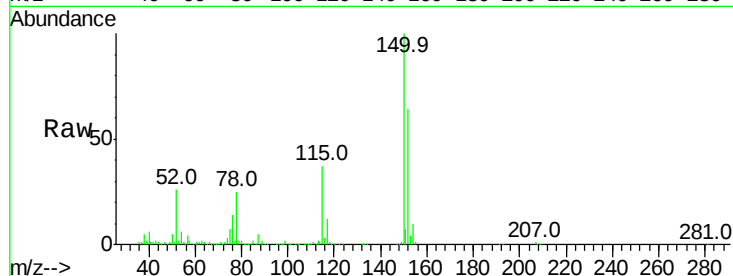


#5

2-Fluorophenol
Concen: 53.934 ng
RT: 5.55 min Scan# 469
Delta R.T. 0.00 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33

Tgt Ion:112 Resp: 1609693
Ion Ratio Lower Upper
112 100
64 65.5 38.6 57.8#
63 33.7 19.3 28.9#

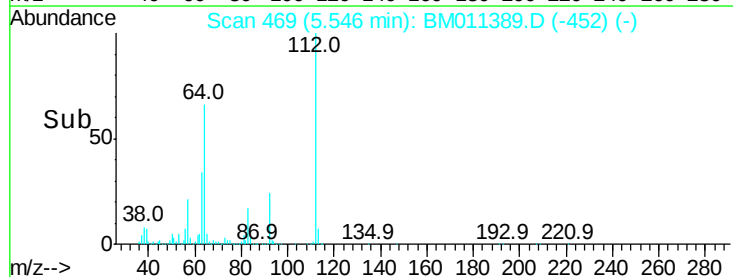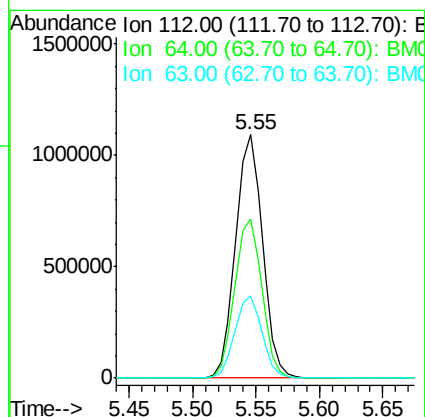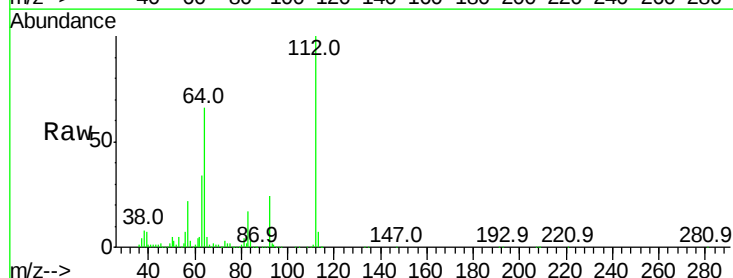

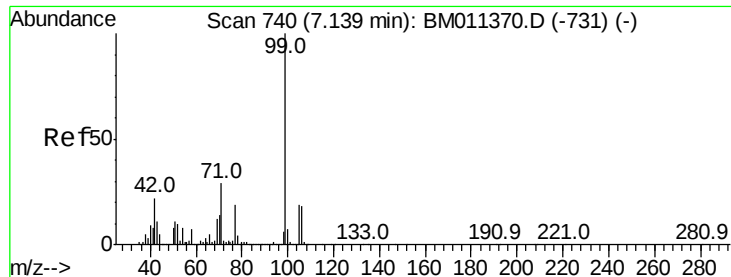

#7

Phenol-d6

Concen: 31.575 ng

RT: 7.13 min Scan# 739

Delta R.T. -0.01 min

Lab File: BM011389.D

Acq: 01 Sep 2017 01:33

Instrument :





BNA_M

ClientSampleId :

3834-CC5

Tot Ion: 99 Resp: 1306692

Ion	Ratio	Lower	Upper
99	100		
42	22.1	11.0	16.4#
71	28.0	23.4	35.2

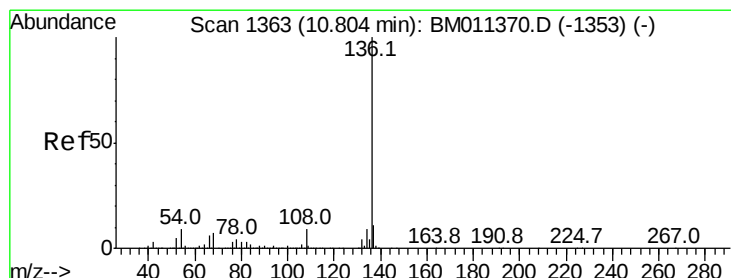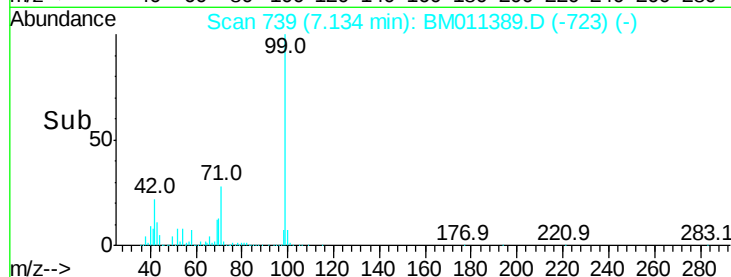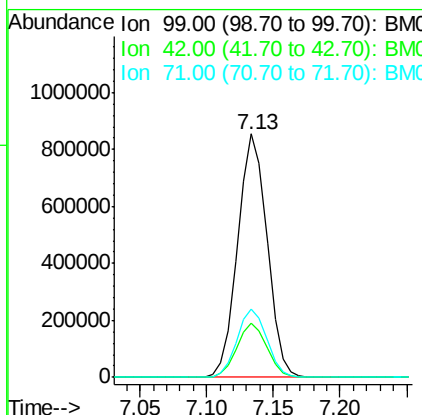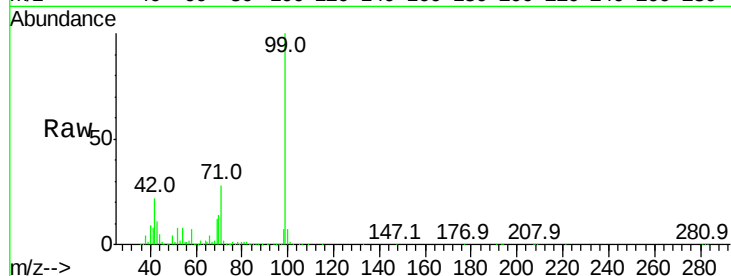

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.80 min Scan# 1362




Delta R.T. -0.01 min


Lab File: BM011389.D

Acq: 01 Sep 2017 01:33

Tgt Ion: 136 Resp: 2208489

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	9.3	4.6	6.8#
68	7.4	3.7	5.5#


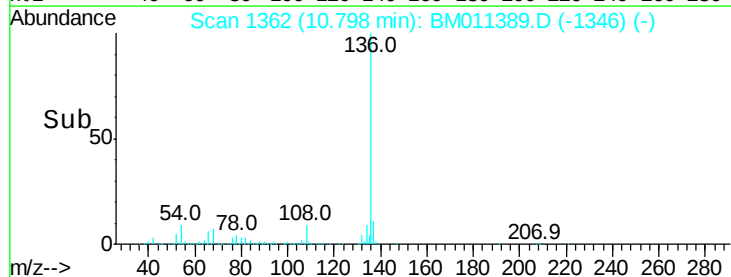
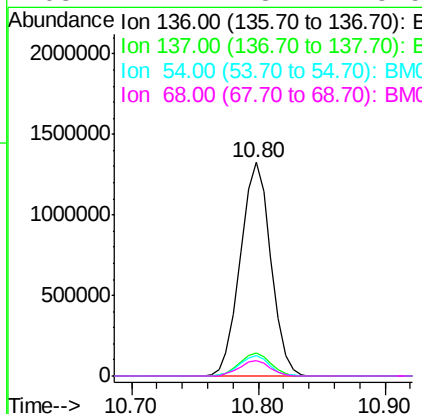
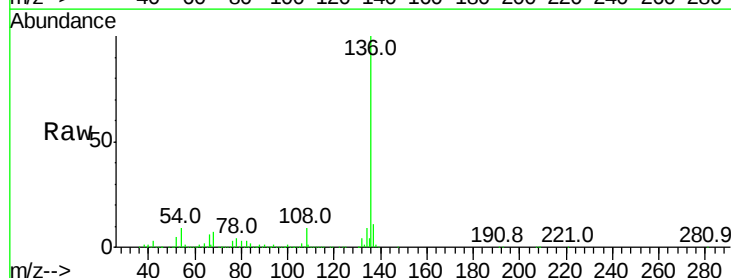


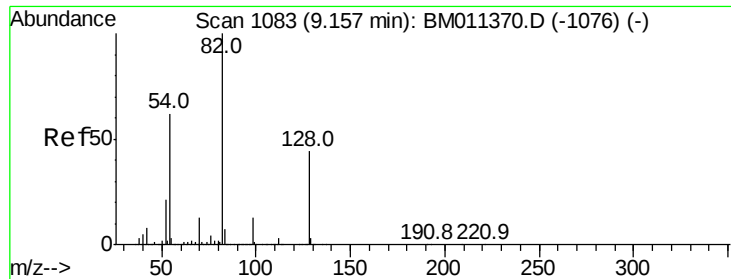

#23
Nitrobenzene-d5
Concen: 88.400 ng
RT: 9.15 min Scan# 1082
Delta R.T. -0.01 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33




Instrument :
BNA_M
ClientSampleId :
3834-CC5


Tot Ion: 82 Resp: 2962590
Ion Ratio Lower Upper
82 100
128 44.2 32.8 49.2
54 62.7 40.6 60.8#

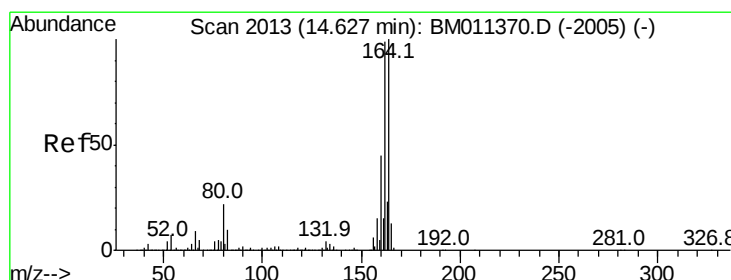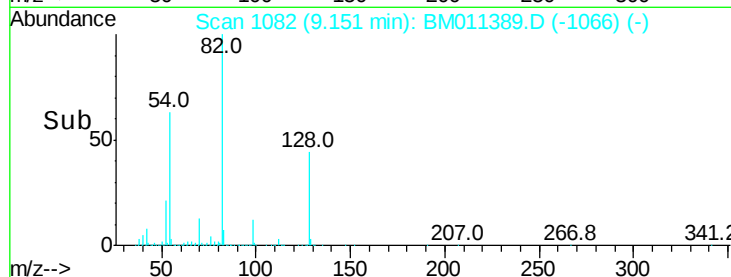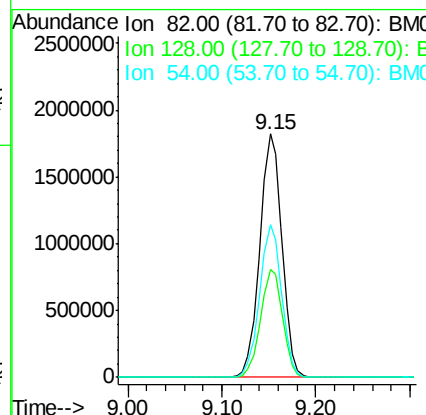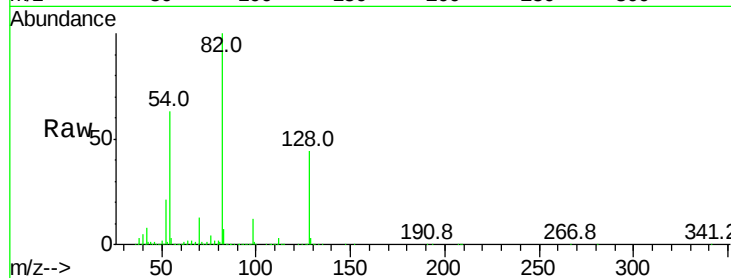

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.62 min Scan# 2012
Delta R.T. -0.01 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33

Tgt Ion: 164 Resp: 1253702
Ion Ratio Lower Upper
164 100
162 99.7 82.4 123.6
160 44.8 35.8 53.6

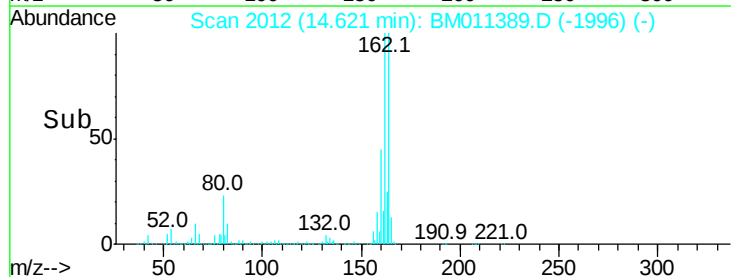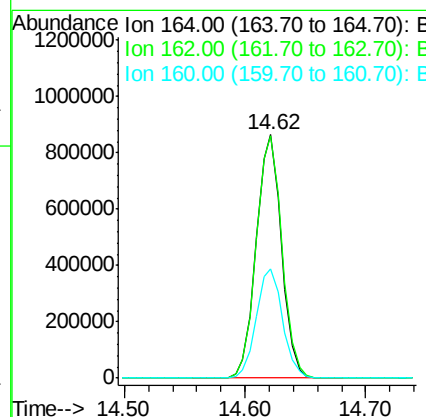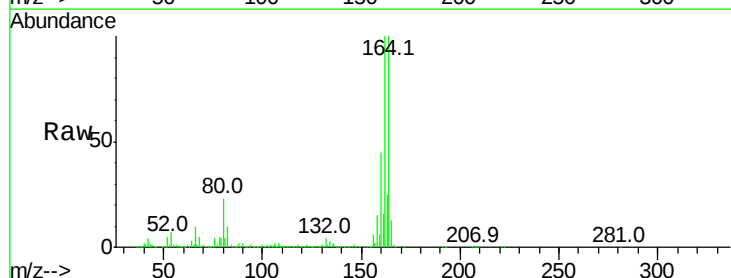


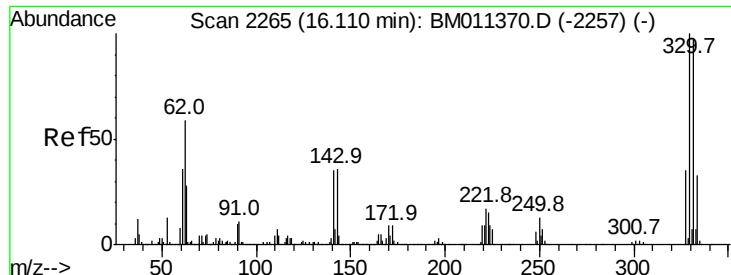




#41
 2,4,6-Tribromophenol
 Concen: 122.184 ng
 RT: 16.10 min Scan# 2264
 Delta R.T. -0.01 min
 Lab File: BM011389.D
 Acq: 01 Sep 2017 01:33

Instrument :
 BNA_M
 ClientSampleId :
 3834-CC5

Tot Ion:330 Resp: 1772255
 Ion Ratio Lower Upper
 330 100
 332 96.4 0.0 0.0#
 141 37.3 0.0 0.0#

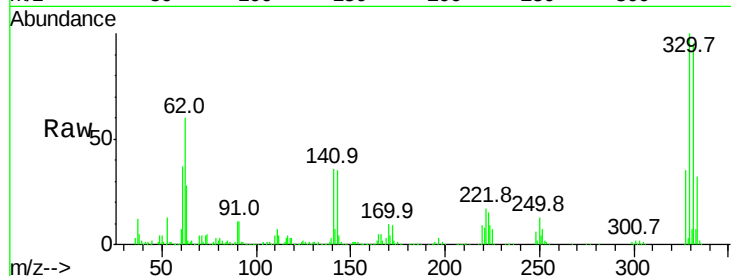


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

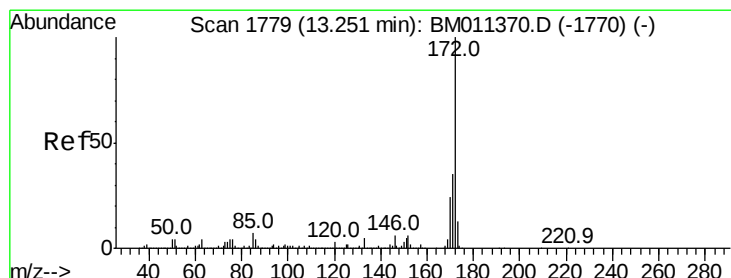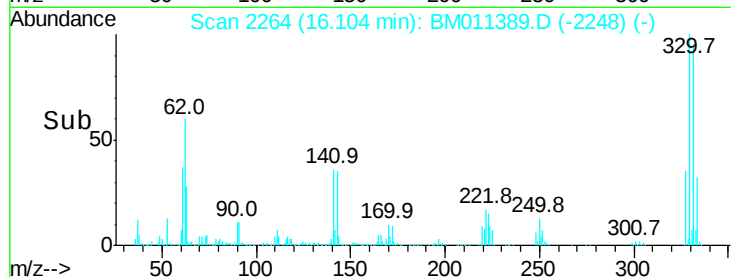
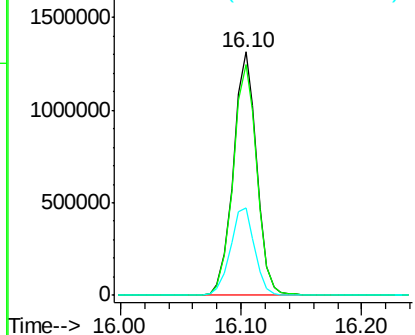


#44
 2-Fluorobiphenyl
 Concen: 86.811 ng
 RT: 13.25 min Scan# 1778
 Delta R.T. -0.01 min
 Lab File: BM011389.D
 Acq: 01 Sep 2017 01:33

Tgt Ion:172 Resp: 7550250
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.5 42.7
 170 24.3 18.8 28.2

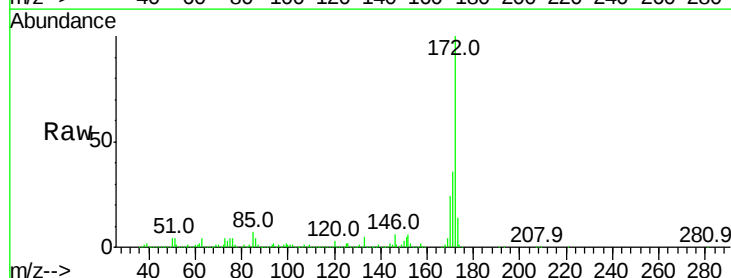

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

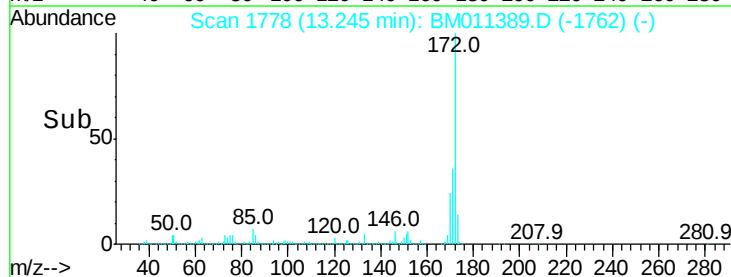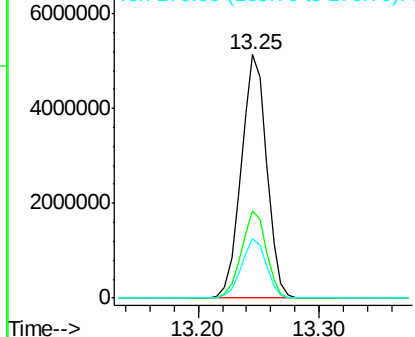







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.36 min Scan# 2477
Delta R.T. -0.01 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33

Instrument :
BNA_M
ClientSampled :
3834-CC5

Tot Ion:188 Resp: 2828421
Ion Ratio Lower Upper
188 100
94 10.6 8.7 13.1
80 12.0 9.3 13.9

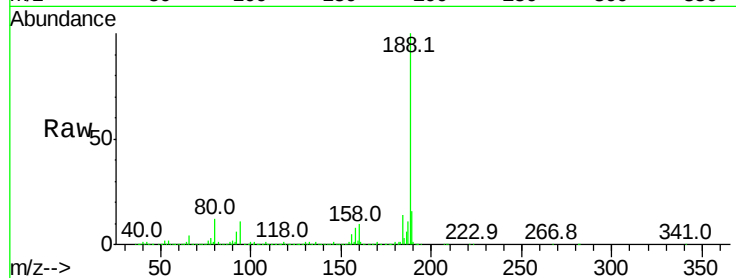


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

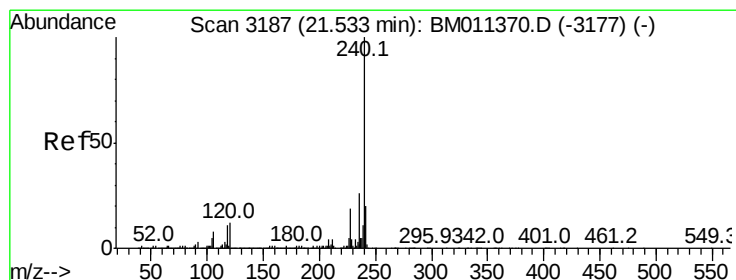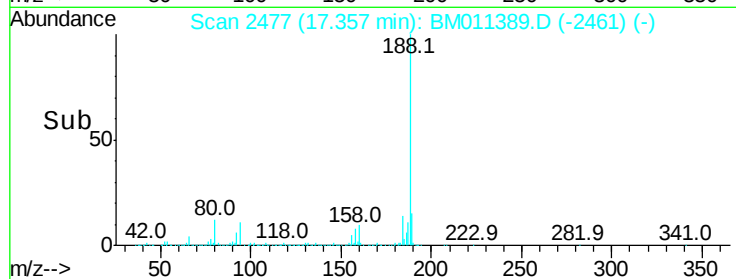
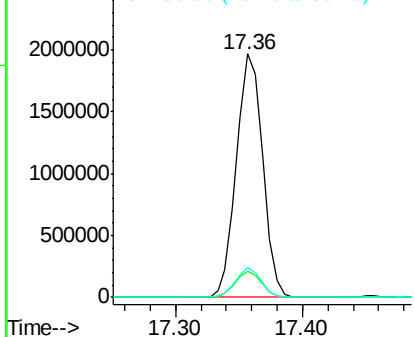



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.52 min Scan# 3185
Delta R.T. -0.01 min
Lab File: BM011389.D
Acq: 01 Sep 2017 01:33

Tgt Ion:240 Resp: 3266644
Ion Ratio Lower Upper
240 100
120 12.1 8.2 12.2
236 25.7 20.0 30.0

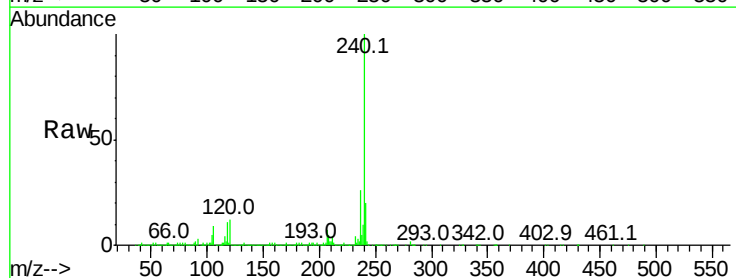

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



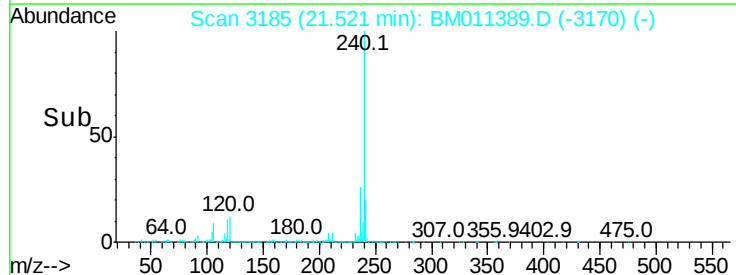
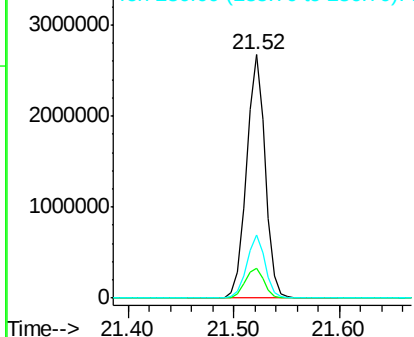


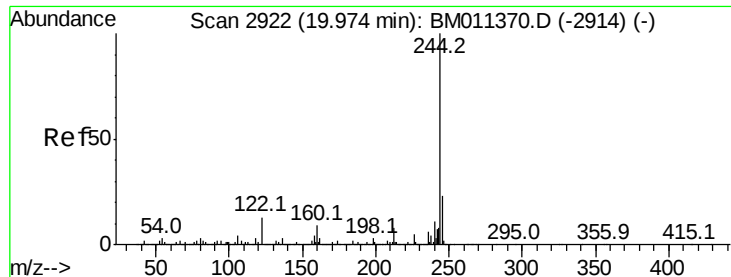

#78
 Terphenyl-d14
 Concen: 77.577 ng
 RT: 19.97 min Scan# 2921
 Delta R.T. -0.01 min
 Lab File: BM011389.D
 Acq: 01 Sep 2017 01:33

Instrument :
 BNA_M
 ClientSampled :
 3834-CC5

Tot Ion:244 Resp:10213443
 Ion Ratio Lower Upper
 244 100
 212 7.9 4.9 7.3#
 122 12.6 6.2 9.4#

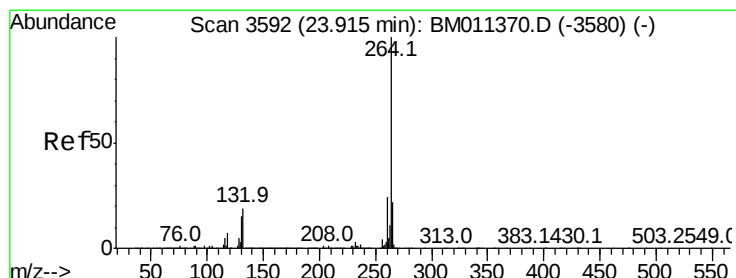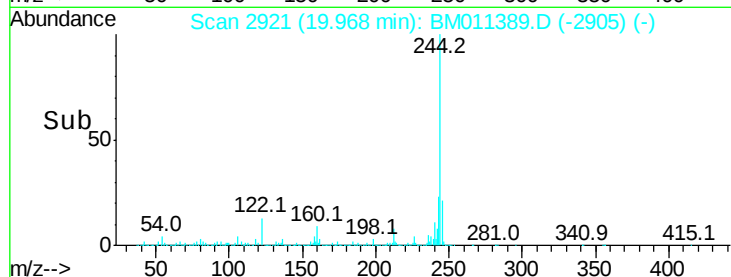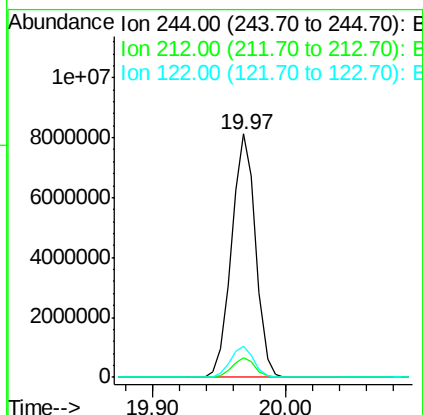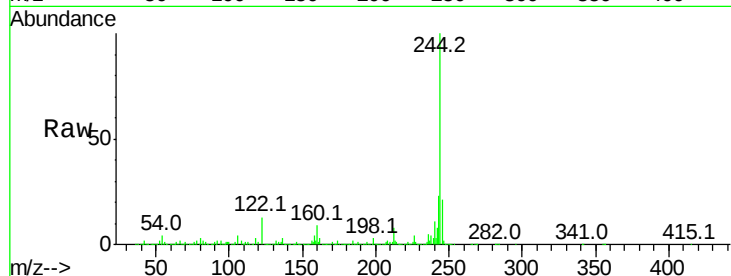

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.90 min Scan# 3590
 Delta R.T. -0.01 min
 Lab File: BM011389.D
 Acq: 01 Sep 2017 01:33

Tgt Ion:264 Resp: 2984706
 Ion Ratio Lower Upper
 264 100
 260 23.0 18.6 27.8
 265 21.5 17.3 25.9

