


Data Path : Z:\HPCHEM1\BNA M\Data\BM083117\
 Data File : BM011375.D
 Acq On : 31 Aug 2017 17:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

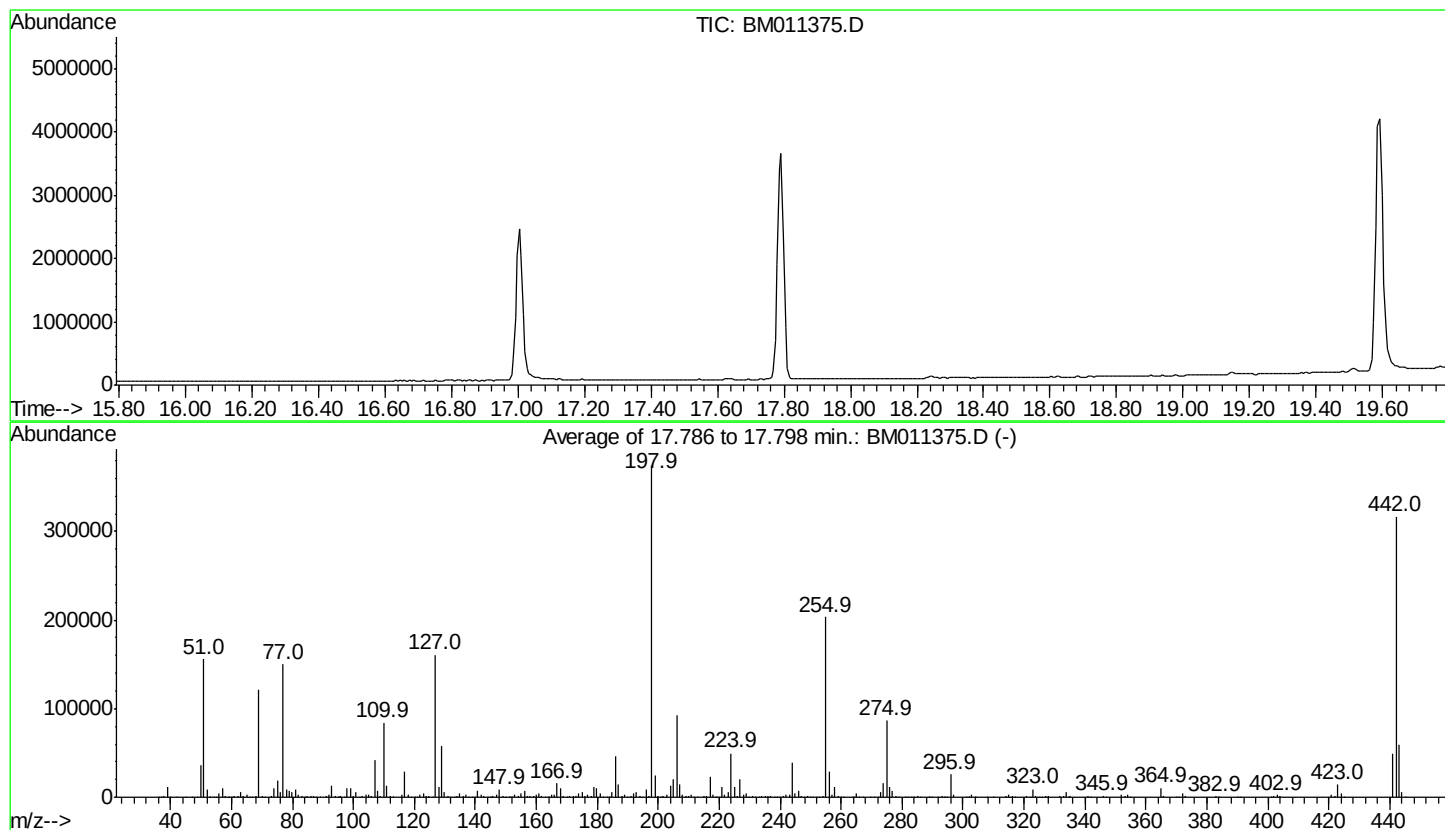

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	155923	PASS
68	69	0.00	2	1.3	1613	PASS
69	198	0.00	100	32.3	120812	PASS
70	69	0.00	2	0.7	874	PASS
127	198	10	80	43.0	160944	PASS
197	198	0.00	2	0.3	1214	PASS
198	198	100	100	100.0	374442	PASS
199	198	5	9	6.7	25112	PASS
275	198	10	60	23.1	86405	PASS
365	198	1	100	2.7	10224	PASS
441	443	0.01	100	81.9	48946	PASS
442	198	50	100	84.7	317120	PASS
443	442	15	24	18.8	59776	PASS