


Data Path : Z:\HPCHEM1\BNA M\Data\BM083117\
 Data File : BM011395.D
 Acq On : 01 Sep 2017 05:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

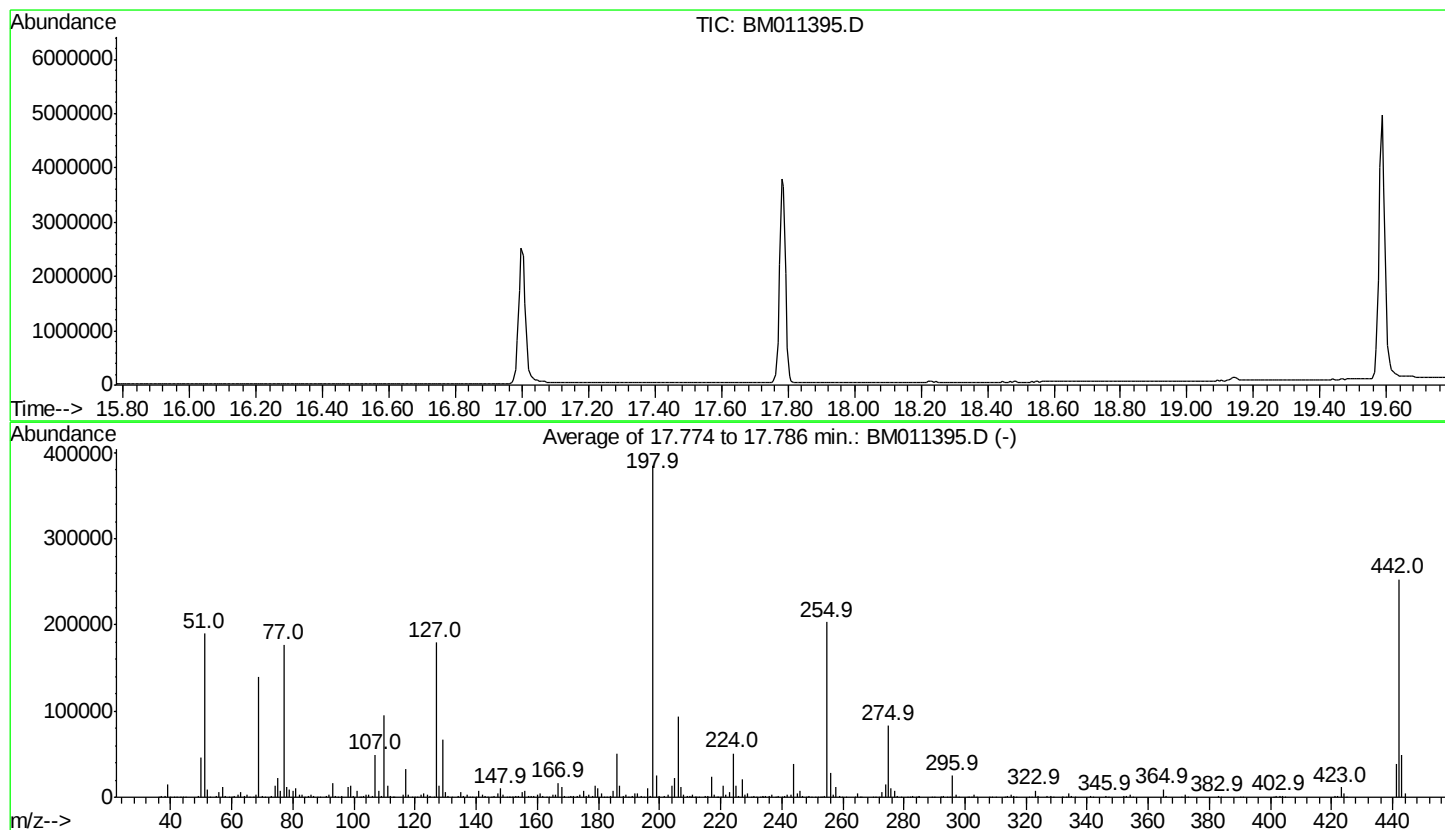

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	189899	PASS
68	69	0.00	2	1.6	2293	PASS
69	198	0.00	100	36.5	140373	PASS
70	69	0.00	2	0.8	1108	PASS
127	198	10	80	46.6	179221	PASS
197	198	0.00	2	0.4	1524	PASS
198	198	100	100	100.0	385002	PASS
199	198	5	9	6.7	25920	PASS
275	198	10	60	21.5	82610	PASS
365	198	1	100	2.5	9652	PASS
441	443	0.01	100	80.6	39296	PASS
442	198	50	100	65.7	253128	PASS
443	442	15	24	19.3	48762	PASS