
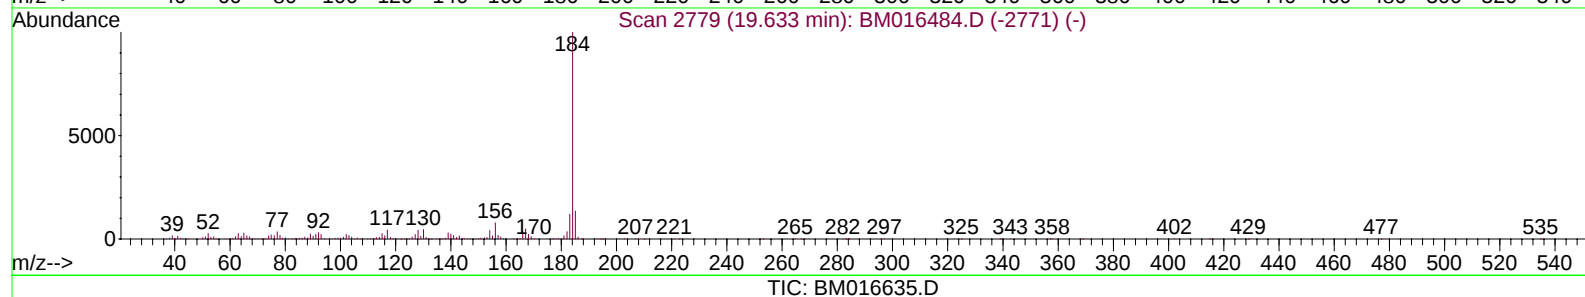
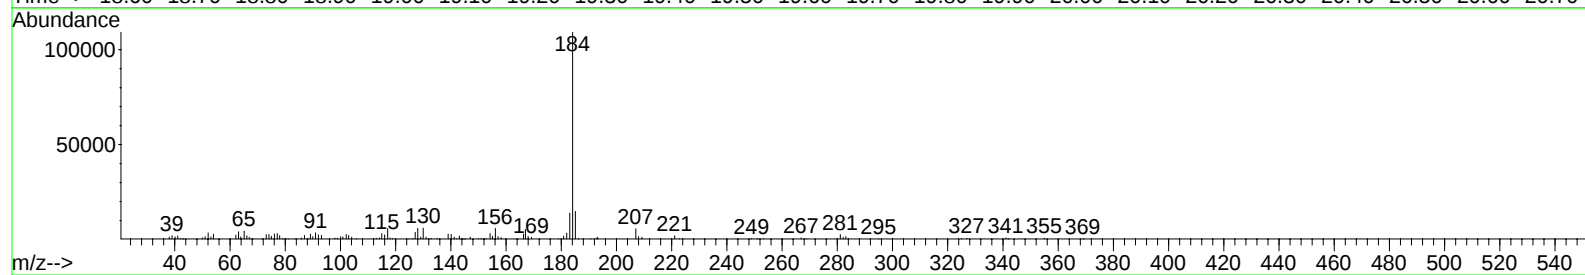


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM083118\
Data File : BM016635.D
Acq On : 31 Aug 2018 13:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 18:58:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

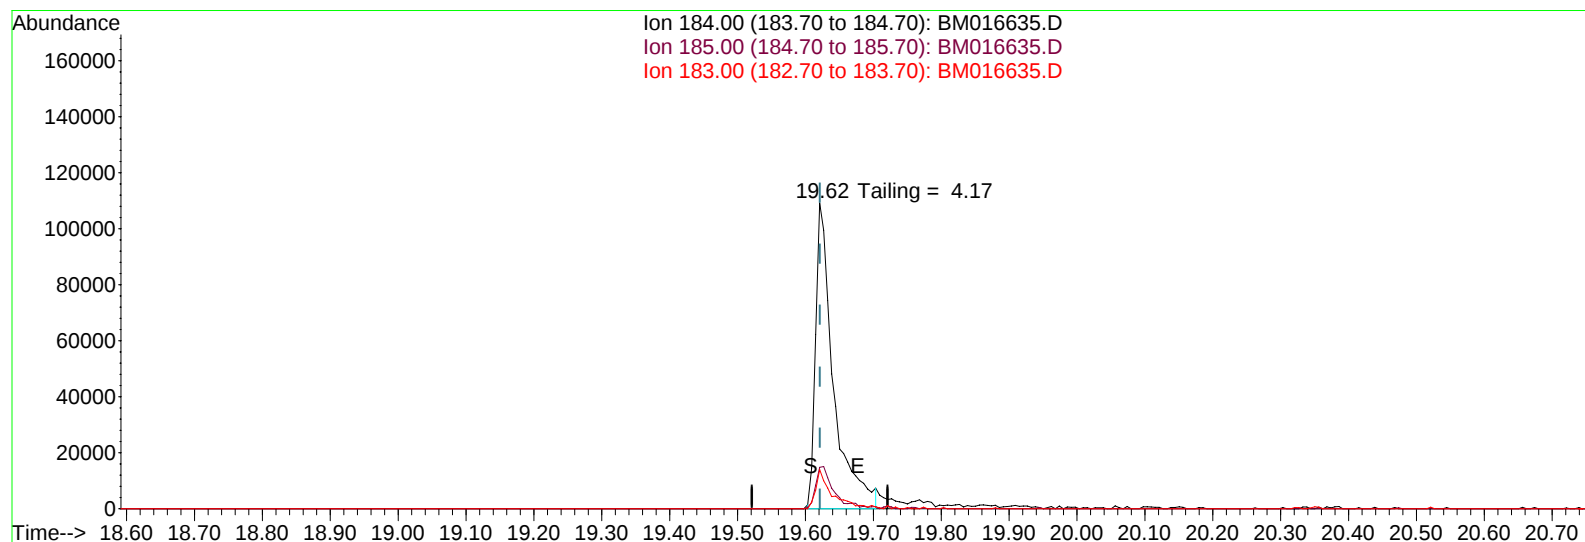

(76) Benzidine




19.621min (-0.000) 72586.00ng

response 209386

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.58
183.00	11.10	12.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM083118\
Data File : BM016635.D
Acq On : 31 Aug 2018 13:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 18:58:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

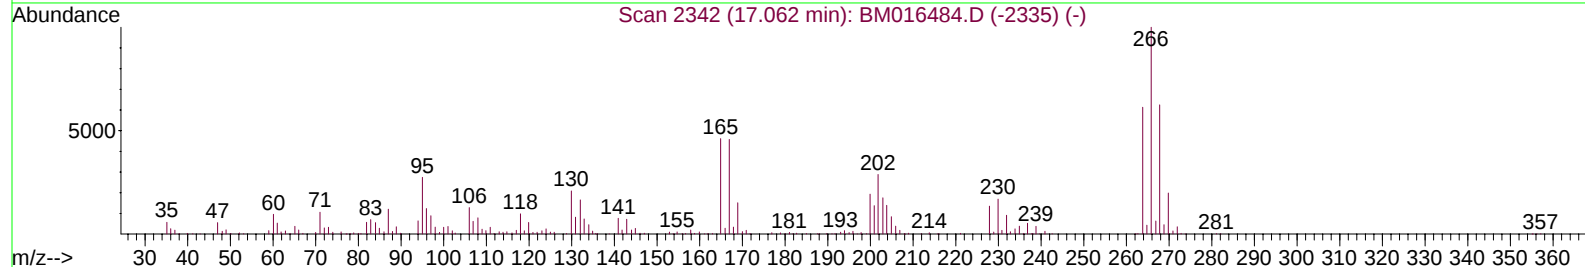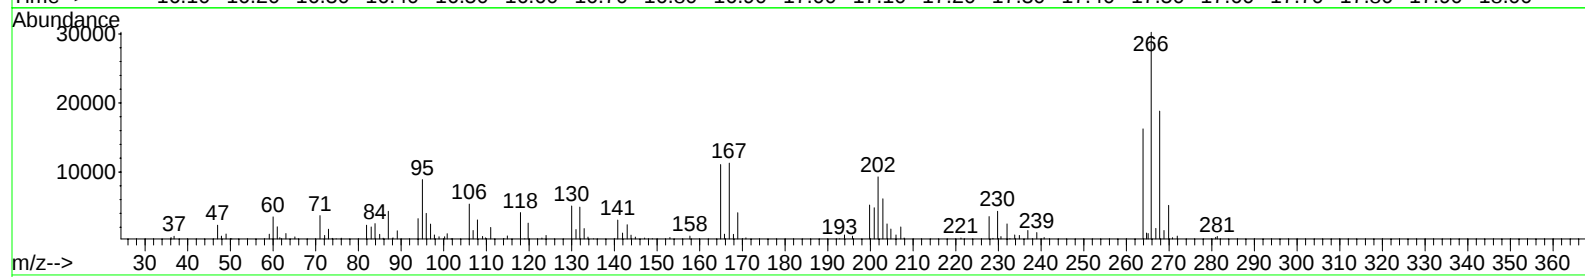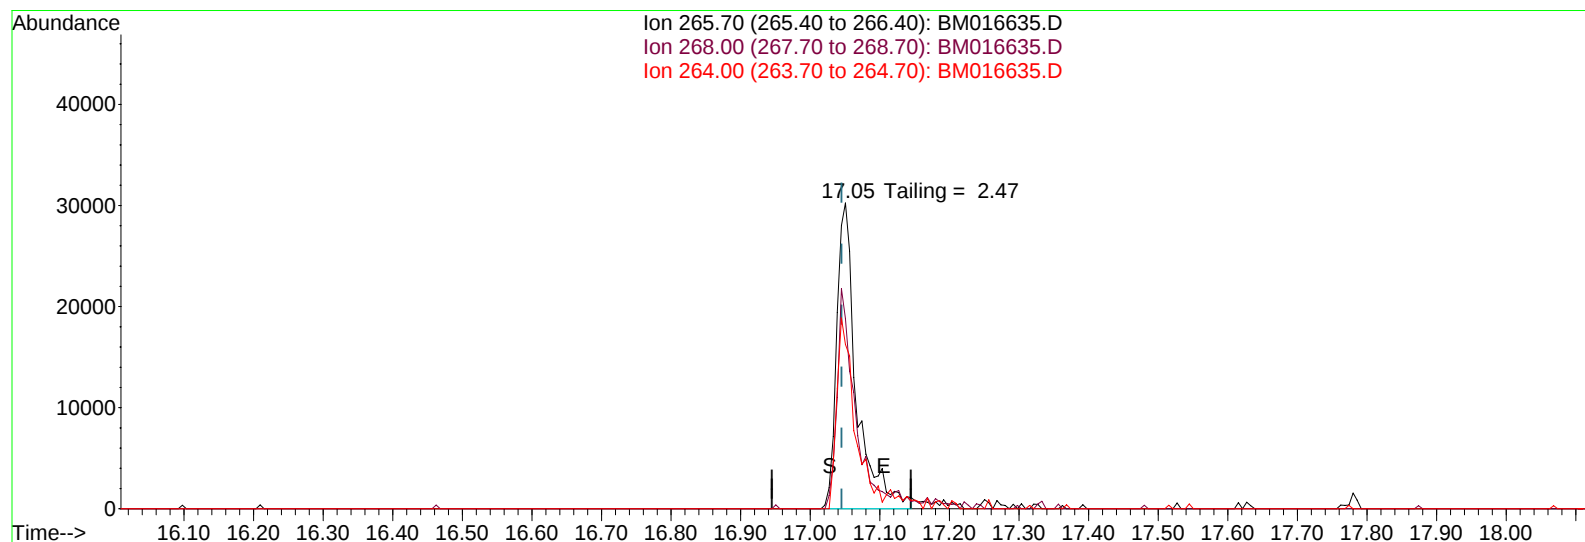

TIC: BM016635.D

(69) Pentachlorophenol (C)

17.051min (+0.006) 0.00ng

response 58412

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.23
264.00	61.20	57.60
0.00	0.00	0.00