

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083118\
 Data File : BM016640.D
 Acq On : 31 Aug 2018 17:13
 Operator : SJ/JU
 Sample : PB112520BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112520BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	378	383	401	rBV	1020487	1742319	18.15%	5.150%
2	7.175	656	661	680	rBV	1065712	1796455	18.71%	5.310%
3	7.528	715	721	737	rBV	1323061	2248482	23.42%	6.646%
4	7.998	797	801	817	rBV	282717	559991	5.83%	1.655%
5	8.316	848	855	870	rBV	1105765	1938993	20.20%	5.731%
6	9.186	997	1003	1017	rBV	571587	1138476	11.86%	3.365%
7	10.804	1272	1278	1293	rBV2	313887	621890	6.48%	1.838%
8	13.257	1689	1695	1711	rBV	2729694	3932538	40.97%	11.623%
9	14.639	1924	1930	1944	rBV2	544141	919943	9.58%	2.719%
10	16.133	2178	2184	2202	rBV	2960027	4354262	45.36%	12.869%
11	17.386	2391	2397	2412	rBV	827910	1341004	13.97%	3.963%
12	19.974	2831	2837	2852	rBV	8519589	9599324	100.00%	28.372%
13	21.527	3097	3101	3112	rBV2	1289846	1821519	18.98%	5.384%
14	23.809	3483	3489	3501	rBV	848513	1818873	18.95%	5.376%


Sum of corrected areas: 33834069

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083118\
Data File : BM016640.D
Acq On : 31 Aug 2018 17:13
Operator : SJ/JU
Sample : PB112520BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112520BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

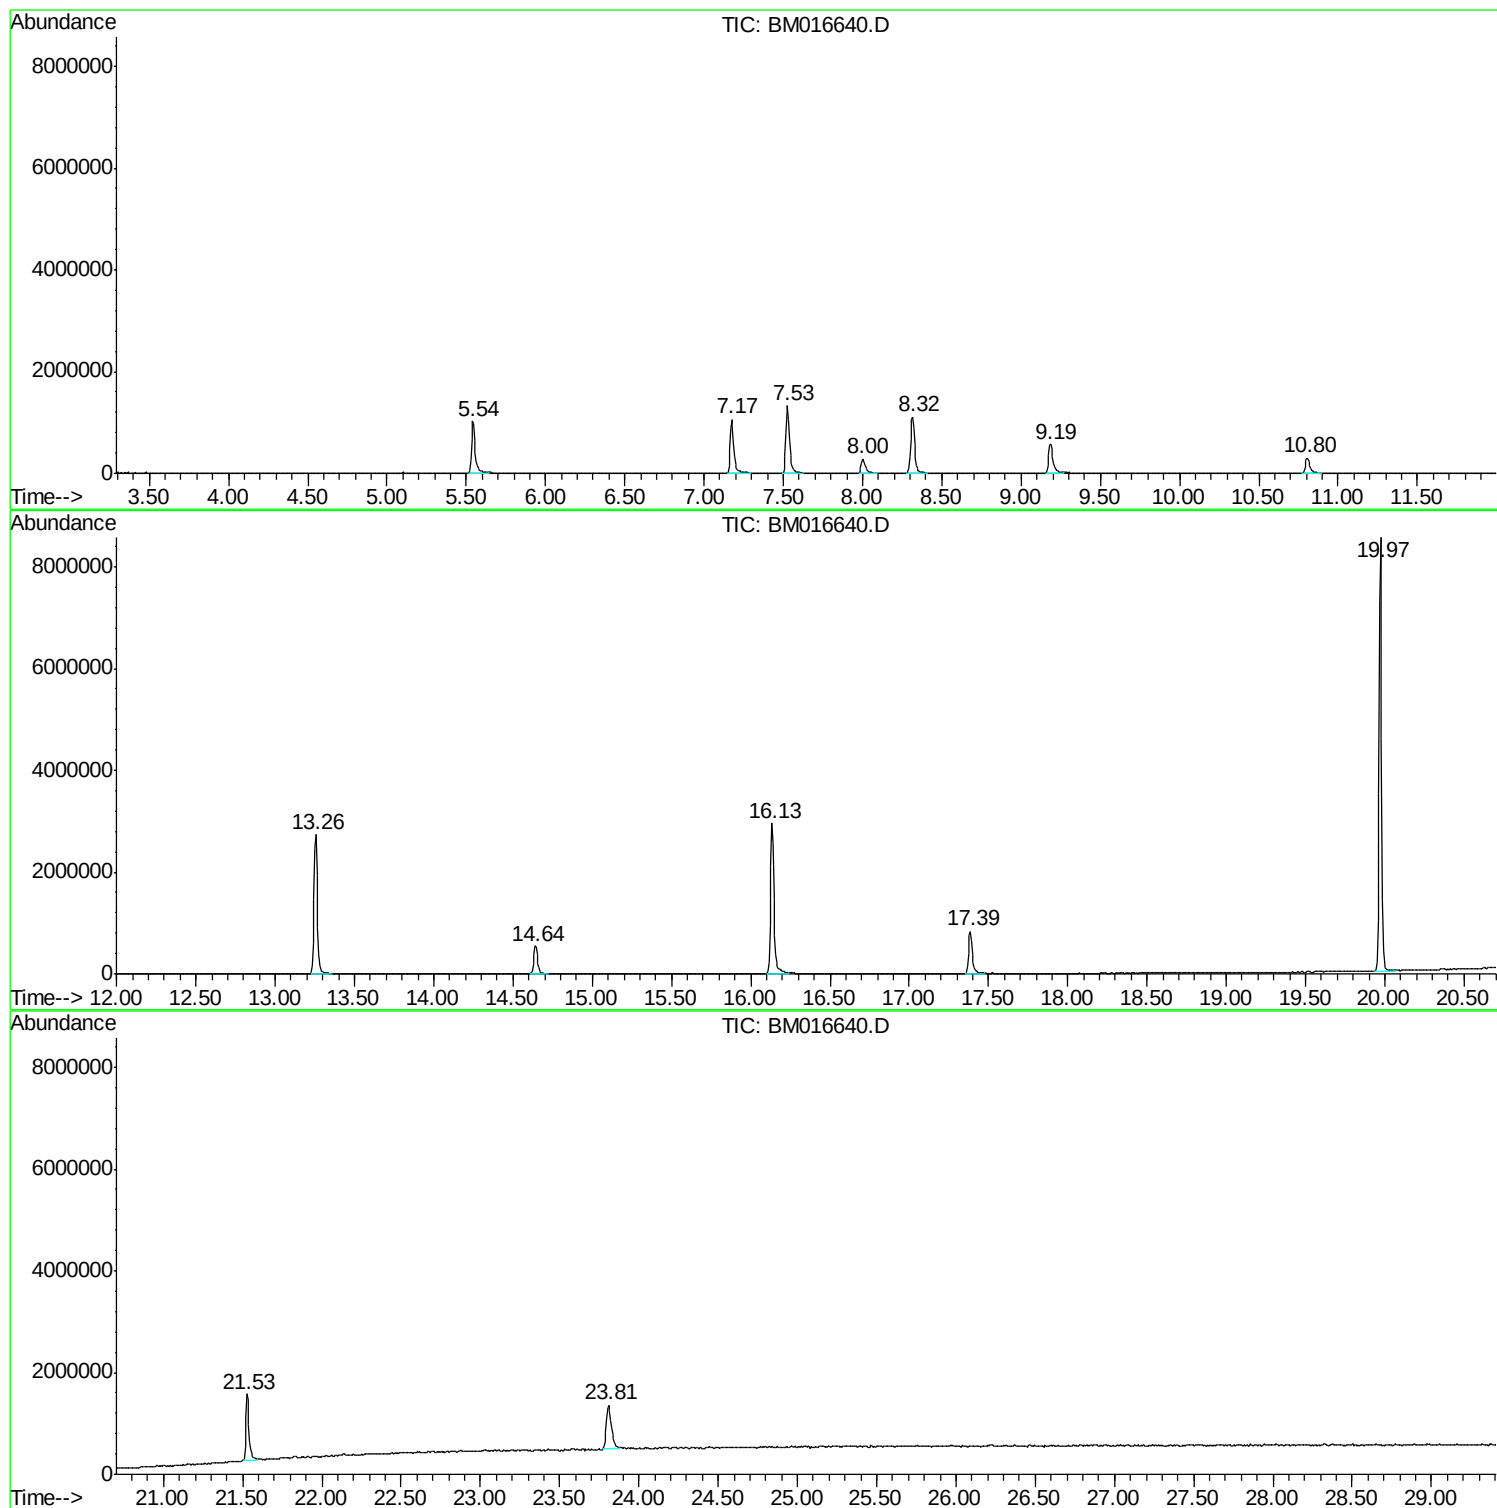

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083118\
Data File : BM016640.D
Acq On : 31 Aug 2018 17:13
Operator : SJ/JU
Sample : PB112520BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112520BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	80.30 ng	2248480	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentadiene	66	C5H6	000542-92-7	27
2		1-Penten-3-yne	66	C5H6	000646-05-9	27
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	22
4		1,4,4a,8a-Tetrahydro-1,4-methano...	174	C11H10O2	001200-89-1	16
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	14

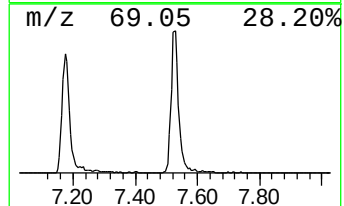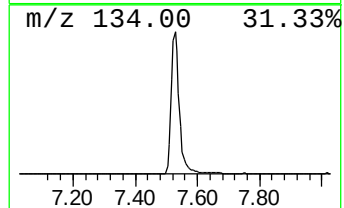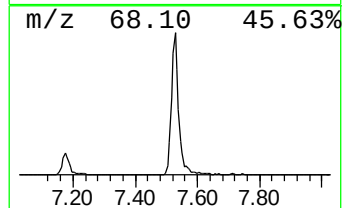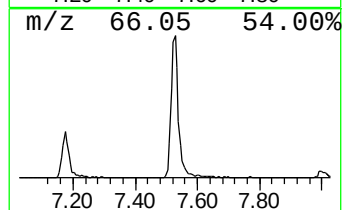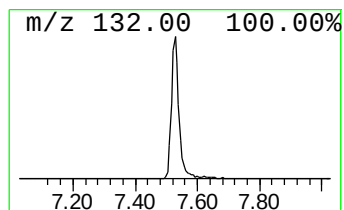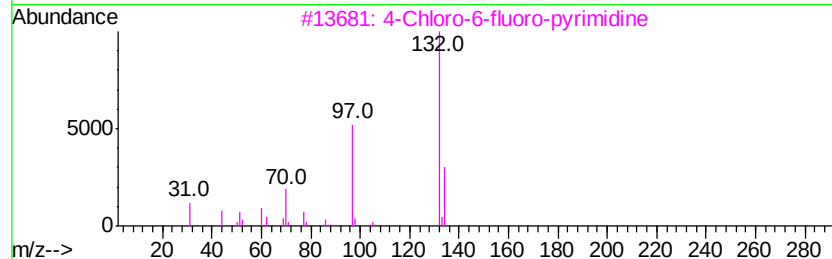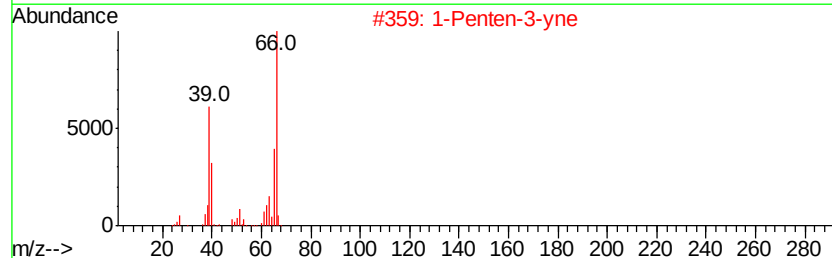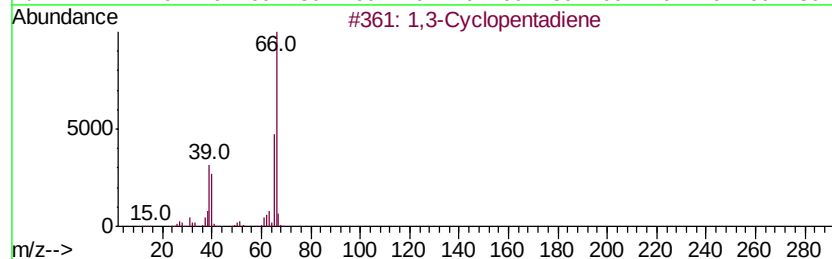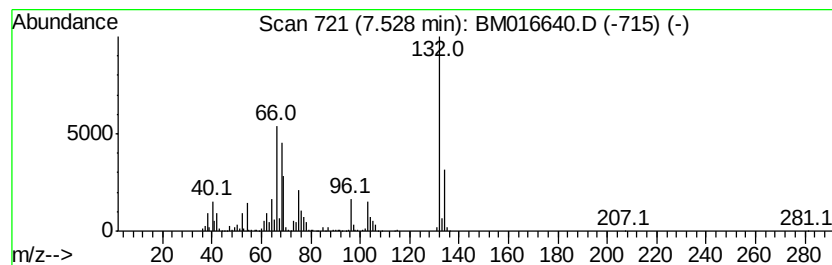

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM083118\
Data File : BM016640.D
Acq On : 31 Aug 2018 17:13
Operator : SJ/JU
Sample : PB112520BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112520BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	80.3	ng	2248480	1	8.00	559991	20.0