


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM083118\
 Data File : BM016635.D
 Acq On : 31 Aug 2018 13:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 27 13:01:22 2018

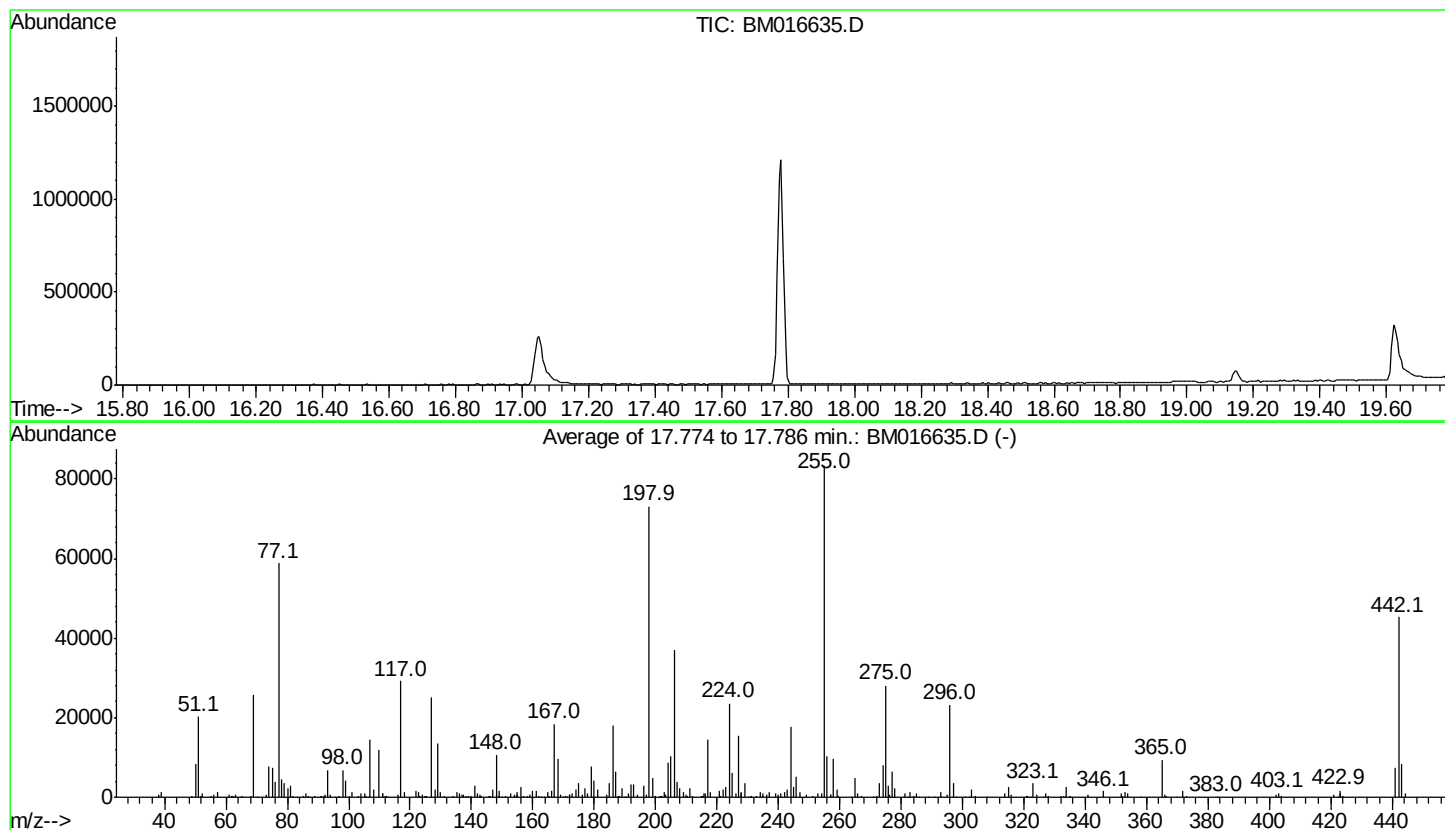

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	20227	PASS
68	69	0.00	2	1.9	488	PASS
69	198	0.00	100	35.3	25796	PASS
70	69	0.00	2	0.5	139	PASS
127	198	10	80	34.2	24970	PASS
197	198	0.00	2	1.1	809	PASS
198	198	100	100	100.0	73048	PASS
199	198	5	9	6.6	4847	PASS
275	198	10	60	38.5	28090	PASS
365	198	1	100	12.9	9404	PASS
441	198	0.01	100	10.2	7451	PASS
442	198	50	100	62.0	45277	PASS
443	442	15	24	18.4	8323	PASS