


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083119\  
 Data File : BM022463.D  
 Acq On : 31 Aug 2019 08:16  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM082919.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Sep 02 03:54:42 2019

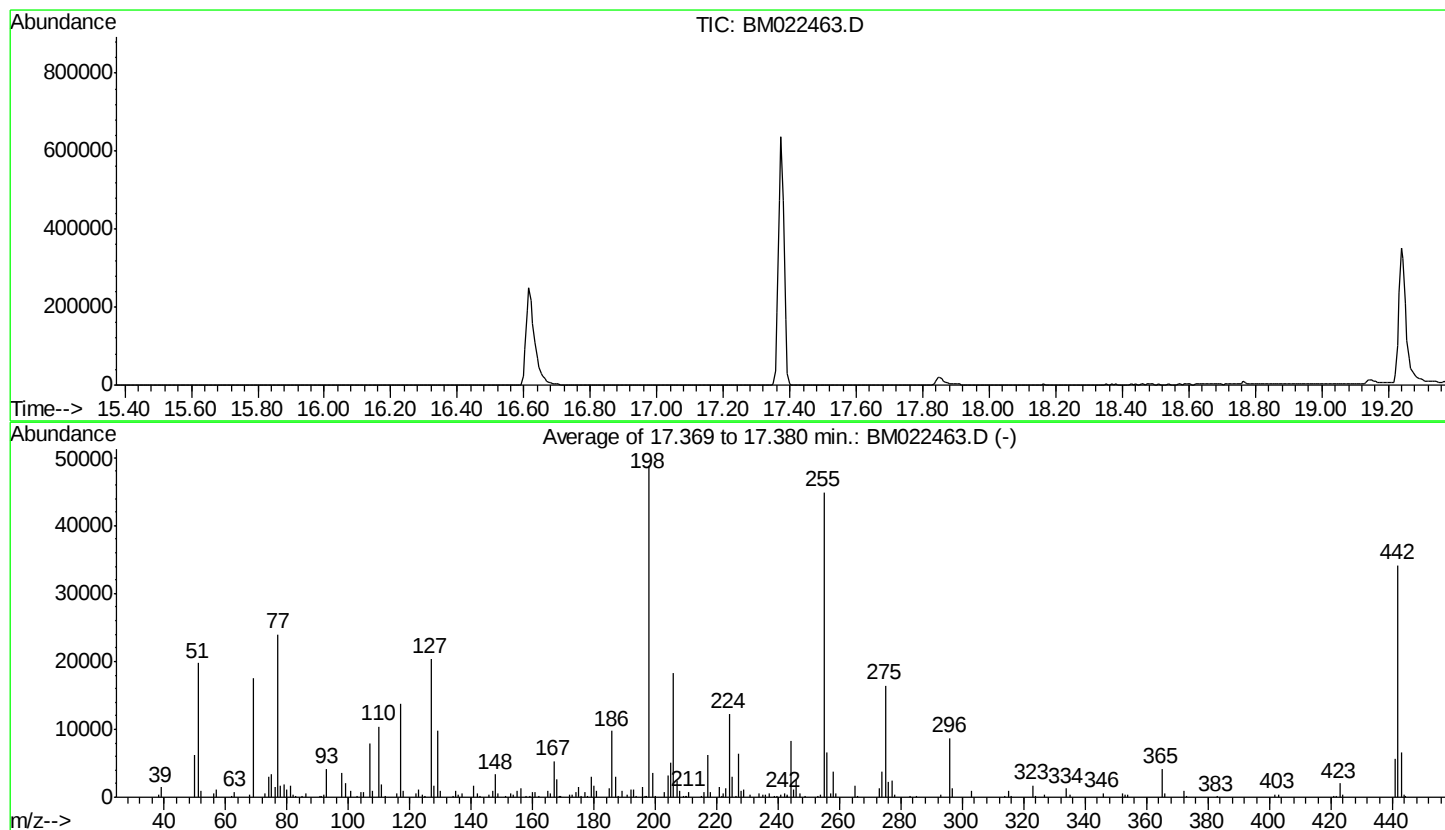

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.5      | 19779   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 296     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.8      | 17506   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 41.8      | 20429   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 242     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 48832   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 3504    | PASS             |
| 275         | 198          | 10           | 60           | 33.7      | 16441   | PASS             |
| 365         | 198          | 1            | 100          | 8.6       | 4213    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.7      | 5689    | PASS             |
| 442         | 198          | 50           | 100          | 70.0      | 34202   | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 6513    | PASS             |