
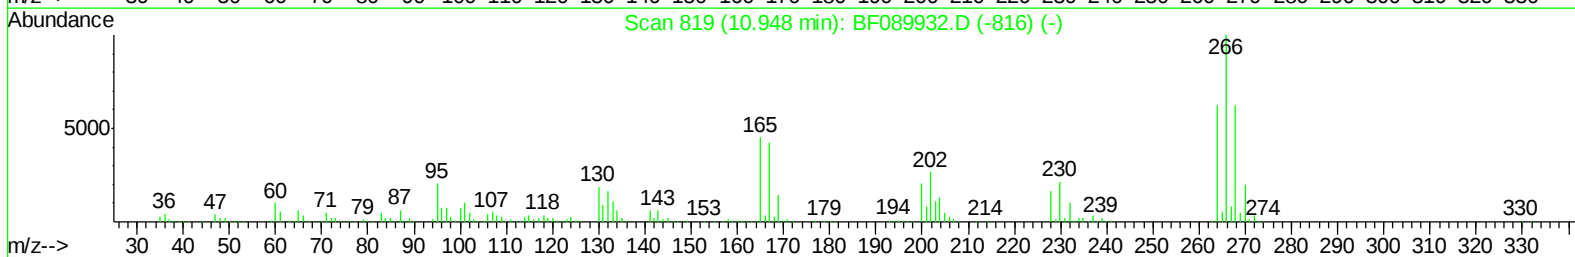
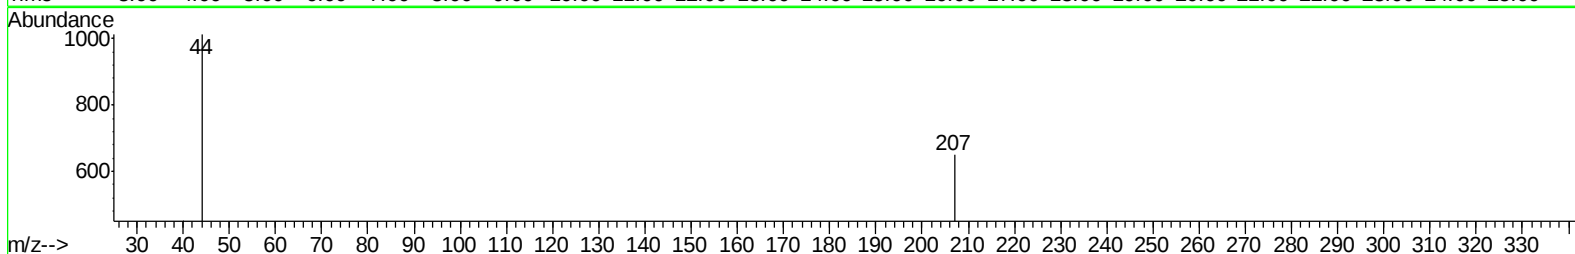


Data Path : Z:\HPCHEM1\BNA_M\Data\BM090116\
Data File : BM007353.D
Acq On : 01 Sep 2016 10:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:50:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

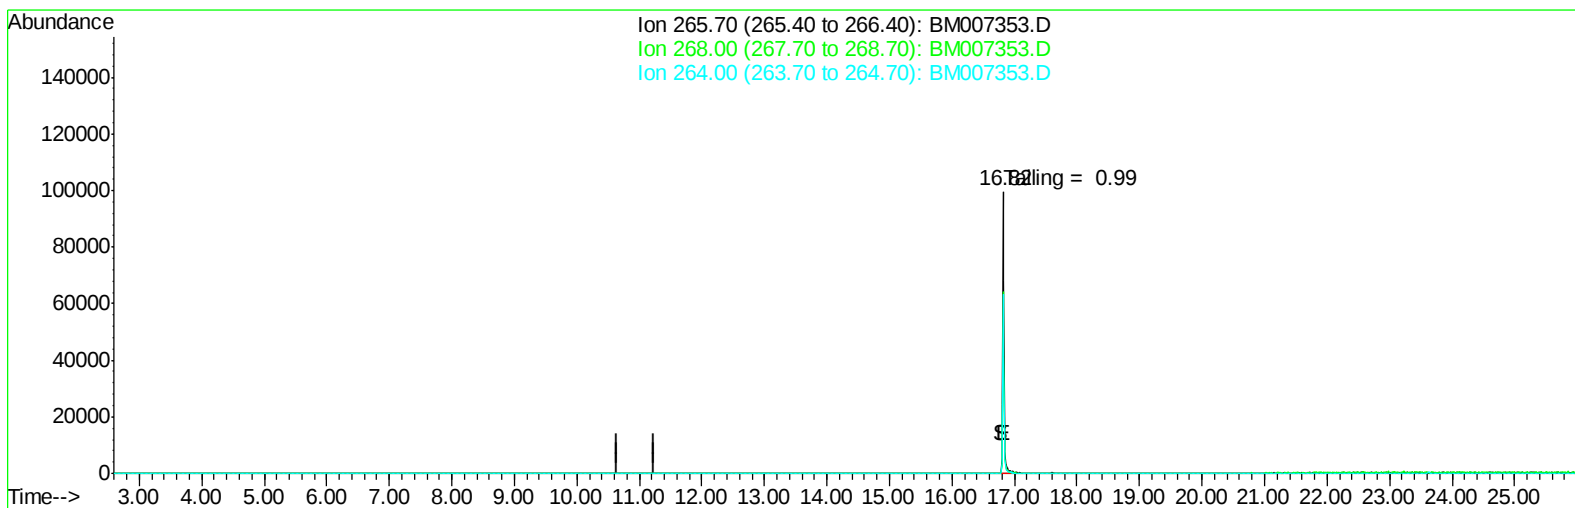

TIC: BM007353.D

(69) Pentachlorophenol (C)




10.947min (-10.947) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.80	0.00#
264.00	63.20	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM090116\
Data File : BM007353.D
Acq On : 01 Sep 2016 10:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:50:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

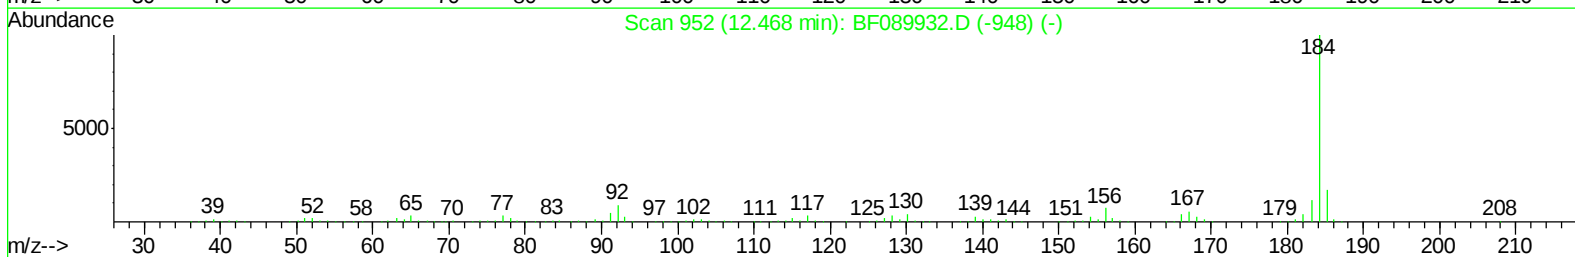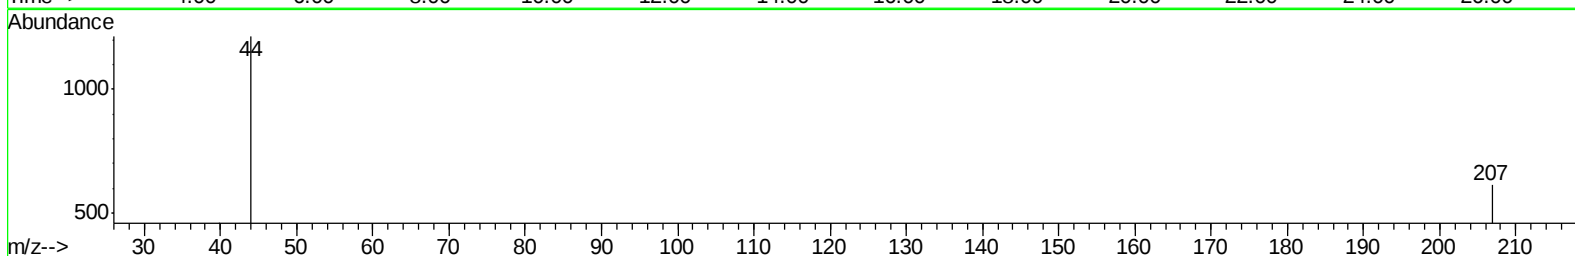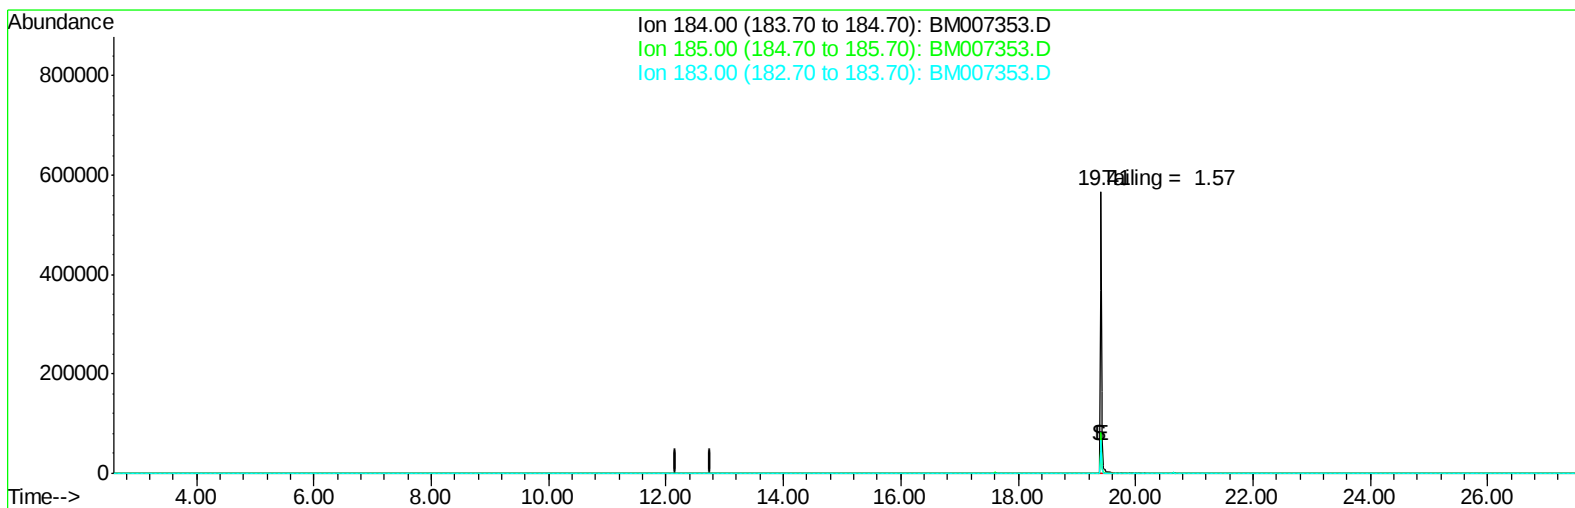

TIC: BM007353.D

(76) Benzidine

12.468min (-12.468) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	17.30	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00