


Data Path : Z:\HPCHEM1\BNA M\Data\BM090116\
 Data File : BM007353.D
 Acq On : 01 Sep 2016 10:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM090116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 12:51:17 2016

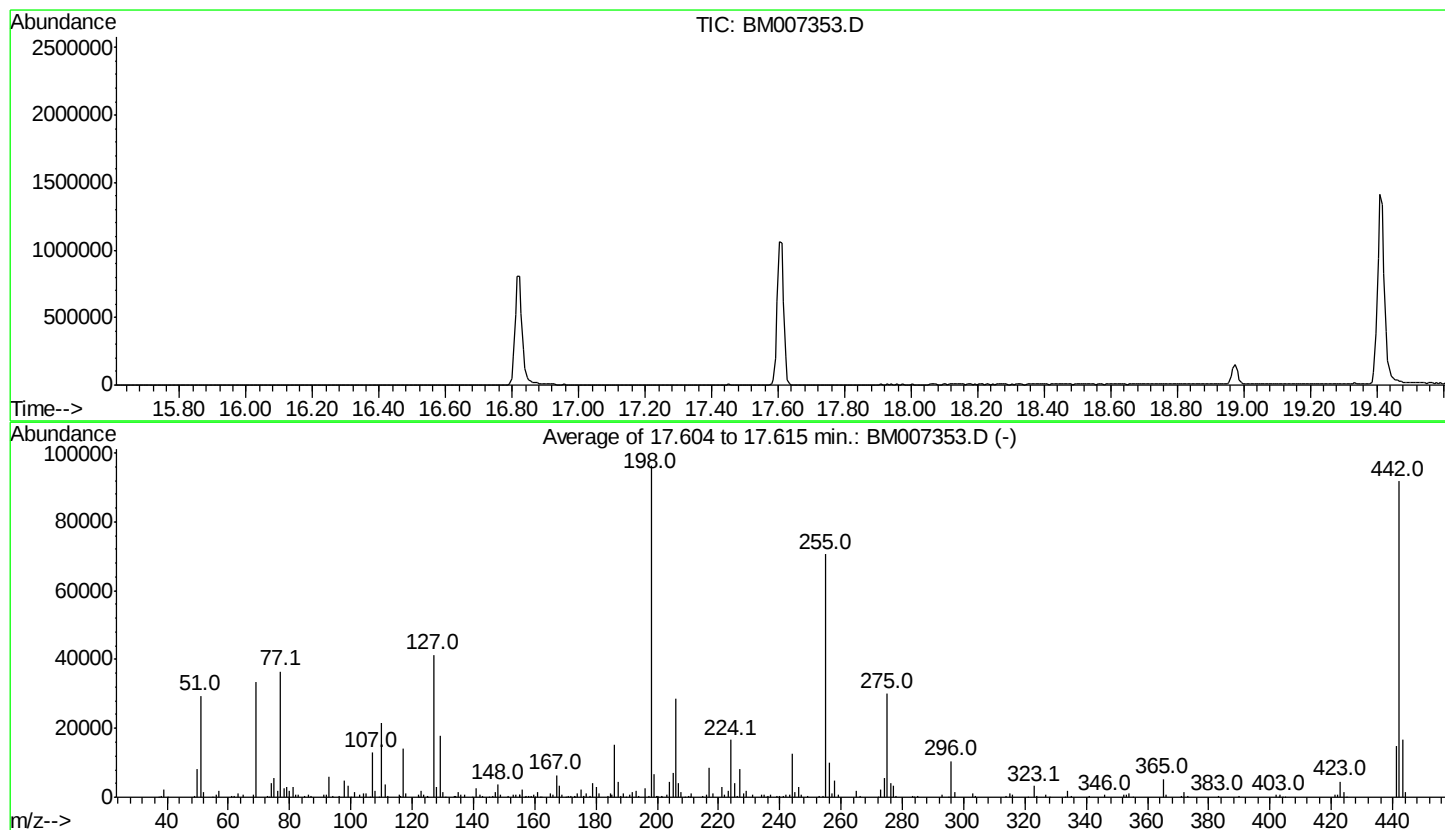

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	29460	PASS
68	69	0.00	2	1.9	641	PASS
69	198	0.00	100	34.6	33330	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	41298	PASS
197	198	0.00	2	0.5	461	PASS
198	198	100	100	100.0	96304	PASS
199	198	5	9	7.0	6760	PASS
275	198	10	60	31.1	29994	PASS
365	198	1	100	5.4	5239	PASS
441	442	0.01	24	16.1	14733	PASS
442	198	50	100	95.3	91773	PASS
443	442	15	24	18.4	16897	PASS