
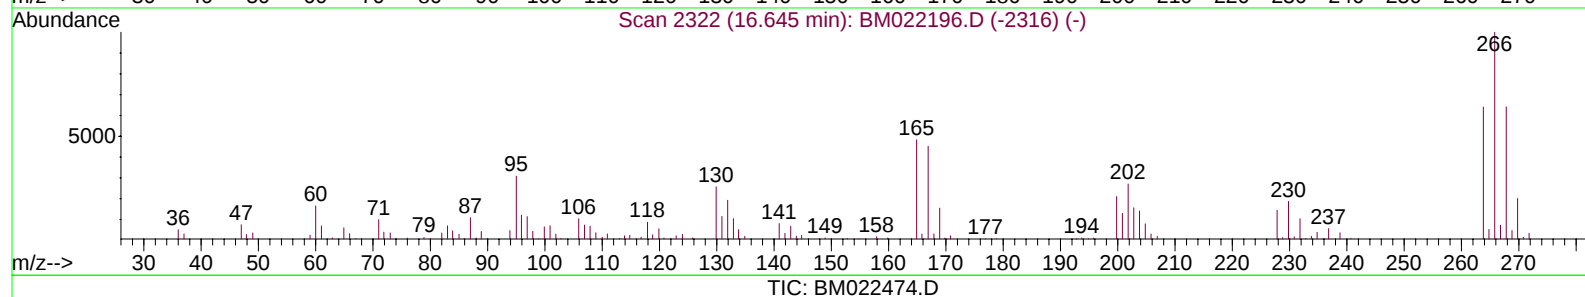
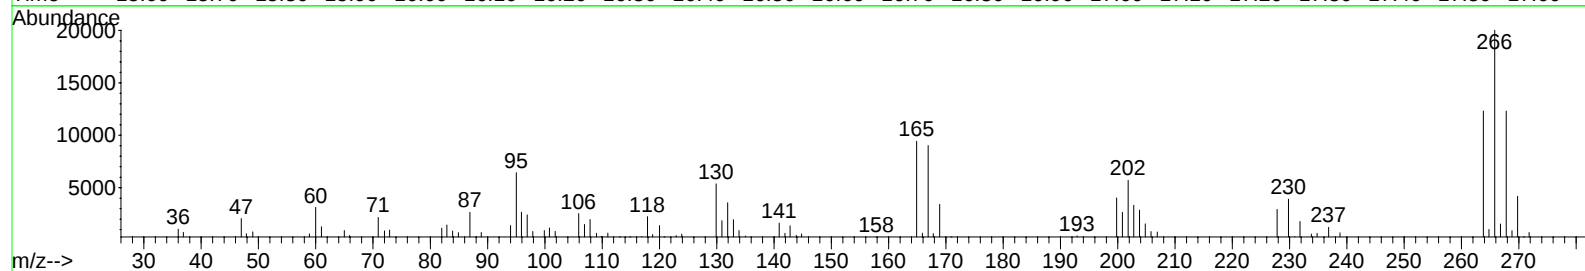


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090119\
Data File : BM022474.D
Acq On : 01 Sep 2019 12:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:48:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 02 03:54:42 2019
Response via : Initial Calibration

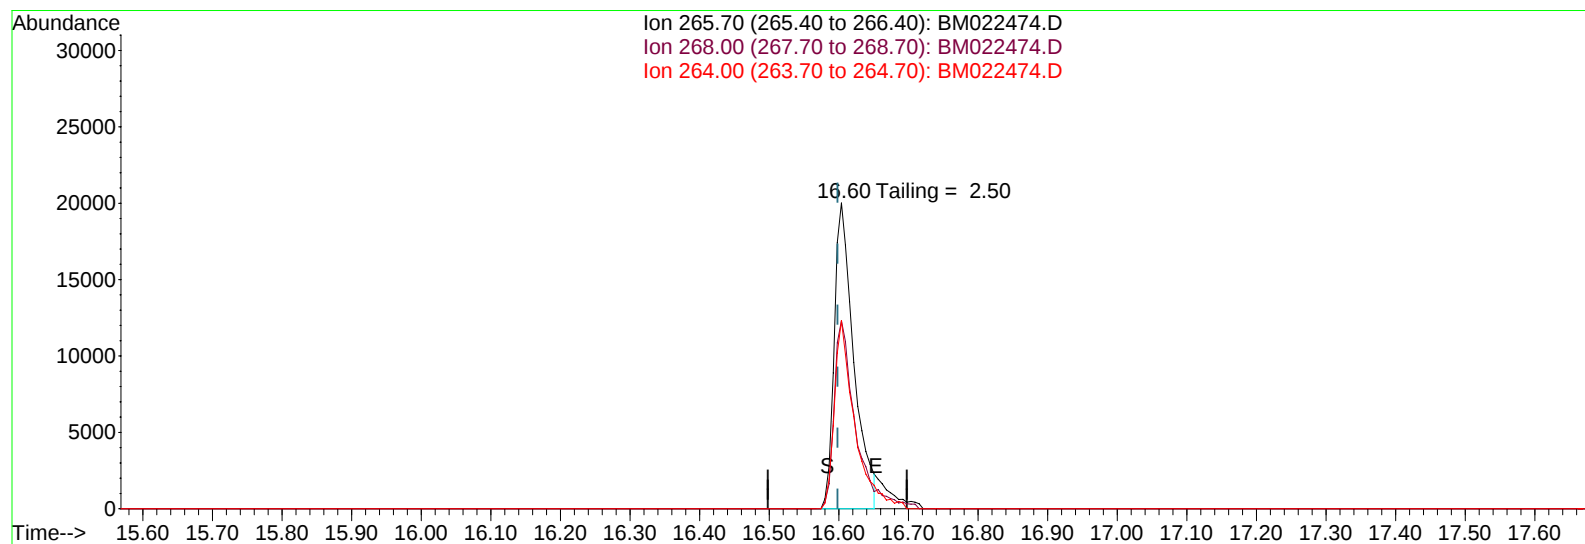

(70) Pentachlorophenol (C)




16.604min (+0.006) 0.00ng

response 41195

Ion	Exp%	Act%
265.70	100	100
268.00	60.50	61.52
264.00	64.60	61.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090119\
 Data File : BM022474.D
 Acq On : 01 Sep 2019 12:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:48:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 02 03:54:42 2019
 Response via : Initial Calibration

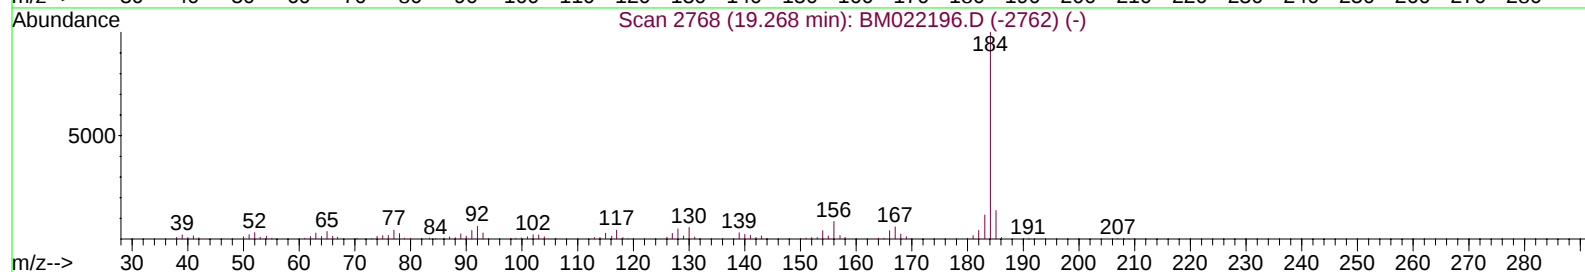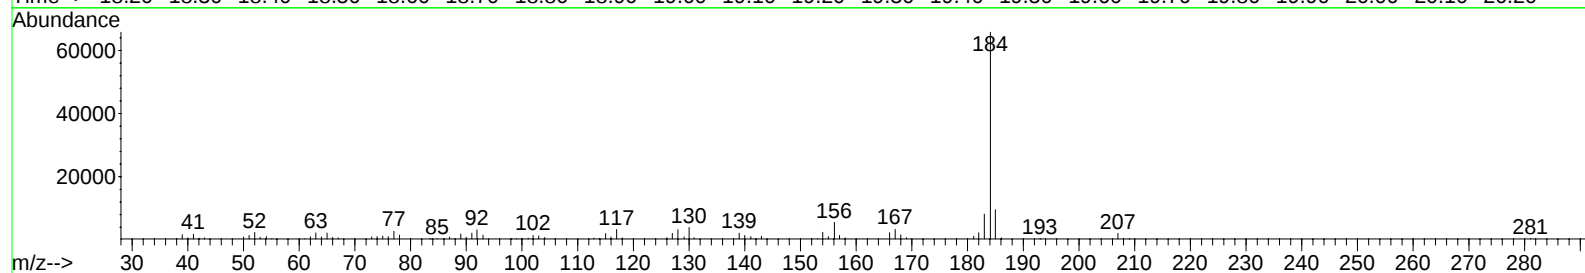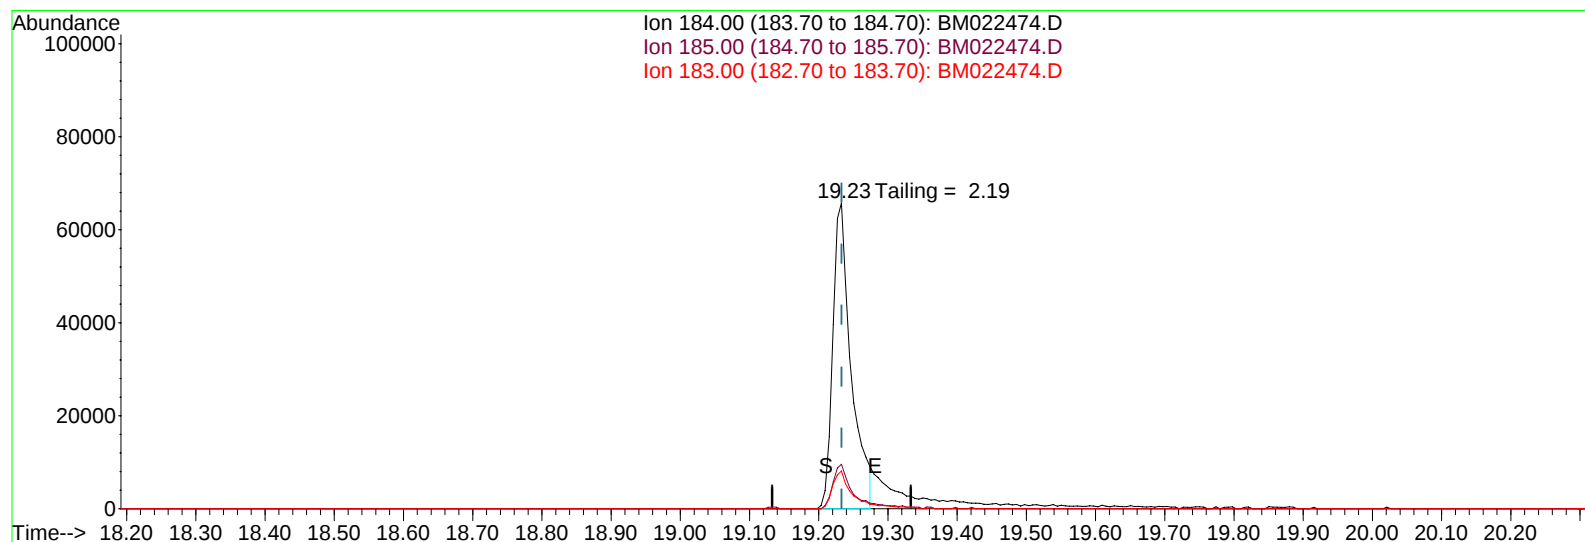

TIC: BM022474.D

(77) Benzidine

19.233min (-0.000) 0.00ng

response 132835

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.55
183.00	11.80	12.38
0.00	0.00	0.00