

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
 Data File : BM022480.D
 Acq On : 01 Sep 2019 16:58
 Operator : HP/JU
 Sample : K4619-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP5-COMP

Quant Time: Sep 02 04:20:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 02 03:54:42 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	10762	20.00	ng	0.00
21) Naphthalene-d8	10.29	136	36146	20.00	ng	0.00
39) Acenaphthene-d10	14.17	164	23789	20.00	ng	0.00
64) Phenanthrene-d10	16.95	188	56672	20.00	ng	0.01
76) Chrysene-d12	21.16	240	89669	20.00	ng	0.00
87) Perylene-d12	23.34	264	110588	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	57879	94.40	ng	0.00
7) Phenol-d6	6.70	99	71750	87.51	ng	0.00
23) Nitrobenzene-d5	8.69	82	49345	59.79	ng	0.00
42) 2,4,6-Tribromophenol	15.69	330	36864	75.73	ng	0.00
45) 2-Fluorobiphenyl	12.77	172	110456	52.60	ng	0.00
79) Terphenyl-d14	19.59	244	307364	45.24	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.67	163	8324	4.023	ng	Qvalue # 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
Data File : BM022480.D
Acq On : 01 Sep 2019 16:58
Operator : HP/JU
Sample : K4619-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP5-COMP

Quant Time: Sep 02 04:20:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 02 03:54:42 2019
Response via : Initial Calibration

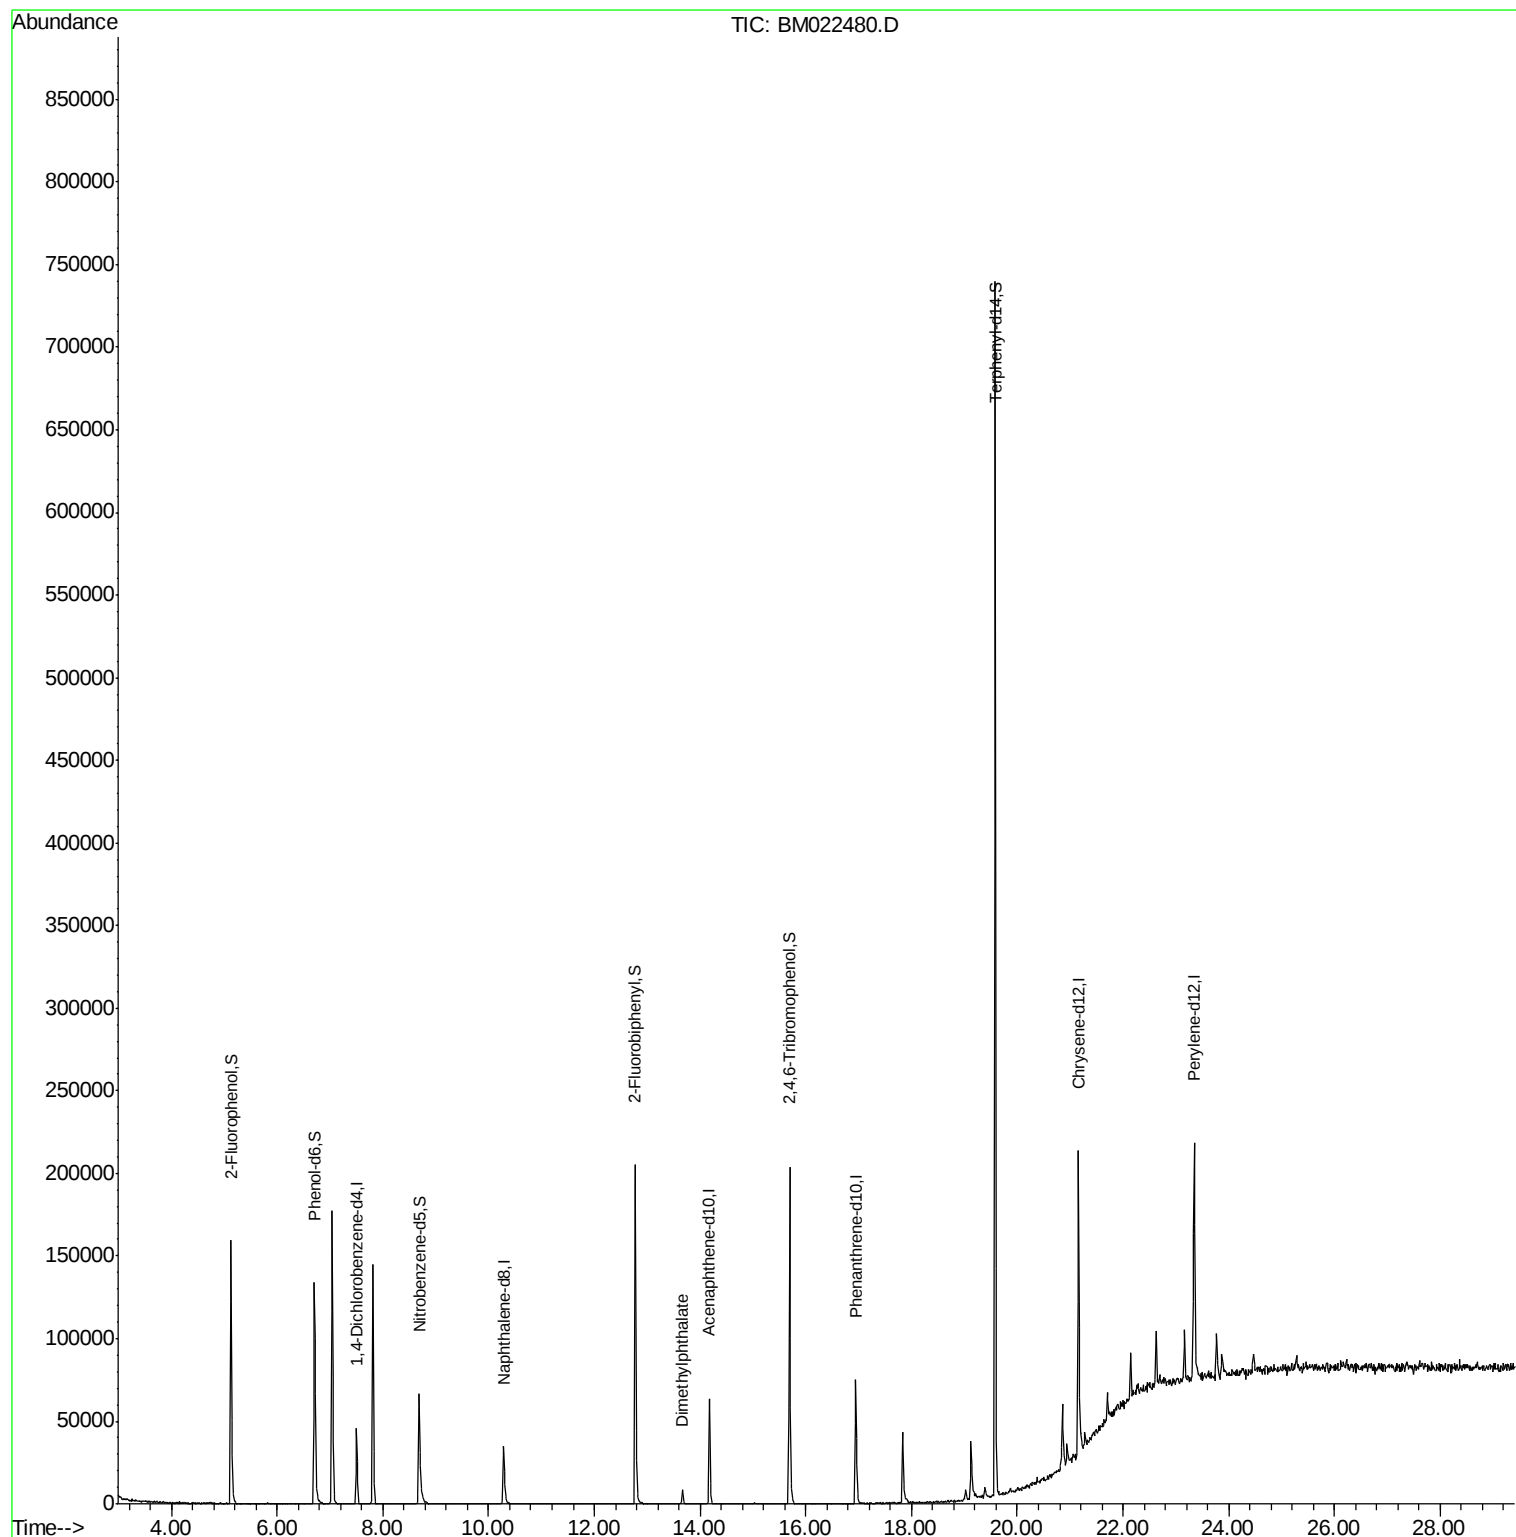

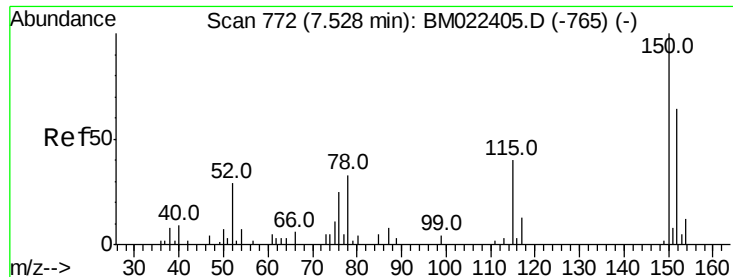


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.50 min Scan# 768
Delta R.T. -0.01 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58

Instrument :
BNA_M
ClientSampleId :
TP5-COMP

Tot Ion:152 Resp: 10762
Ion Ratio Lower Upper
152 100
150 149.9 125.4 188.0
115 63.9 50.3 75.5

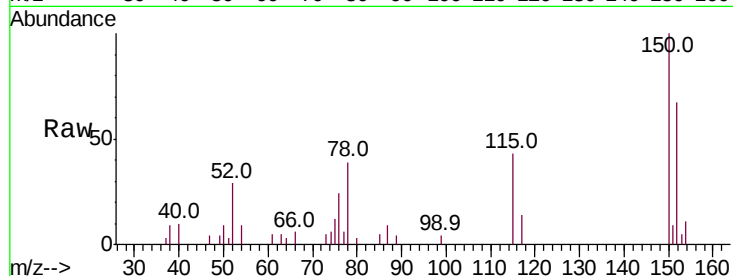


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

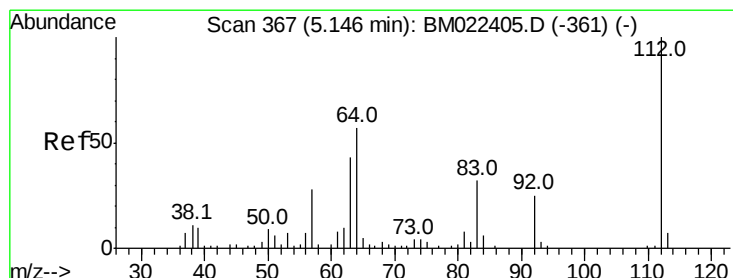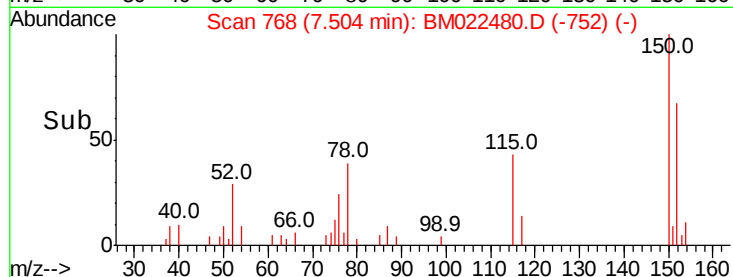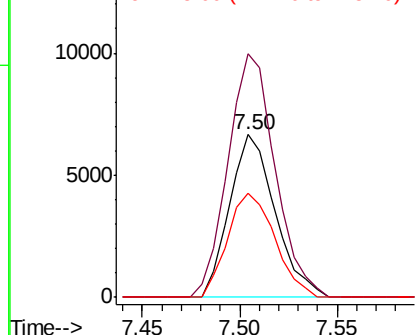



#5


2-Fluorophenol
Concen: 94.403 ng
RT: 5.13 min Scan# 364
Delta R.T. -0.00 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58

Tgt Ion:112 Resp: 57879
Ion Ratio Lower Upper
112 100
64 63.5 45.4 68.2
63 44.4 34.5 51.7

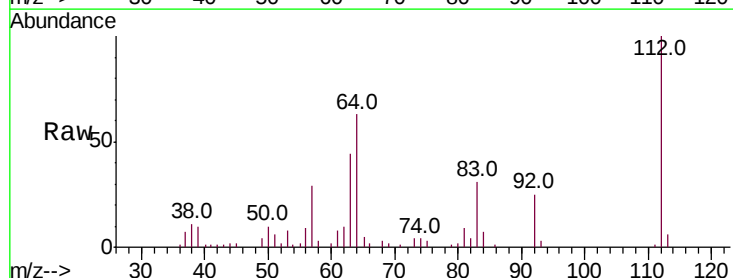

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

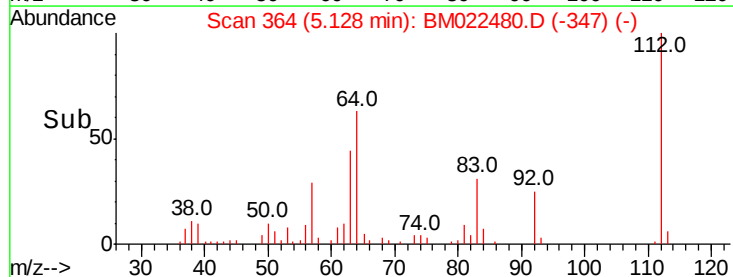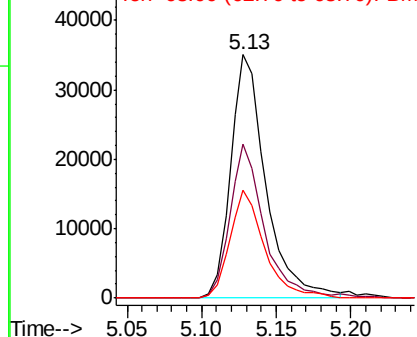

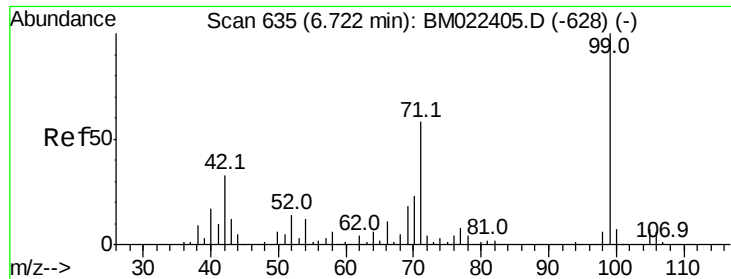

#7

Phenol-d6

Concen: 87.513 ng

RT: 6.70 min Scan# 632

Delta R.T. -0.01 min

Lab File: BM022480.D

Acq: 01 Sep 2019 16:58

Instrument :

BNA_M

ClientSampleId :

TP5-COMP


Tot Ion: 99 Resp: 71750

Ion Ratio Lower Upper

99 100

42 34.0 26.3 39.5




71 54.0 46.6 69.8

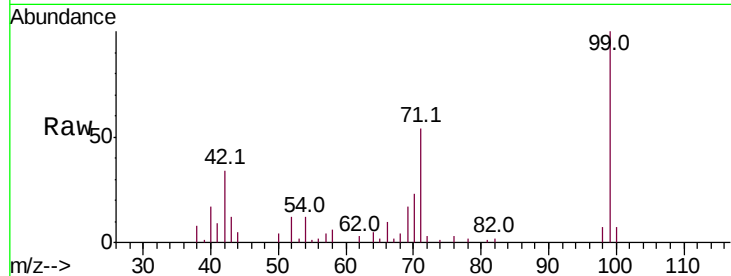

Abundance Ion 99.00 (98.70 to 99.70): BM022405.D (-628) (-)

Ion 42.00 (41.70 to 42.70): BM022405.D (-628) (-)

Ion 71.00 (70.70 to 71.70): BM022405.D (-628) (-)

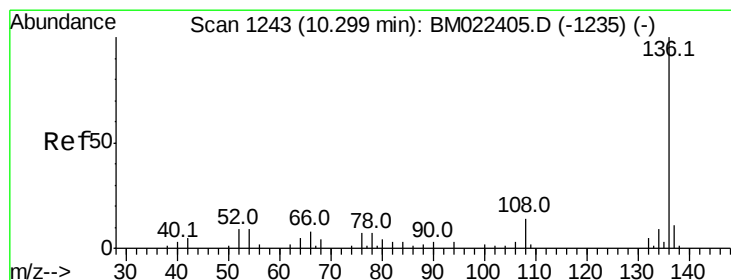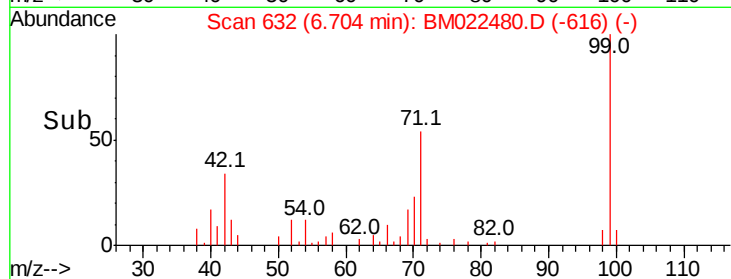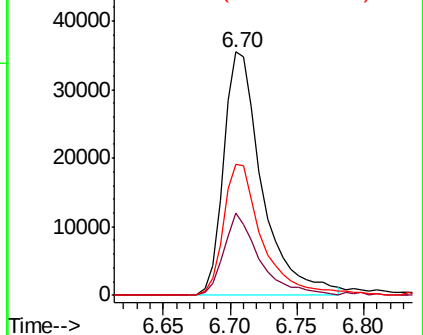

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.29 min Scan# 1241

Delta R.T. 0.01 min

Lab File: BM022480.D

Acq: 01 Sep 2019 16:58

Tgt Ion: 136 Resp: 36146


Ion Ratio Lower Upper

136 100

137 11.4 8.6 13.0

54 10.8 7.0 10.6#

68 4.0 2.9 4.3


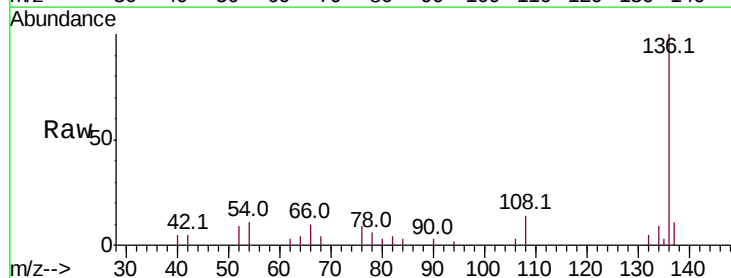



Abundance Ion 136.00 (135.70 to 136.70): BM022405.D (-1235) (-)

Ion 137.00 (136.70 to 137.70): BM022405.D (-1235) (-)

Ion 54.00 (53.70 to 54.70): BM022405.D (-1235) (-)

Ion 68.00 (67.70 to 68.70): BM022405.D (-1235) (-)



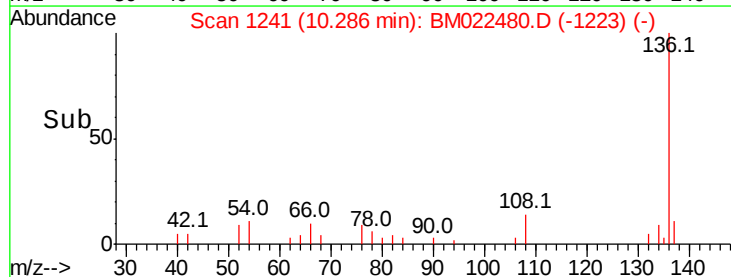
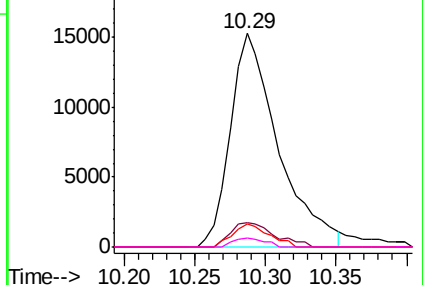


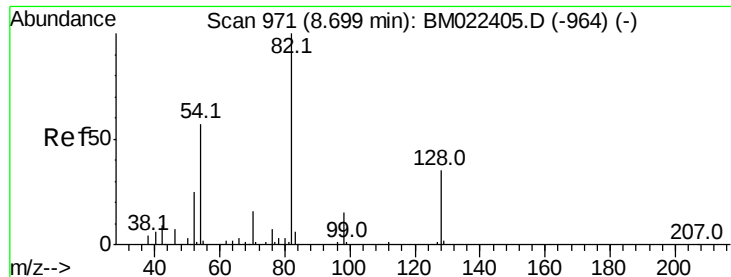

#23
Nitrobenzene-d5
Concen: 59.794 ng
RT: 8.69 min Scan# 969
Delta R.T. 0.01 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58




Instrument :
BNA_M
ClientSampled :
TP5-COMP


Tot Ion	Ratio	Lower	Upper
82	100		
128	34.1	27.9	41.9
54	57.5	45.2	67.8

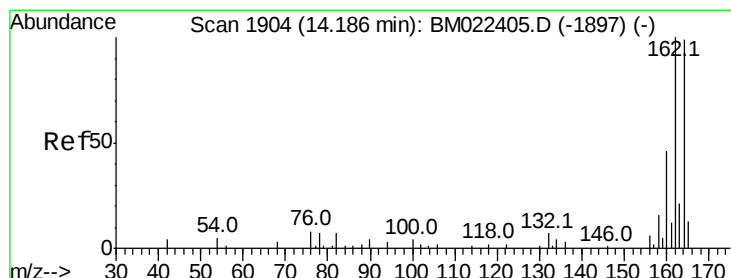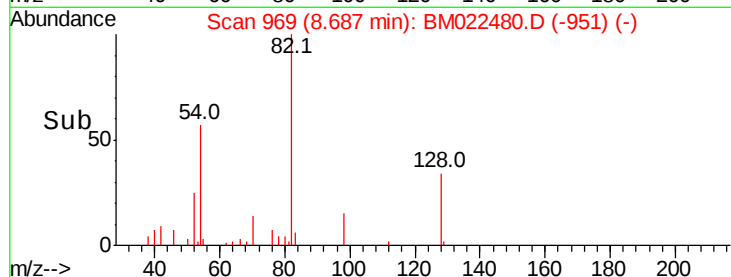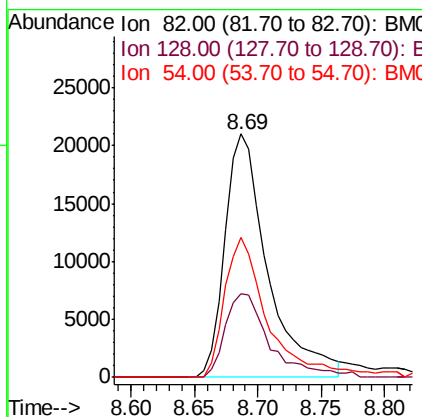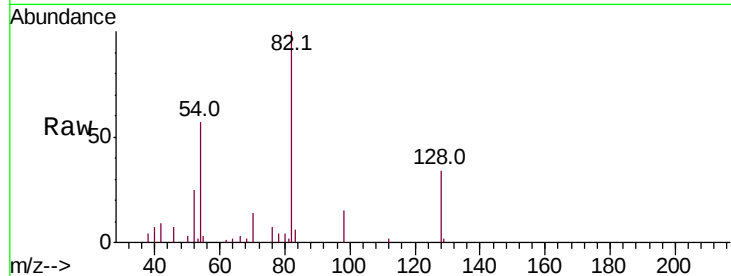

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.17 min Scan# 1902
Delta R.T. 0.01 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58

Tgt Ion	Ratio	Lower	Upper
164	100		
162	111.6	80.6	121.0
160	47.2	37.3	55.9

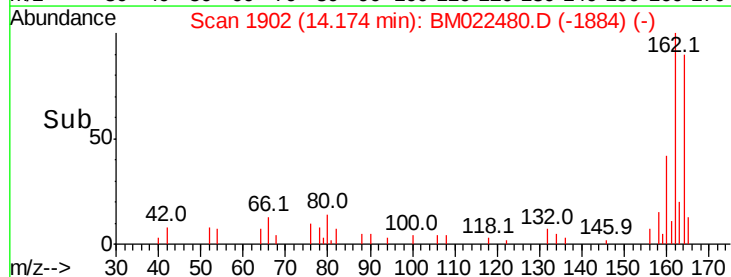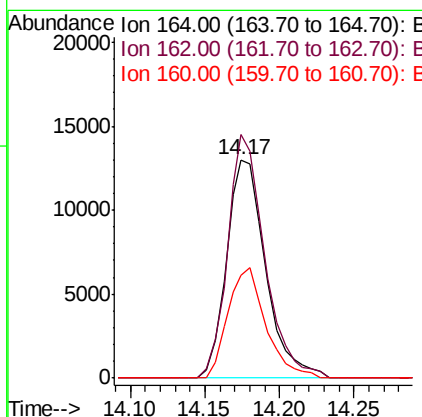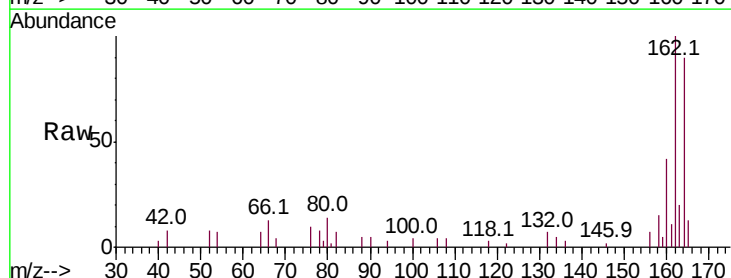


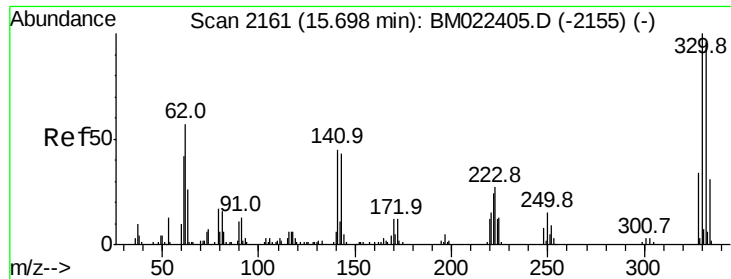




#42
 2,4,6-Tribromophenol
 Concen: 75.729 ng
 RT: 15.69 min Scan# 2160
 Delta R.T. 0.01 min
 Lab File: BM022480.D
 Acq: 01 Sep 2019 16:58

Instrument :
 BNA_M
 ClientSampleId :
 TP5-COMP

Tot Ion:330 Resp: 36864
 Ion Ratio Lower Upper
 330 100
 332 99.0 77.8 116.8
 141 52.1 35.6 53.4

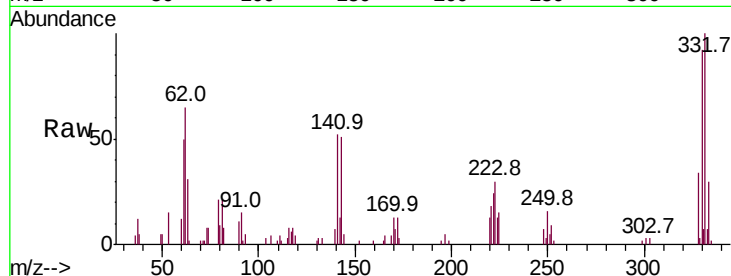


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

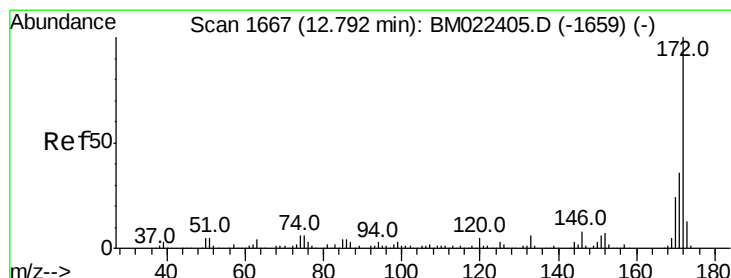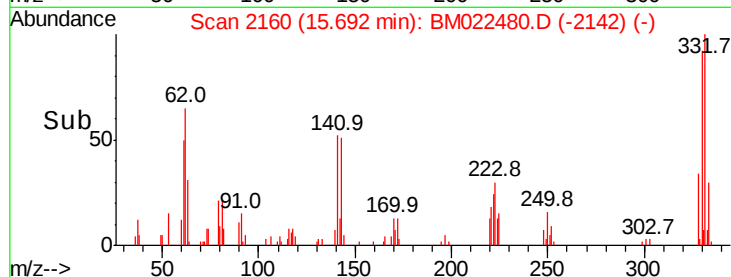
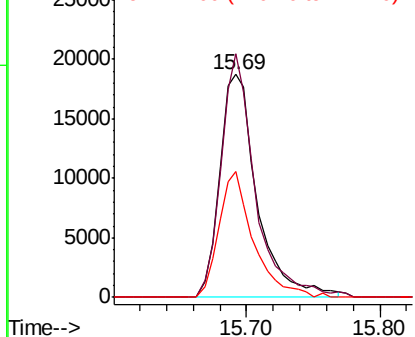



#45
 2-Fluorobiphenyl
 Concen: 52.600 ng
 RT: 12.77 min Scan# 1664
 Delta R.T. -0.00 min
 Lab File: BM022480.D
 Acq: 01 Sep 2019 16:58

Tgt Ion:172 Resp: 110456
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.5 42.7
 170 24.7 18.9 28.3

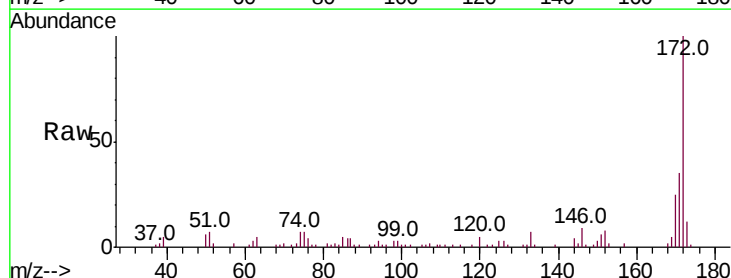

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

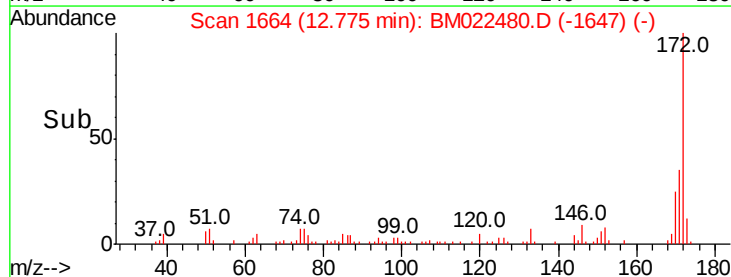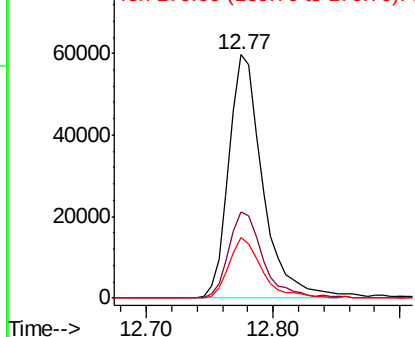


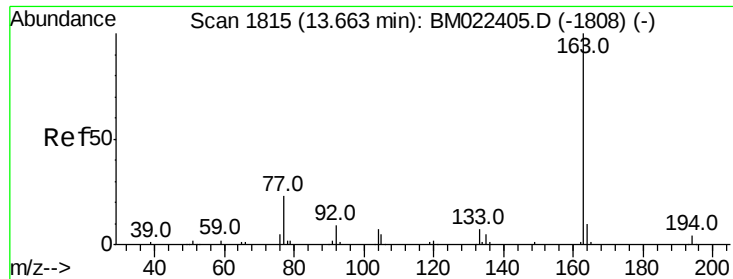




#50
Dimethylphthalate
Concen: 4.023 ng
RT: 13.67 min Scan# 1816
Delta R.T. 0.02 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58

Instrument :
BNA_M
ClientSampleId :
TP5-COMP

Tot Ion:163 Resp: 8324
Ion Ratio Lower Upper
163 100
194 0.0 3.4 5.2#
164 8.8 8.2 12.2

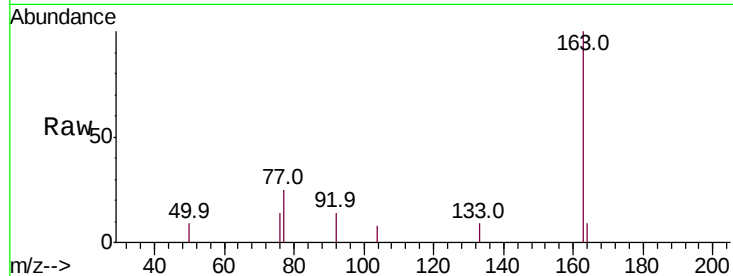


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

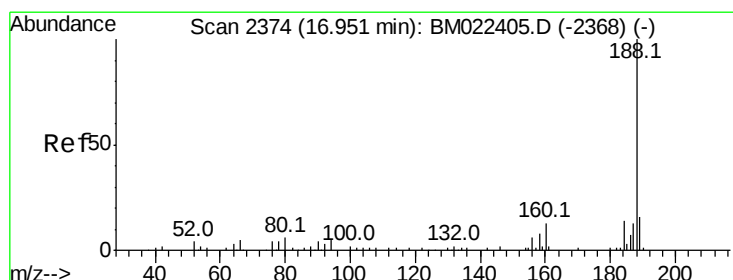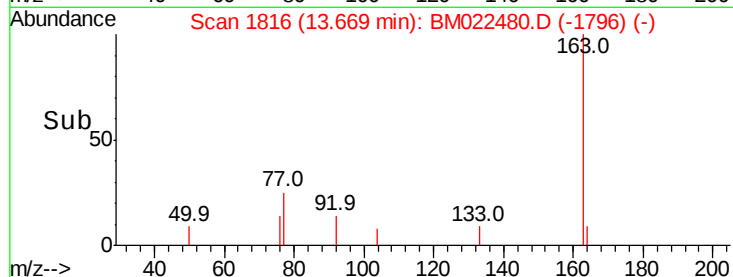
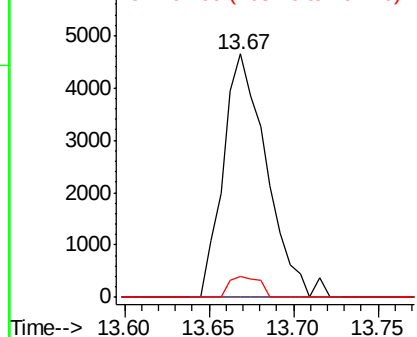



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.95 min Scan# 2374
Delta R.T. 0.01 min
Lab File: BM022480.D
Acq: 01 Sep 2019 16:58

Tgt Ion:188 Resp: 56672
Ion Ratio Lower Upper
188 100
94 6.0 4.4 6.6
80 7.5 5.0 7.6

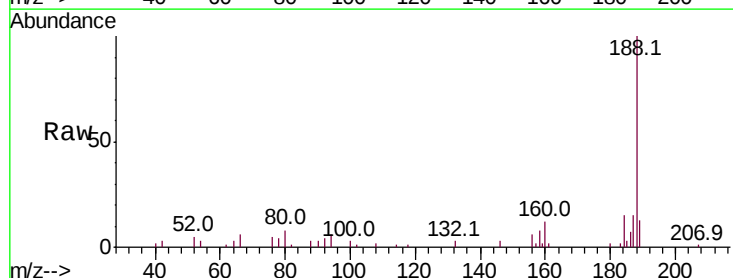

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM



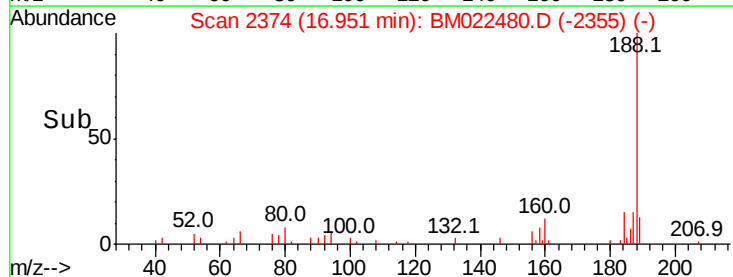
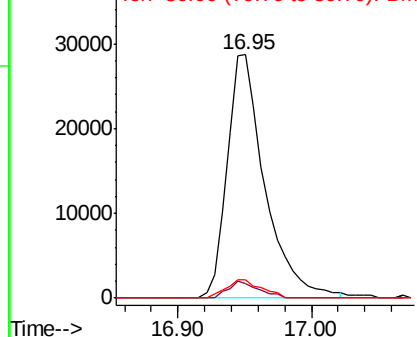


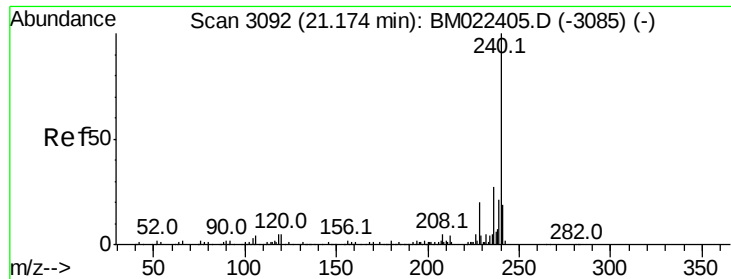

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.16 min Scan# 3090
 Delta R.T. 0.01 min
 Lab File: BM022480.D
 Acq: 01 Sep 2019 16:58




Instrument :
 BNA_M
 ClientSampleId :
 TP5-COMP


Tot Ion:240 Resp: 89669
 Ion Ratio Lower Upper
 240 100
 120 5.9 3.9 5.9#
 236 28.0 21.4 32.2

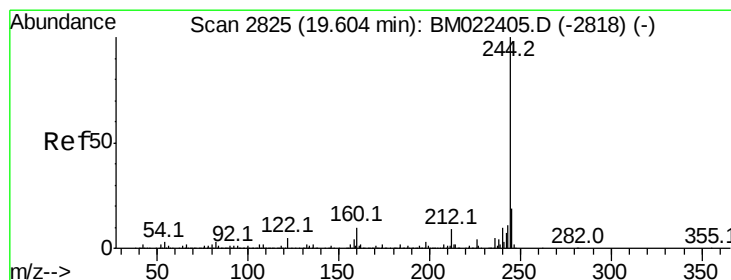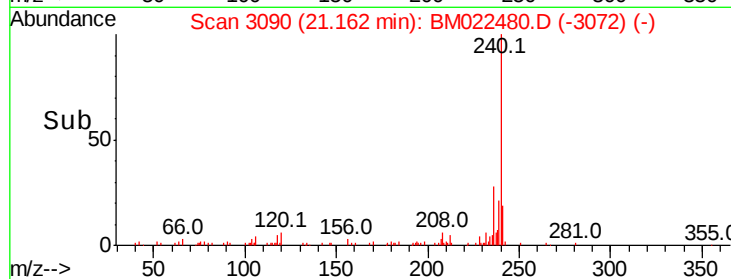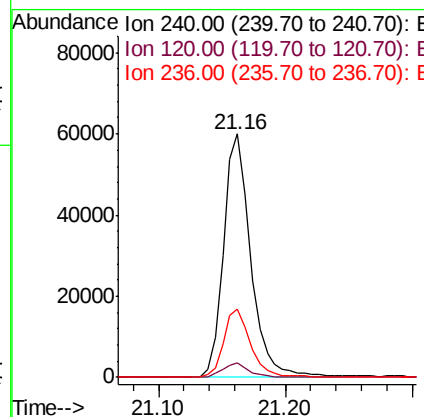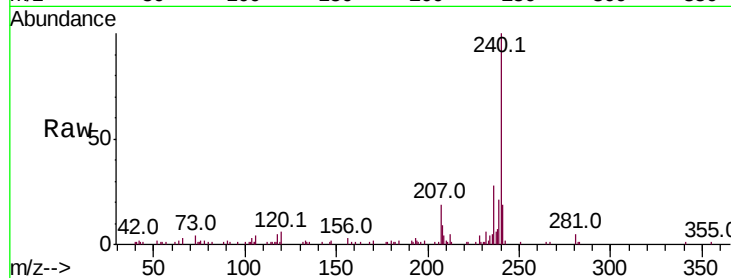

#79
 Terphenyl-d14
 Concen: 45.238 ng
 RT: 19.59 min Scan# 2822
 Delta R.T. -0.00 min
 Lab File: BM022480.D
 Acq: 01 Sep 2019 16:58

Tgt Ion:244 Resp: 307364
 Ion Ratio Lower Upper
 244 100
 212 9.4 7.0 10.4
 122 5.8 3.9 5.9

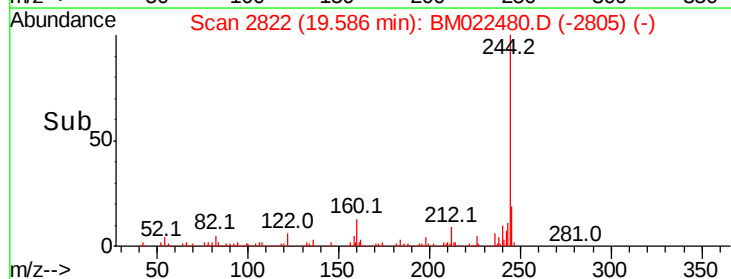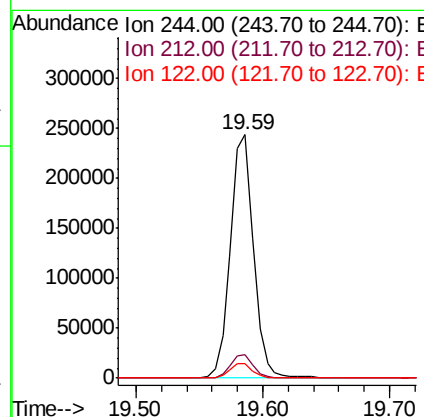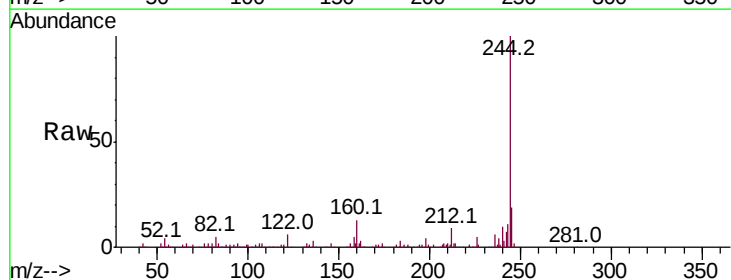


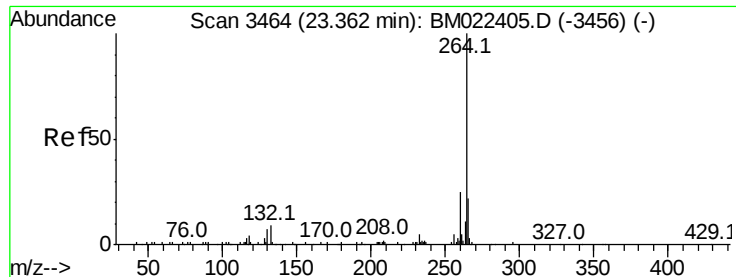

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.34 min Scan# 3461
 Delta R.T. -0.00 min
 Lab File: BM022480.D
 Acq: 01 Sep 2019 16:58

Instrument :
 BNA_M
 ClientSampleId :
 TP5-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	26.0	20.2	30.2
265	24.3	18.2	27.2

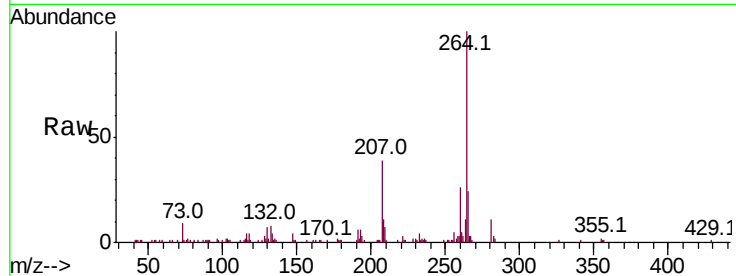

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

