

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
 Data File : BM022483.D
 Acq On : 01 Sep 2019 18:49
 Operator : HP/JU
 Sample : K4555-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-14

Quant Time: Sep 02 04:30:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 02 03:54:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	10000	20.00	ng	0.00
21) Naphthalene-d8	10.29	136	34356	20.00	ng	0.00
39) Acenaphthene-d10	14.17	164	22543	20.00	ng	0.00
64) Phenanthrene-d10	16.94	188	51643	20.00	ng	0.00
76) Chrysene-d12	21.16	240	78253	20.00	ng	0.00
87) Perylene-d12	23.34	264	96907	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	37002	64.95	ng	0.00
7) Phenol-d6	6.71	99	26841	35.23	ng	0.00
23) Nitrobenzene-d5	8.68	82	75743	96.56	ng	0.00
42) 2,4,6-Tribromophenol	15.69	330	58801	127.47	ng	0.00
45) 2-Fluorobiphenyl	12.77	172	170087	85.47	ng	0.00
79) Terphenyl-d14	19.59	244	508336	85.73	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
Data File : BM022483.D
Acq On : 01 Sep 2019 18:49
Operator : HP/JU
Sample : K4555-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-14

Quant Time: Sep 02 04:30:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 02 03:54:42 2019
Response via : Initial Calibration

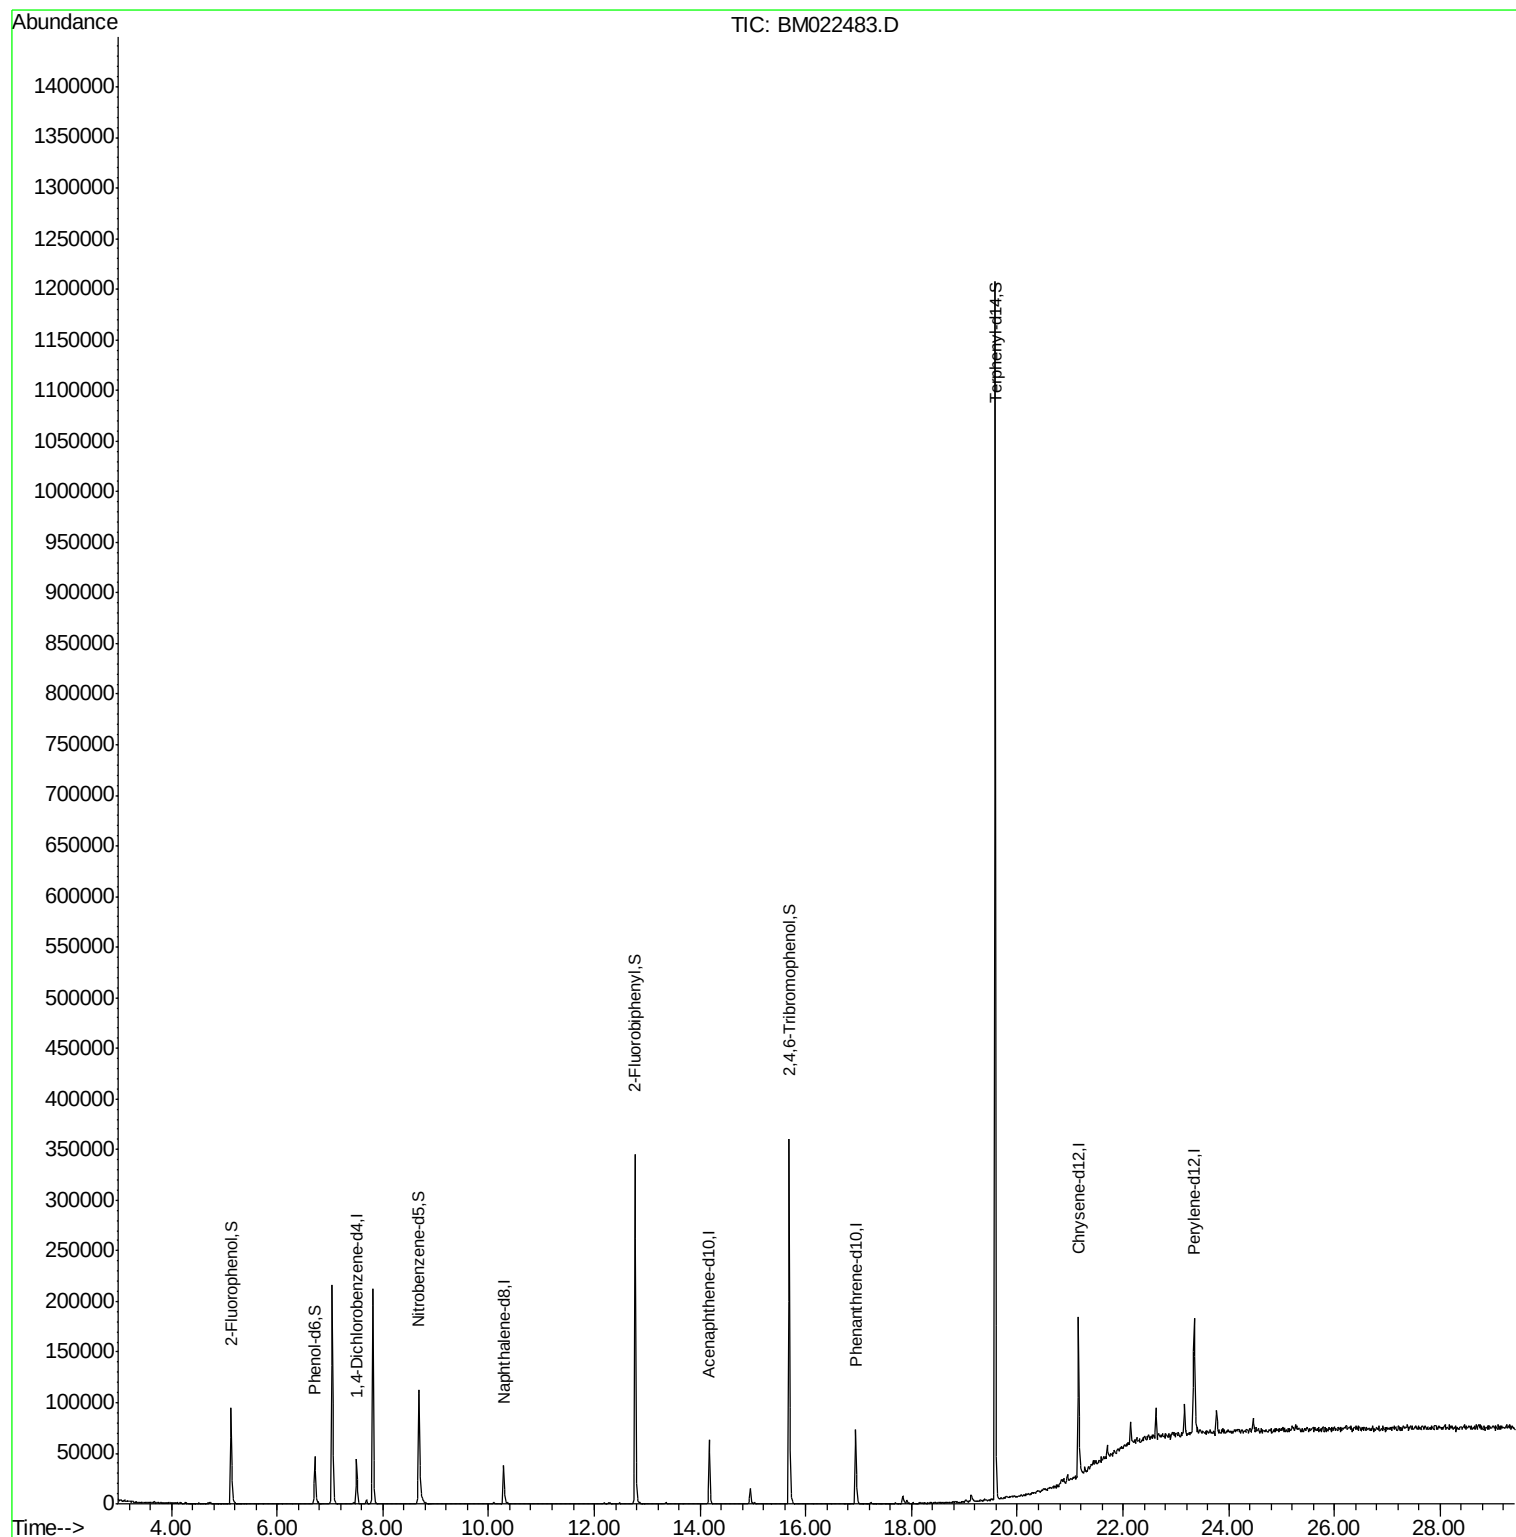

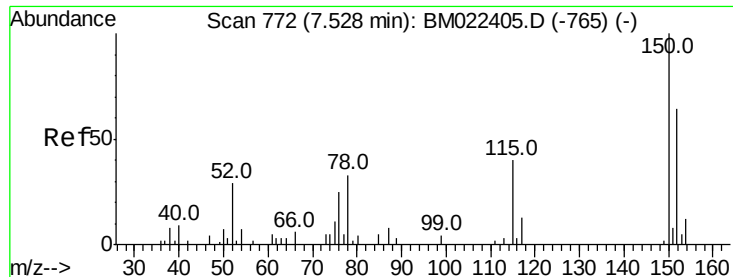


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.51 min Scan# 769
Delta R.T. -0.00 min
Lab File: BM022483.D
Acq: 01 Sep 2019 18:49

Instrument :
BNA_M
ClientSampleId :
TW-14

Tot Ion:152 Resp: 10000
Ion Ratio Lower Upper
152 100
150 149.9 125.4 188.0
115 65.5 50.3 75.5

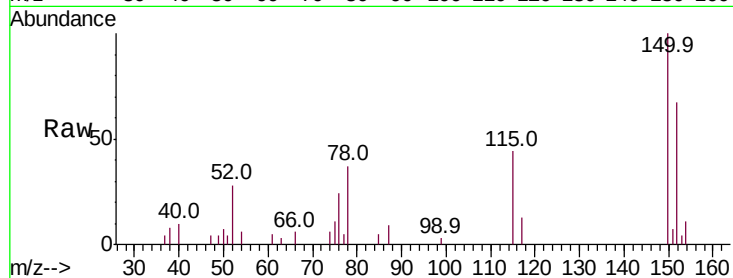


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

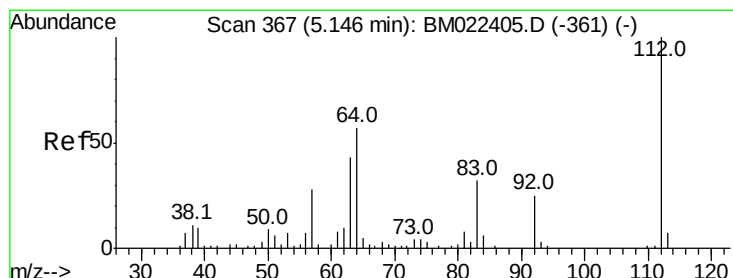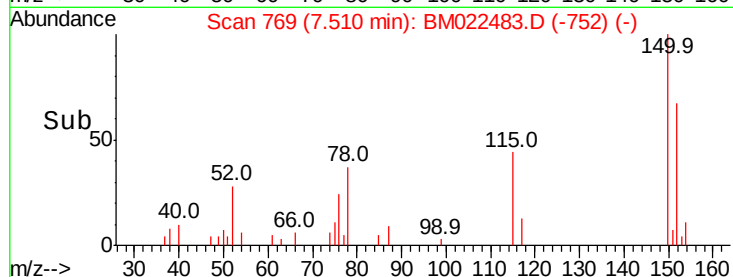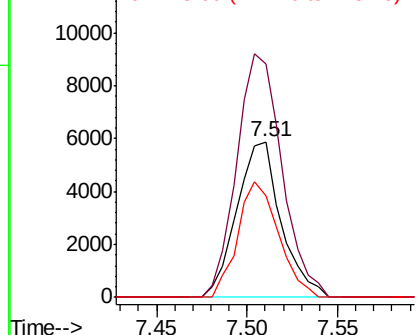



#5


2-Fluorophenol
Concen: 64.951 ng
RT: 5.13 min Scan# 365
Delta R.T. 0.01 min
Lab File: BM022483.D
Acq: 01 Sep 2019 18:49

Tgt Ion:112 Resp: 37002
Ion Ratio Lower Upper
112 100
64 63.4 45.4 68.2
63 40.5 34.5 51.7

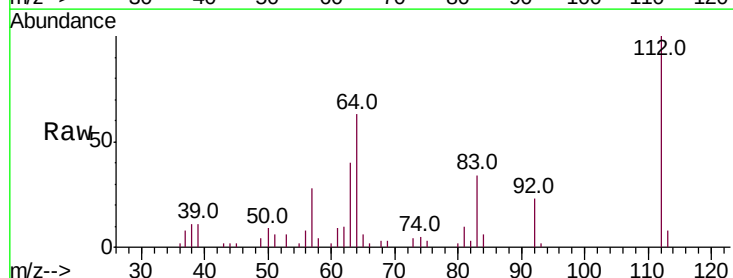

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

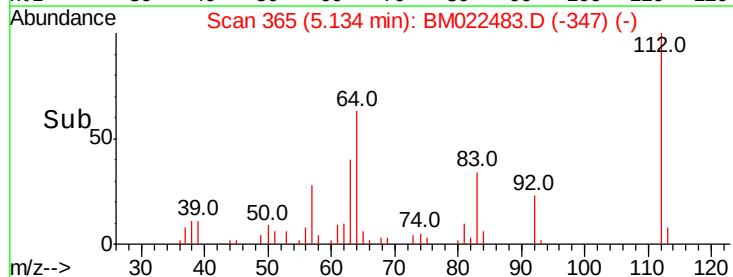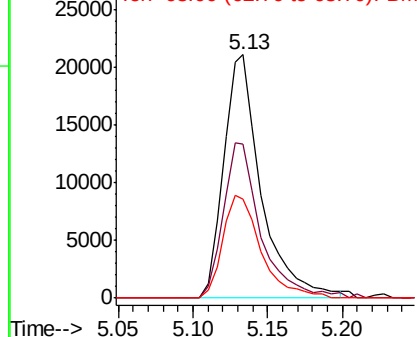

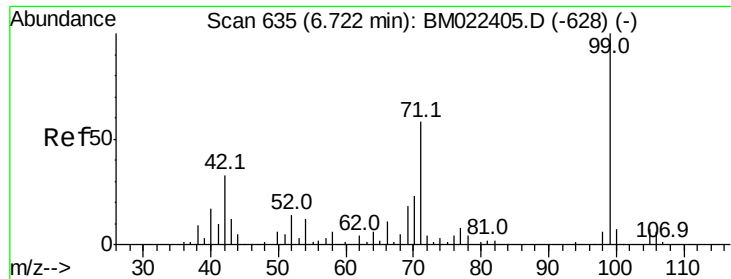

#7

Phenol-d6

Concen: 35.232 ng

RT: 6.71 min Scan# 633

Delta R.T. -0.00 min

Lab File: BM022483.D

Acq: 01 Sep 2019 18:49

Instrument :

BNA_M

ClientSampleId :

TW-14


Tot Ion: 99 Resp: 26841

Ion Ratio Lower Upper

99 100

42 32.6 26.3 39.5




71 60.1 46.6 69.8

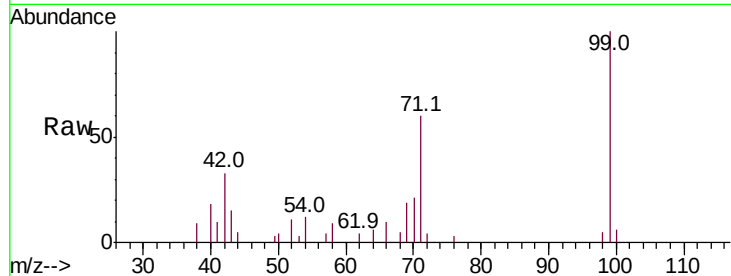

Abundance Ion 99.00 (98.70 to 99.70): BM022405.D (-628) (-)

Ion 42.00 (41.70 to 42.70): BM022405.D (-628) (-)

Ion 71.00 (70.70 to 71.70): BM022405.D (-628) (-)

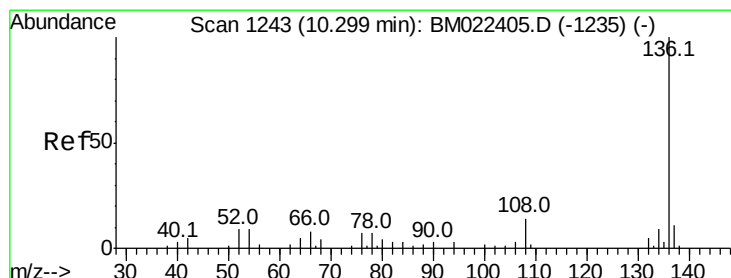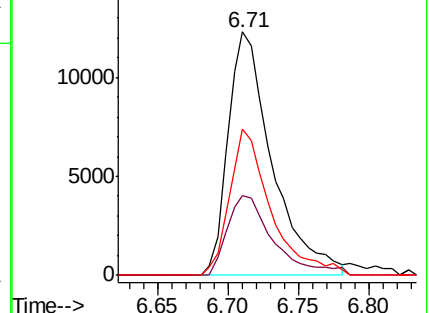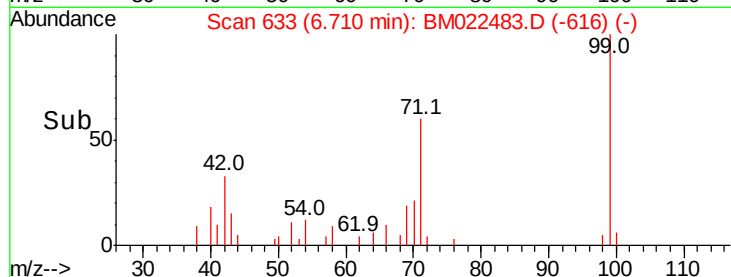

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.29 min Scan# 1241

Delta R.T. 0.01 min

Lab File: BM022483.D

Acq: 01 Sep 2019 18:49

Tgt Ion: 136 Resp: 34356


Ion Ratio Lower Upper

136 100

137 11.3 8.6 13.0

54 8.6 7.0 10.6

68 4.7 2.9 4.3#


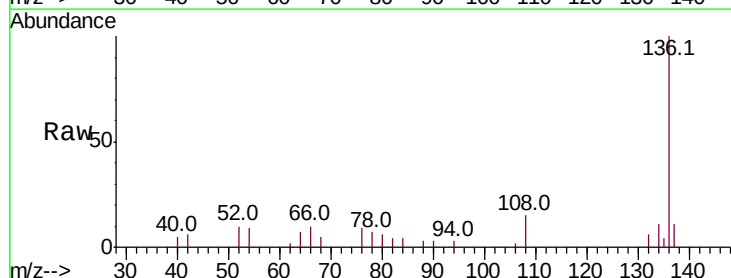



Abundance Ion 136.00 (135.70 to 136.70): BM022405.D (-1235) (-)

Ion 137.00 (136.70 to 137.70): BM022405.D (-1235) (-)

Ion 54.00 (53.70 to 54.70): BM022405.D (-1235) (-)

Ion 68.00 (67.70 to 68.70): BM022405.D (-1235) (-)



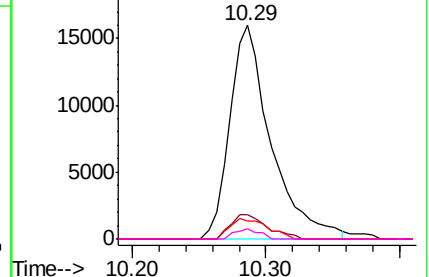
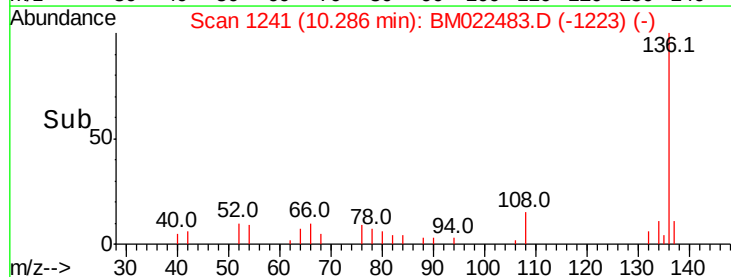


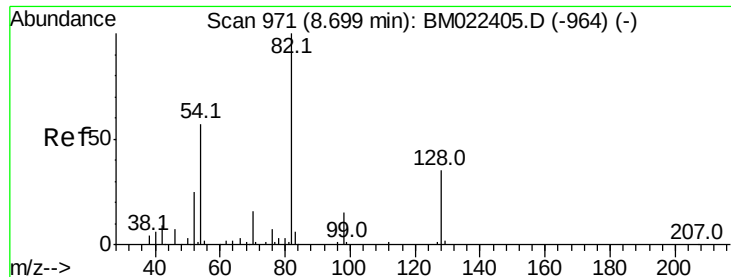

#23
Nitrobenzene-d5
Concen: 96.565 ng
RT: 8.68 min Scan# 968
Delta R.T. -0.00 min
Lab File: BM022483.D
Acq: 01 Sep 2019 18:49




Instrument :
BNA_M
ClientSampleId :
TW-14


Tot Ion	82	Resp	75743
Ion Ratio	Lower	Upper	
82	100		
128	36.2	27.9	41.9
54	55.8	45.2	67.8

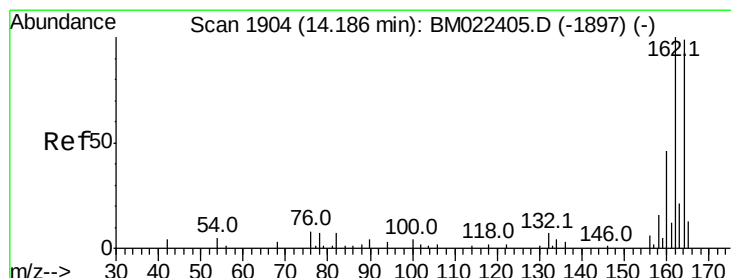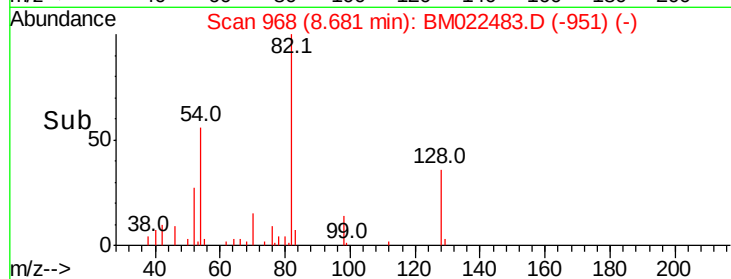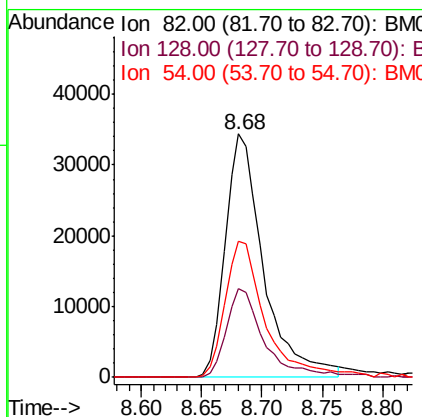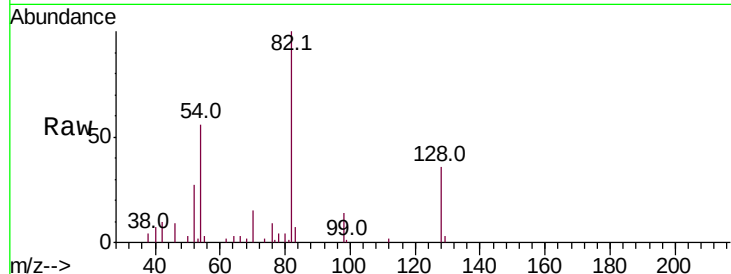

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.17 min Scan# 1902
Delta R.T. 0.01 min
Lab File: BM022483.D
Acq: 01 Sep 2019 18:49

Tgt Ion	164	Resp	22543
Ion Ratio	Lower	Upper	
164	100		
162	110.9	80.6	121.0
160	51.3	37.3	55.9

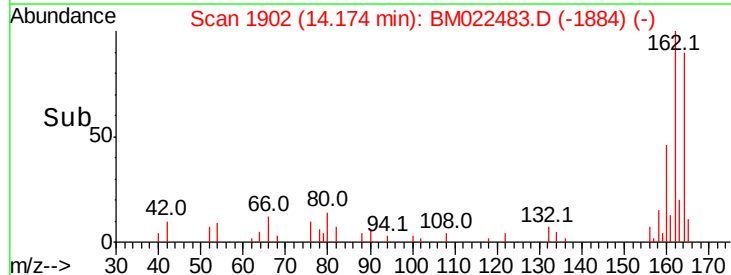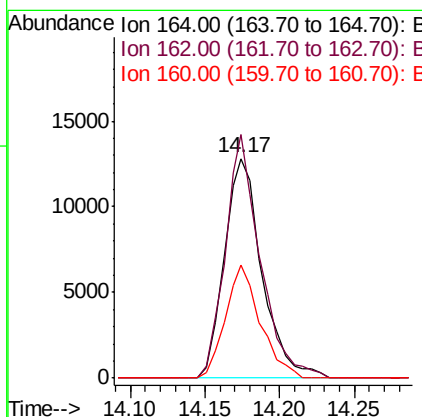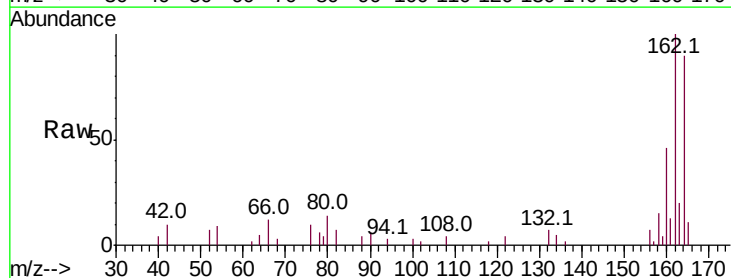


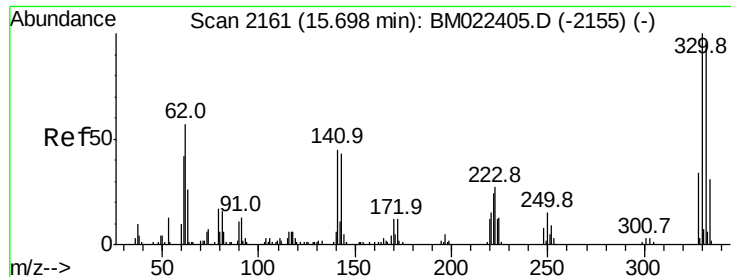




#42
 2,4,6-Tribromophenol
 Concen: 127.470 ng
 RT: 15.69 min Scan# 2159
 Delta R.T. -0.00 min
 Lab File: BM022483.D
 Acq: 01 Sep 2019 18:49

Instrument :
 BNA_M
 ClientSampled :
 TW-14

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.8	116.8
141	52.1	35.6	53.4

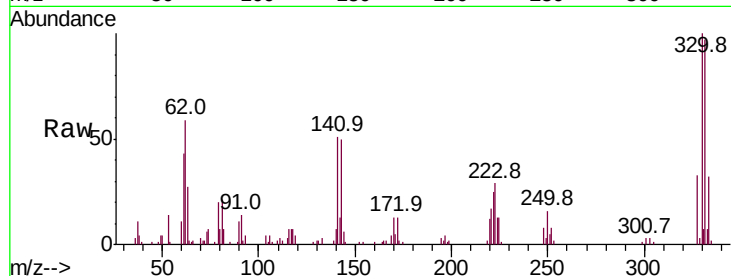


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

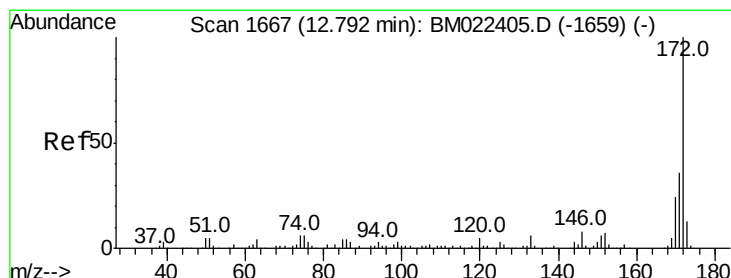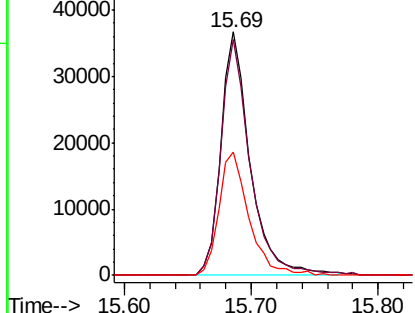
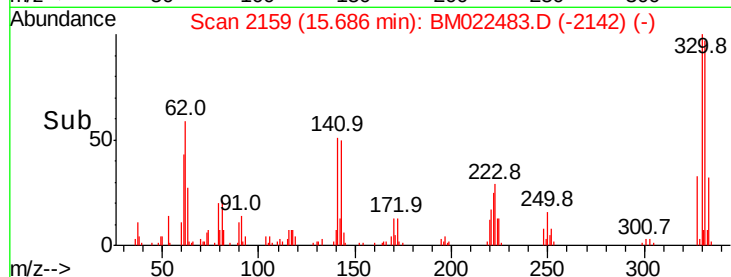



#45
 2-Fluorobiphenyl
 Concen: 85.473 ng
 RT: 12.77 min Scan# 1664
 Delta R.T. -0.00 min
 Lab File: BM022483.D
 Acq: 01 Sep 2019 18:49

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.5	42.7
170	24.0	18.9	28.3

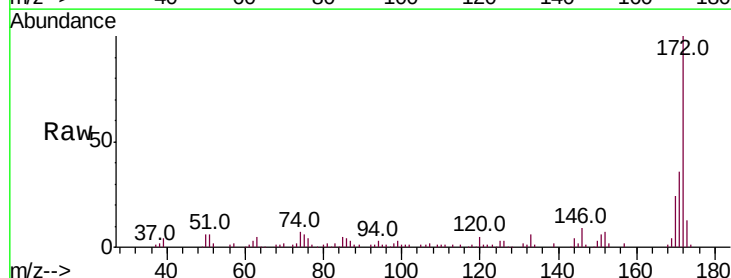

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

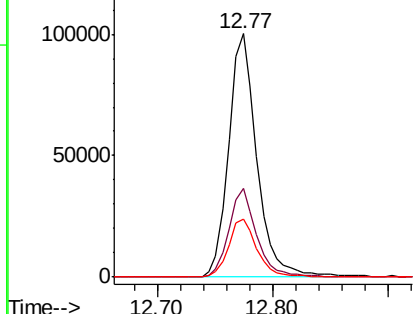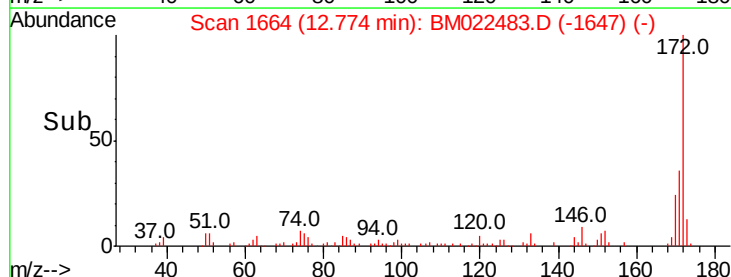

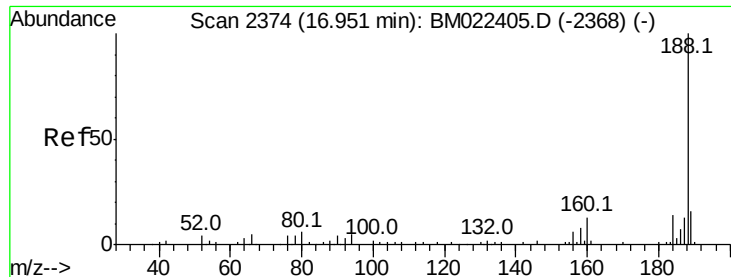

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.94 min Scan# 2373

Delta R.T. 0.01 min

Lab File: BM022483.D

Acq: 01 Sep 2019 18:49

Instrument :

BNA_M

ClientSampled :

TW-14


Tot Ion:188 Resp: 51643

Ion Ratio Lower Upper

188 100

94 6.1 4.4 6.6




80 8.6 5.0 7.6#

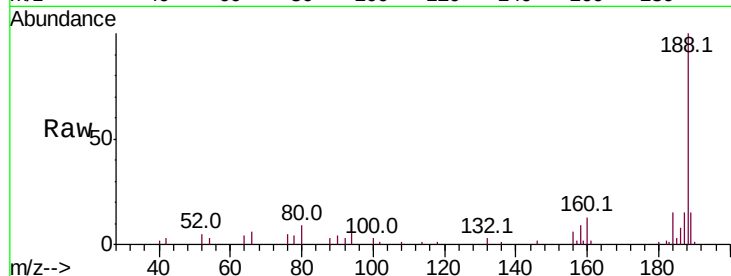

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

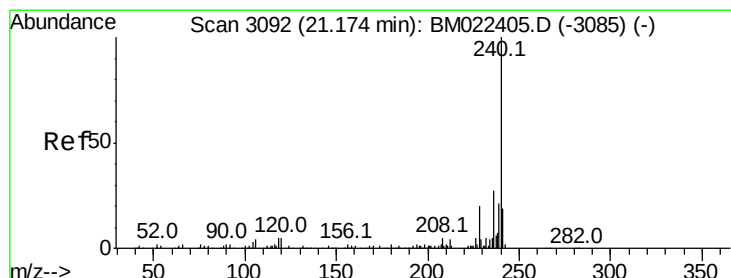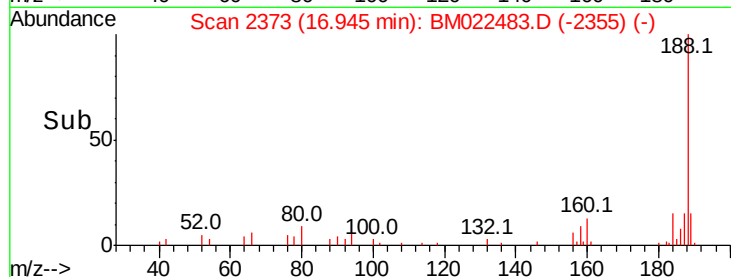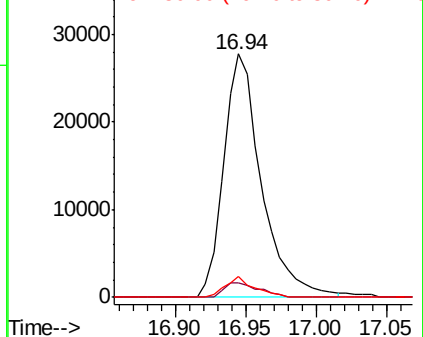

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.16 min Scan# 3090

Delta R.T. 0.01 min

Lab File: BM022483.D

Acq: 01 Sep 2019 18:49


Tgt Ion:240 Resp: 78253

Ion Ratio Lower Upper

240 100

120 5.3 3.9 5.9



236 28.1 21.4 32.2

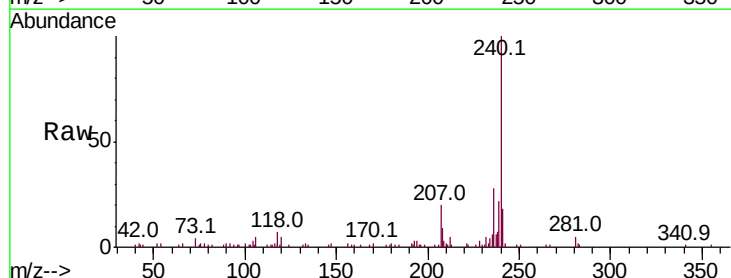


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



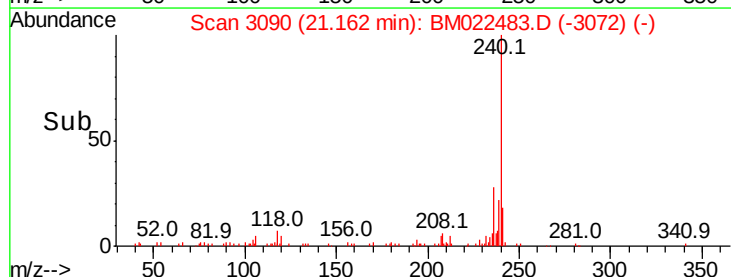
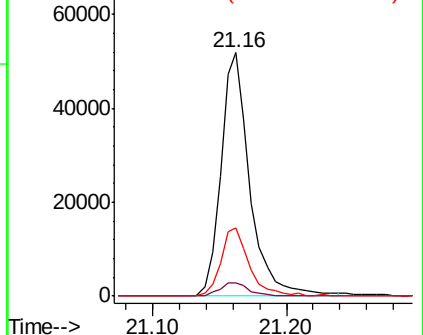


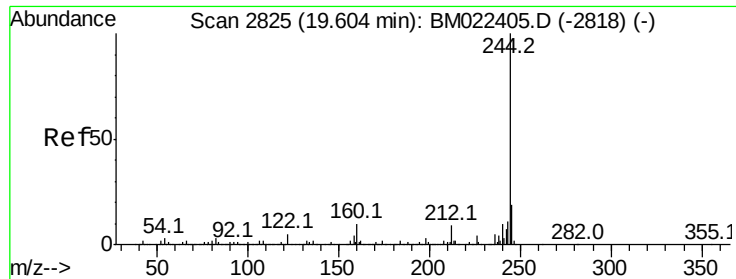

#79
 Terphenyl-d14
 Concen: 85.732 ng
 RT: 19.59 min Scan# 2822
 Delta R.T. -0.00 min
 Lab File: BM022483.D
 Acq: 01 Sep 2019 18:49

Instrument :
 BNA_M
 ClientSampled :
 TW-14

Tot Ion:	244	Resp:	508336
Ion	Ratio	Lower	Upper
244	100		
212	8.9	7.0	10.4
122	5.0	3.9	5.9

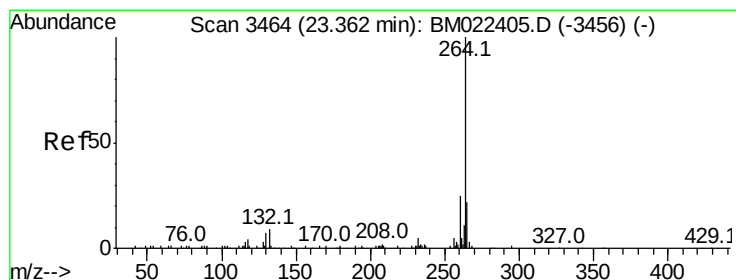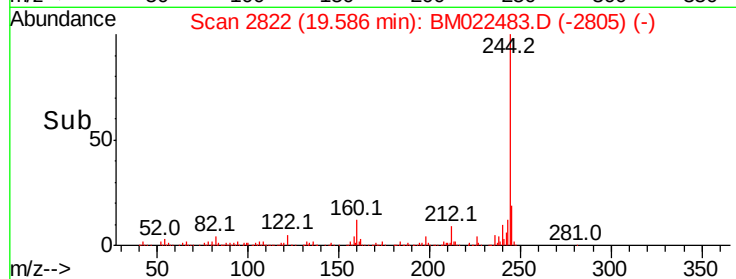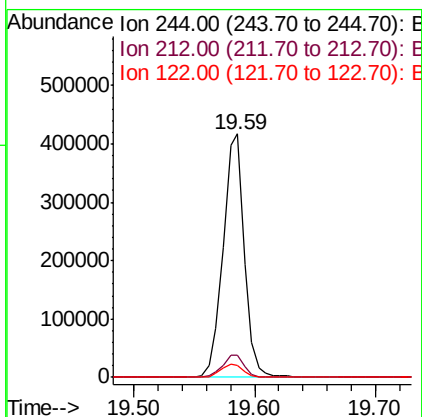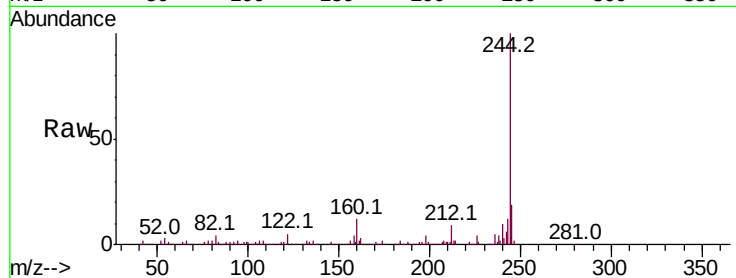

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.34 min Scan# 3461
 Delta R.T. -0.00 min
 Lab File: BM022483.D
 Acq: 01 Sep 2019 18:49

Tgt Ion:	264	Resp:	96907
Ion	Ratio	Lower	Upper
264	100		
260	24.1	20.2	30.2
265	22.9	18.2	27.2

