

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
 Data File : BM022487.D
 Acq On : 01 Sep 2019 21:16
 Operator : HP/JU
 Sample : K4555-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	359	364	380	rBV	105690	169238	11.36%	3.547%
2	6.710	628	633	647	rBV	51726	103611	6.96%	2.171%
3	7.040	684	689	706	rBB	224420	370988	24.91%	7.775%
4	7.504	763	768	776	rBB	50029	72196	4.85%	1.513%
5	7.810	815	820	831	rBB	212627	350034	23.50%	7.336%
6	8.681	962	968	989	rBV	114387	248282	16.67%	5.203%
7	10.287	1235	1241	1258	rBB	34513	77836	5.23%	1.631%
8	12.775	1658	1664	1684	rBV	341146	575512	38.64%	12.061%
9	14.175	1897	1902	1913	rBB2	64033	107026	7.19%	2.243%
10	15.686	2153	2159	2179	rBB	343419	579715	38.92%	12.149%
11	16.945	2368	2373	2385	rBV	73747	133826	8.99%	2.805%
12	19.580	2816	2821	2829	rBV	1243154	1489356	100.00%	31.213%
13	21.156	3085	3089	3098	rBV	158212	232066	15.58%	4.863%
14	23.339	3455	3460	3472	rVB	118572	261929	17.59%	5.489%


Sum of corrected areas: 4771615

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
Data File : BM022487.D
Acq On : 01 Sep 2019 21:16
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

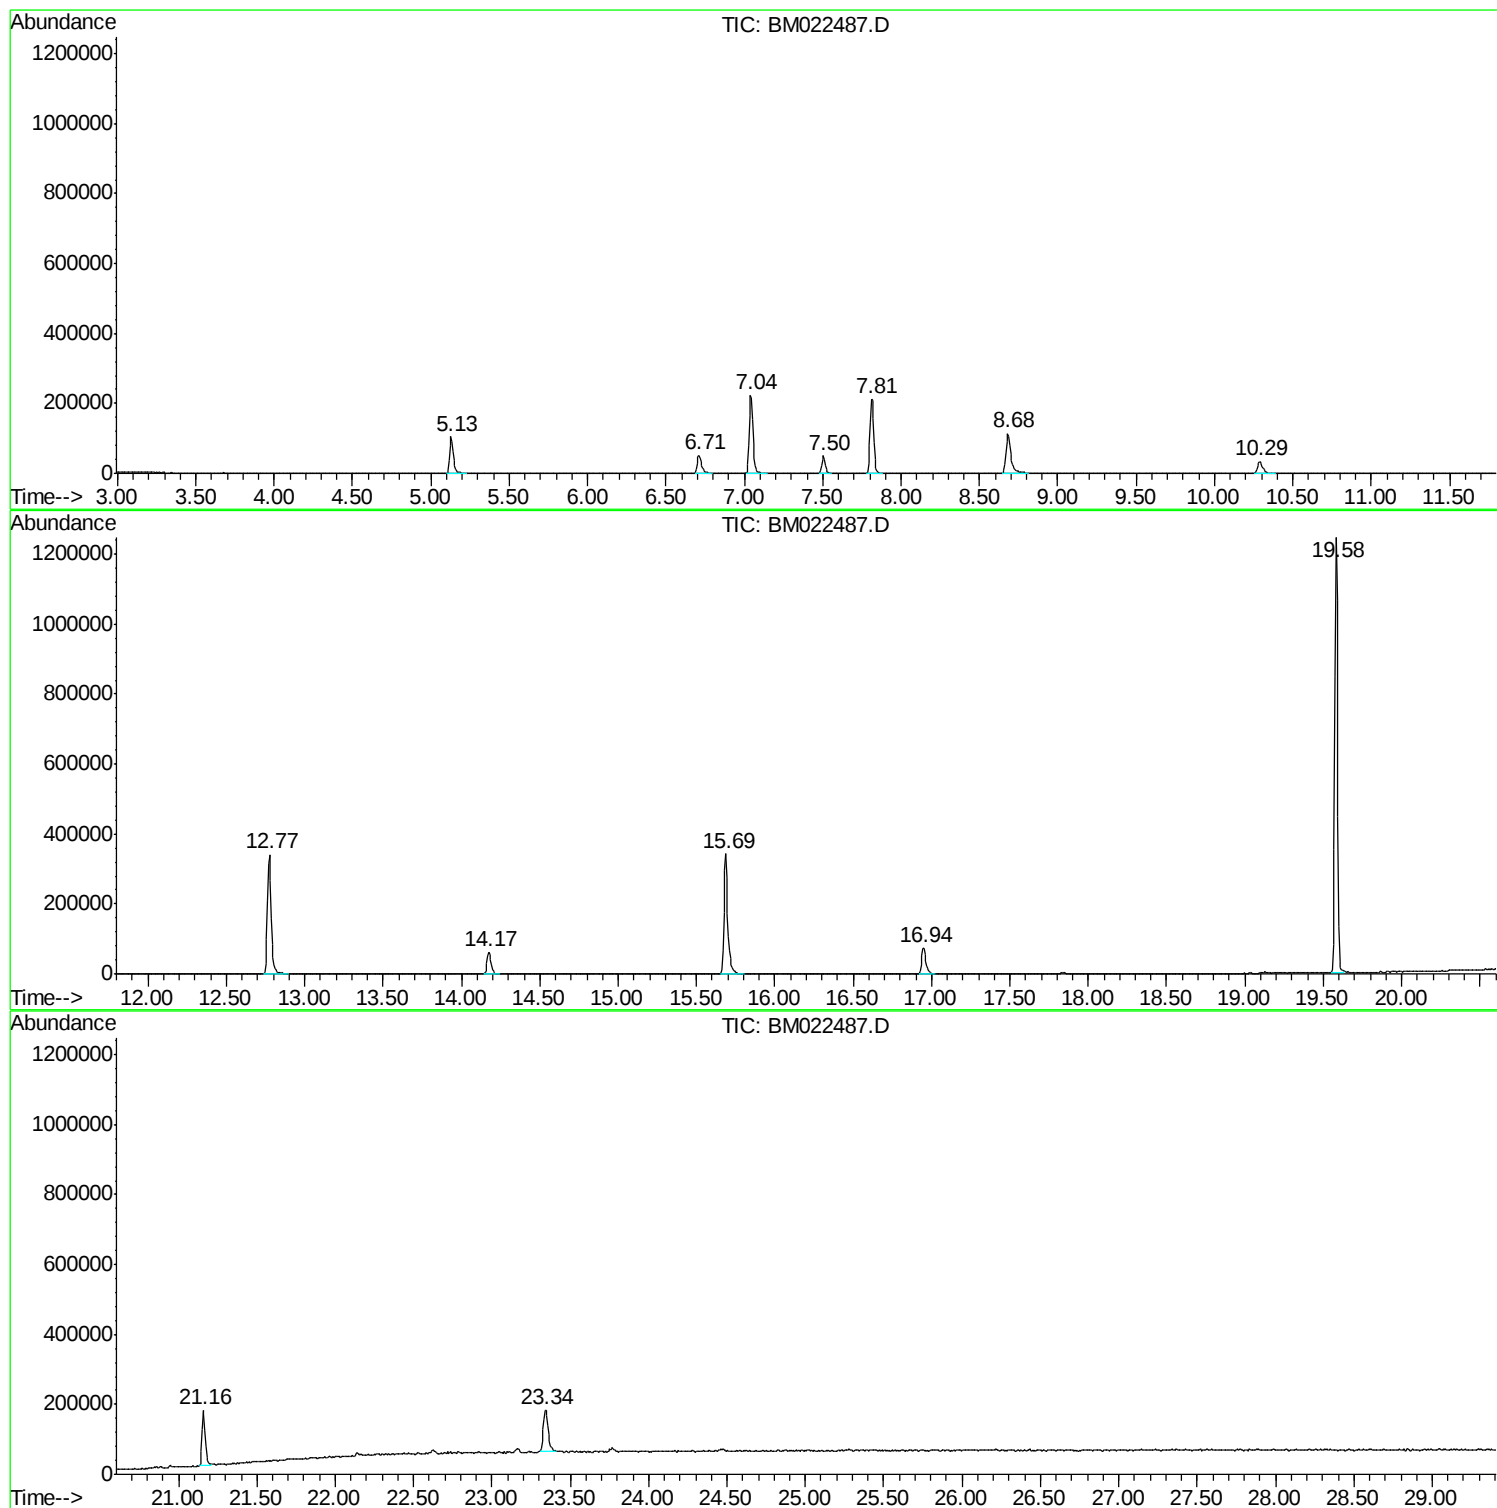

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
Data File : BM022487.D
Acq On : 01 Sep 2019 21:16
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	102.77 ng	370988	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

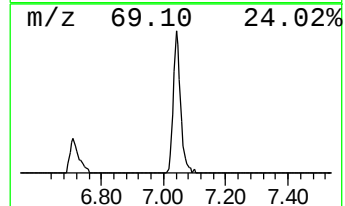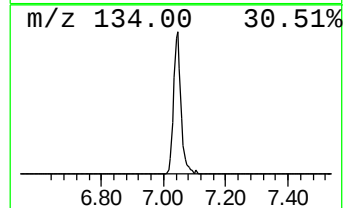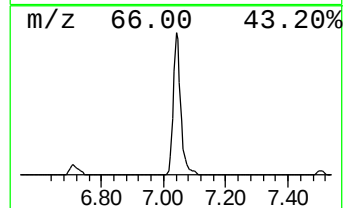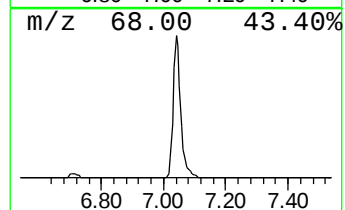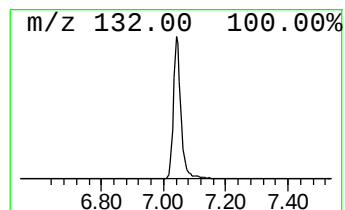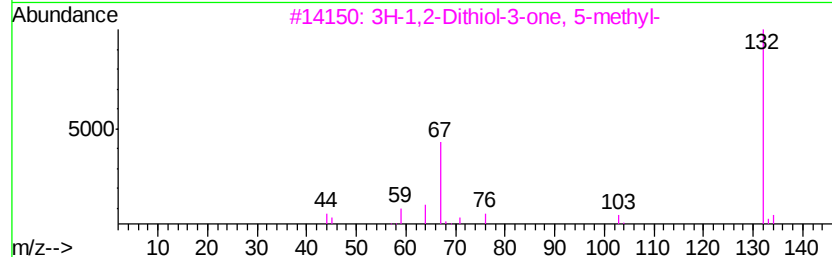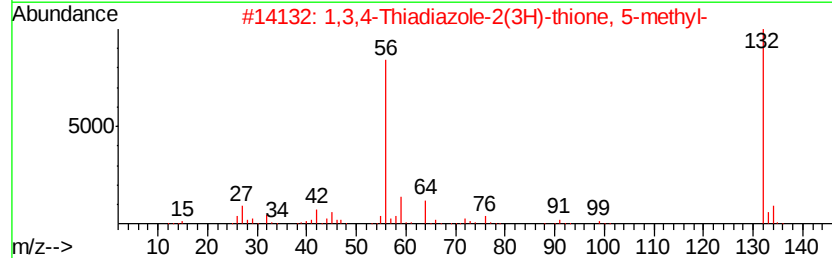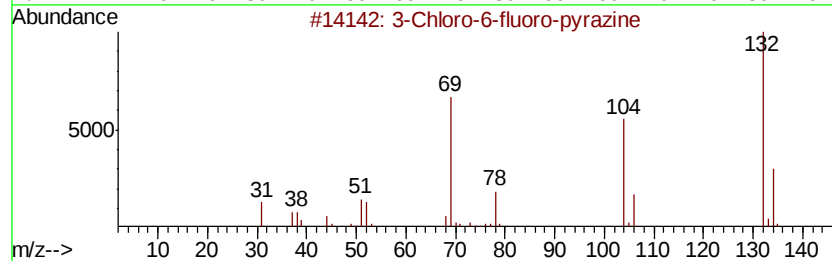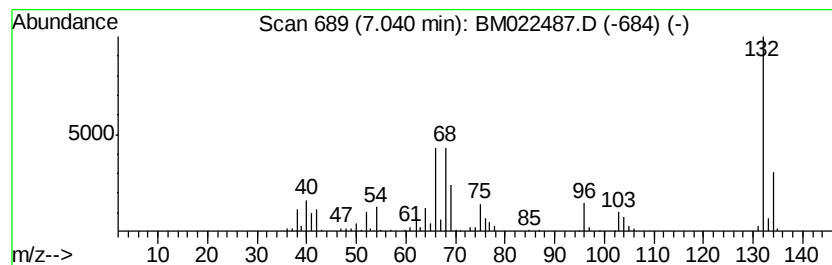

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090119\
Data File : BM022487.D
Acq On : 01 Sep 2019 21:16
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	102.8	ng	370988	1	7.50	72196	20.0