


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090119\
 Data File : BM022474.D
 Acq On : 01 Sep 2019 12:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 02 03:54:42 2019

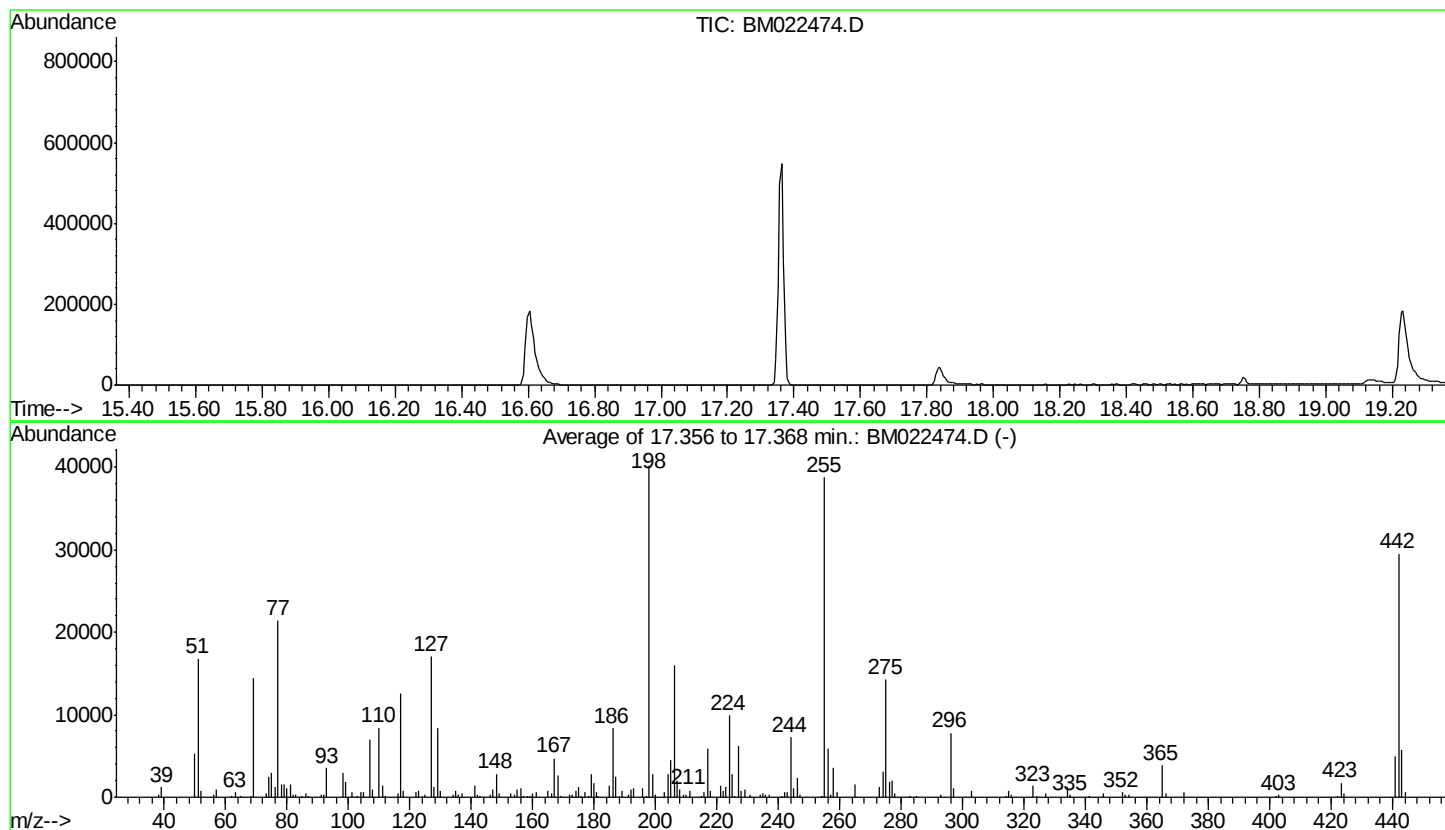

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	16837	PASS
68	69	0.00	2	1.6	230	PASS
69	198	0.00	100	35.9	14445	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	17060	PASS
197	198	0.00	2	0.3	131	PASS
198	198	100	100	100.0	40216	PASS
199	198	5	9	7.0	2819	PASS
275	198	10	60	35.4	14243	PASS
365	198	1	100	9.6	3880	PASS
441	198	0.01	100	12.2	4904	PASS
442	198	50	100	73.5	29549	PASS
443	442	15	24	19.3	5710	PASS