

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
 Data File : BM036475.D
 Acq On : 01 Sep 2022 16:23
 Operator : CG/JU
 Sample : PB147416BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Quant Time: Sep 02 01:35:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	187397	20.000	ng/u1	0.00
20) Naphthalene-d8	10.522	136	853090	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.374	164	528627	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.121	188	1099231	20.000	ng/u1	0.00
79) Chrysene-d12	21.309	240	1112552	20.000	ng/u1	0.00
88) Perylene-d12	23.609	264	1132543	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	30385	6.179	ng/uL	0.00
4) Pyridine-d5	3.551	84	395446	29.163	ng/u1	0.00
7) Phenol-d5	6.898	99	503605	31.483	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.057	67	357462	35.502	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.251	132	438195	34.866	ng/u1	0.00
15) 4-Methylphenol-d8	8.445	113	422438	35.370	ng/u1	0.00
21) Nitrobenzene-d5	8.892	128	218167	33.730	ng/u1	0.00
24) 2-Nitrophenol-d4	9.610	143	222641	33.935	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.145	165	379414	32.365	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	341167	18.773	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	1306718	39.073	ng/u1	0.00
49) Acenaphthylene-d8	14.068	160	1552411	37.217	ng/u1	0.00
54) 4-Nitrophenol-d4	14.721	143	570	0.090	ng/u1	0.12
60) Fluorene-d10	15.368	176	1166761	38.609	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	174876	30.944	ng/u1	0.00
73) Anthracene-d10	17.221	188	1854895	37.950	ng/u1	0.00
81) Pyrene-d10	19.521	212	2196724	38.063	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.462	264	2125807	38.283	ng/u1	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.445	70	11296	1.181	ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
Data File : BM036475.D
Acq On : 01 Sep 2022 16:23
Operator : CG/JU
Sample : PB147416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416


Quant Time: Sep 02 01:35:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration

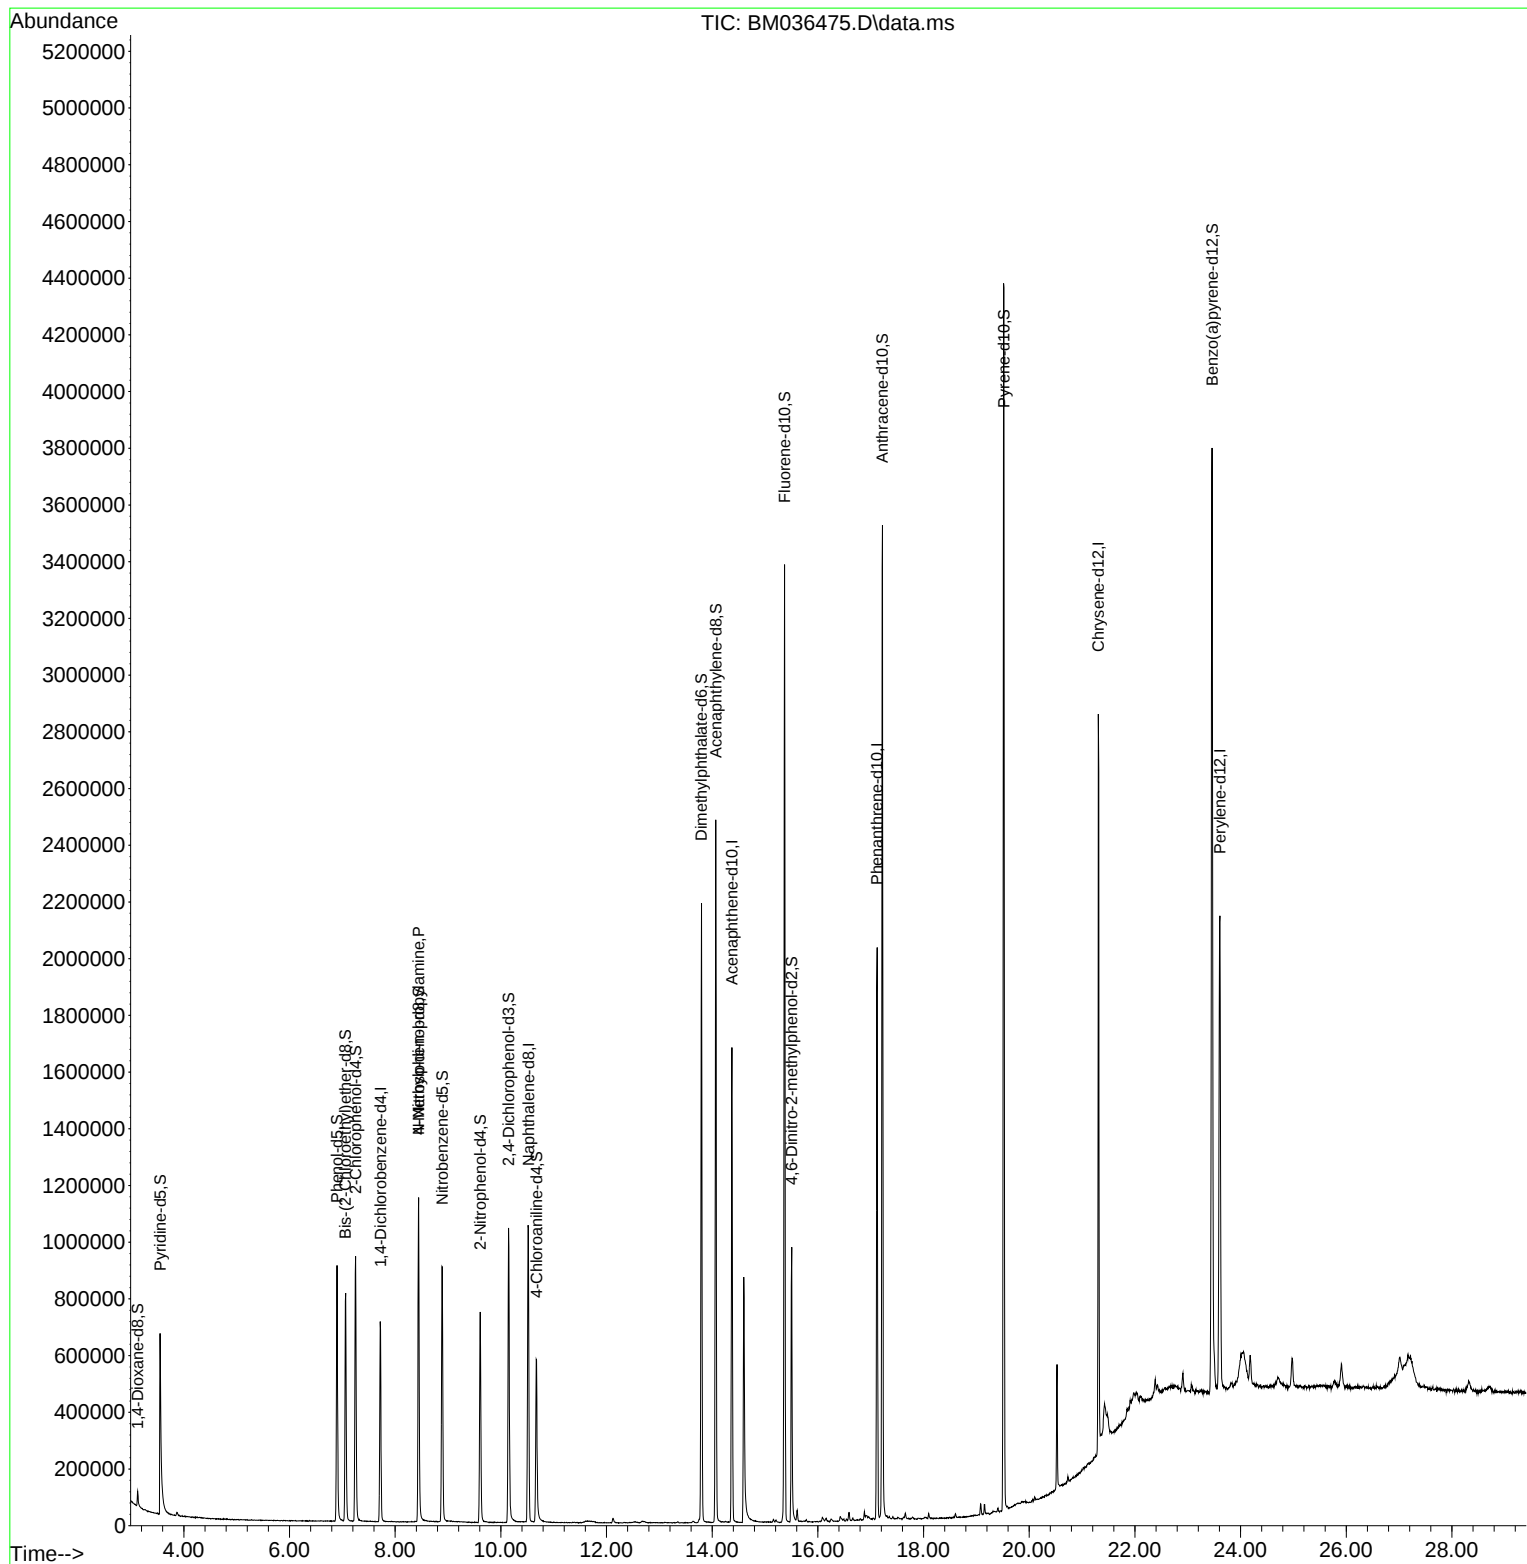

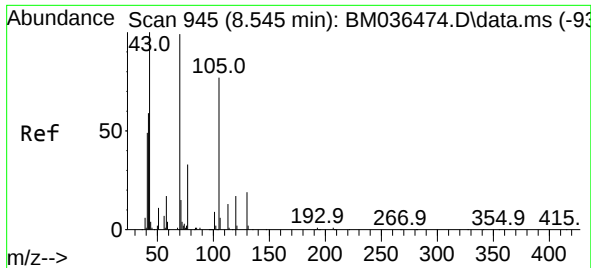

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.181 ng/ul
 RT: 8.445 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BM036475.D
 Acq: 01 Sep 2022 16:23

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

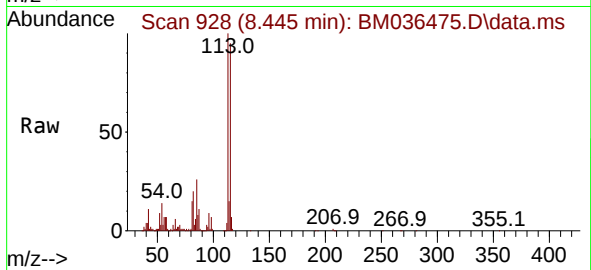

Tgt Ion: 70 Resp: 11296
 Ion Ratio Lower Upper
 70 100
 42 395.2 49.6 74.4#
 101 0.0 8.1 12.1#
 130 0.0 18.4 27.6#

