

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
 Data File : BM036480.D
 Acq On : 01 Sep 2022 19:25
 Operator : CG/JU
 Sample : N4458-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0KW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	29	rBV	40312	53419	0.76%	0.096%
2	3.563	95	98	119	rBV	178458	361556	5.13%	0.650%
3	3.781	130	135	146	rVB2	28086	53909	0.77%	0.097%
4	3.875	146	151	159	rBV	32779	49823	0.71%	0.090%
5	3.987	168	170	176	rVB6	4883	8646	0.12%	0.016%
6	4.257	214	216	223	rBV8	4155	8485	0.12%	0.015%
7	5.022	341	346	355	rVB4	8615	16308	0.23%	0.029%
8	6.851	649	657	659	rBV7	4566	7713	0.11%	0.014%
9	6.910	661	667	679	rVV	135726	241448	3.43%	0.434%
10	7.069	686	694	710	rBV	736757	1161052	16.48%	2.088%
11	7.257	720	726	736	rBV	558306	913214	12.97%	1.642%
12	7.722	799	805	815	rBV	742053	1211295	17.20%	2.178%
13	8.081	859	866	870	rBV4	9381	15326	0.22%	0.028%
14	8.451	922	929	945	rBV	484244	828071	11.76%	1.489%
15	8.892	998	1004	1019	rBV	851594	1454094	20.64%	2.615%
16	9.286	1066	1071	1077	rVB2	14920	25212	0.36%	0.045%
17	9.351	1077	1082	1087	rBV8	4882	7949	0.11%	0.014%
18	9.616	1120	1127	1139	rBV	481894	852102	12.10%	1.532%
19	10.151	1210	1218	1242	rBV	738935	1355665	19.25%	2.438%
20	10.386	1254	1258	1262	rVB4	9410	15616	0.22%	0.028%
21	10.522	1273	1281	1291	rBV	1177552	1908409	27.10%	3.432%
22	10.675	1300	1307	1327	rBV	422425	837854	11.90%	1.507%
23	10.904	1342	1346	1352	rVB9	4708	8055	0.11%	0.014%
24	11.780	1488	1495	1502	rBV	38582	63827	0.91%	0.115%
25	11.957	1521	1525	1530	rVB7	6555	9452	0.13%	0.017%
26	12.127	1548	1554	1561	rBV	17118	32525	0.46%	0.058%
27	12.727	1652	1656	1660	rBV5	5623	8864	0.13%	0.016%
28	13.198	1728	1736	1743	rVB5	20679	38607	0.55%	0.069%
29	13.404	1766	1771	1780	rVB3	9568	17698	0.25%	0.032%
30	13.716	1820	1824	1831	rVB	27356	40871	0.58%	0.073%
31	13.798	1831	1838	1853	rBV	2170795	2928828	41.58%	5.267%
32	14.068	1877	1884	1896	rBV	2532116	3521966	50.00%	6.334%
33	14.374	1930	1936	1946	rBV	1879090	2618273	37.17%	4.708%
34	14.645	1977	1982	1987	rBV5	11852	26035	0.37%	0.047%
35	15.139	2061	2066	2068	rBV2	6586	10185	0.14%	0.018%
36	15.174	2068	2072	2076	rVV	23856	34046	0.48%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
 Data File : BM036480.D
 Acq On : 01 Sep 2022 19:25
 Operator : CG/JU
 Sample : N4458-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0KW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	15.221	2076	2080	2086	rVB5	6230	13778	0.20%	0.025%
38	15.368	2095	2105	2114	rBV	3031933	4241131	60.21%	7.627%
39	15.515	2124	2130	2141	rBV6	13695	36852	0.52%	0.066%
40	15.615	2143	2147	2154	rVB3	15080	25885	0.37%	0.047%
41	16.086	2224	2227	2235	rBV5	9307	15515	0.22%	0.028%
42	16.157	2237	2239	2247	rVB7	4856	7054	0.10%	0.013%
43	16.598	2308	2314	2318	rBV3	9687	16636	0.24%	0.030%
44	16.804	2345	2349	2355	rBV7	3782	7493	0.11%	0.013%
45	16.880	2358	2362	2365	rBV4	13698	20065	0.28%	0.036%
46	16.909	2365	2367	2375	rVB7	5384	10393	0.15%	0.019%
47	17.121	2397	2403	2411	rBV	2272268	3081829	43.75%	5.542%
48	17.221	2413	2420	2436	rVV	4446092	5893235	83.67%	10.598%
49	17.415	2450	2453	2457	rVB4	5965	7117	0.10%	0.013%
50	17.621	2485	2488	2490	rBV3	6897	7680	0.11%	0.014%
51	17.662	2492	2495	2500	rVB4	6953	8517	0.12%	0.015%
52	18.027	2555	2557	2561	rBV4	5819	8334	0.12%	0.015%
53	18.098	2566	2569	2576	rVB	13888	18661	0.26%	0.034%
54	18.315	2604	2606	2611	rBV6	6535	9580	0.14%	0.017%
55	18.498	2634	2637	2641	rBV6	17255	21548	0.31%	0.039%
56	18.603	2652	2655	2658	rBV4	6345	9028	0.13%	0.016%
57	19.080	2732	2736	2741	rBV2	48158	65425	0.93%	0.118%
58	19.150	2745	2748	2753	rBV	45055	59752	0.85%	0.107%
59	19.515	2804	2810	2819	rBV	5213146	6884734	97.75%	12.381%
60	20.521	2978	2981	2987	rBV	169291	200563	2.85%	0.361%
61	21.309	3110	3115	3122	rBV	2950761	3580336	50.83%	6.439%
62	23.450	3473	3479	3495	rVB2	3768075	7043396	100.00%	12.666%
63	23.597	3498	3504	3514	rVB2	1909518	3566617	50.64%	6.414%




Sum of corrected areas: 55607552

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
Data File : BM036480.D
Acq On : 01 Sep 2022 19:25
Operator : CG/JU
Sample : N4458-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

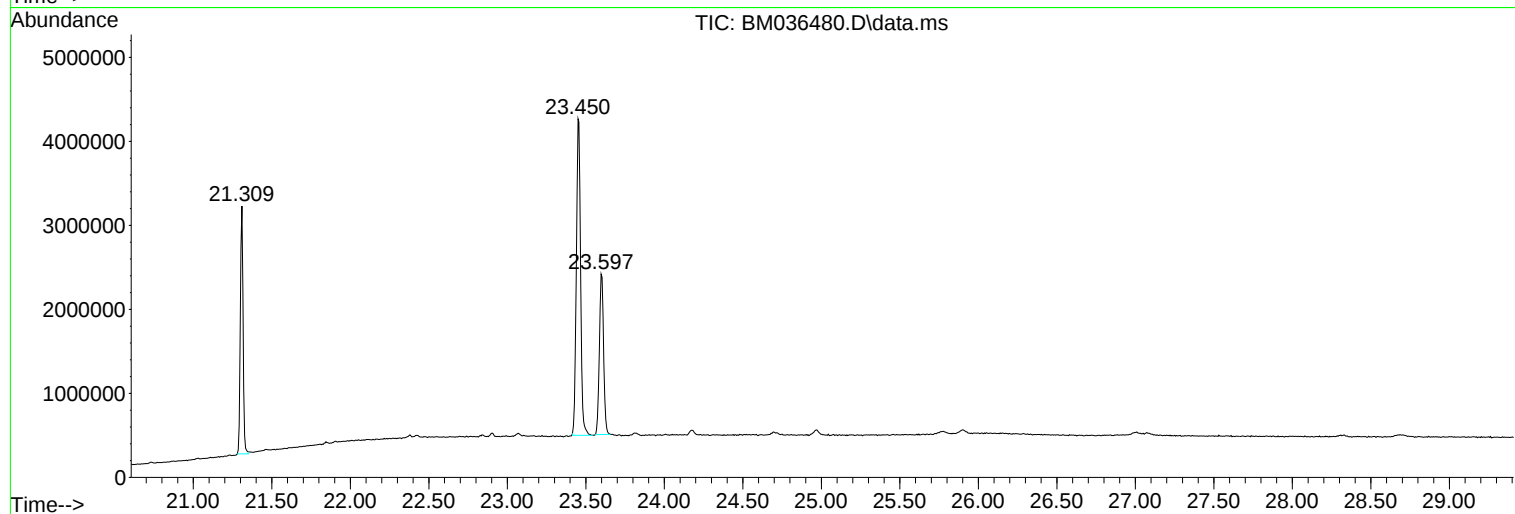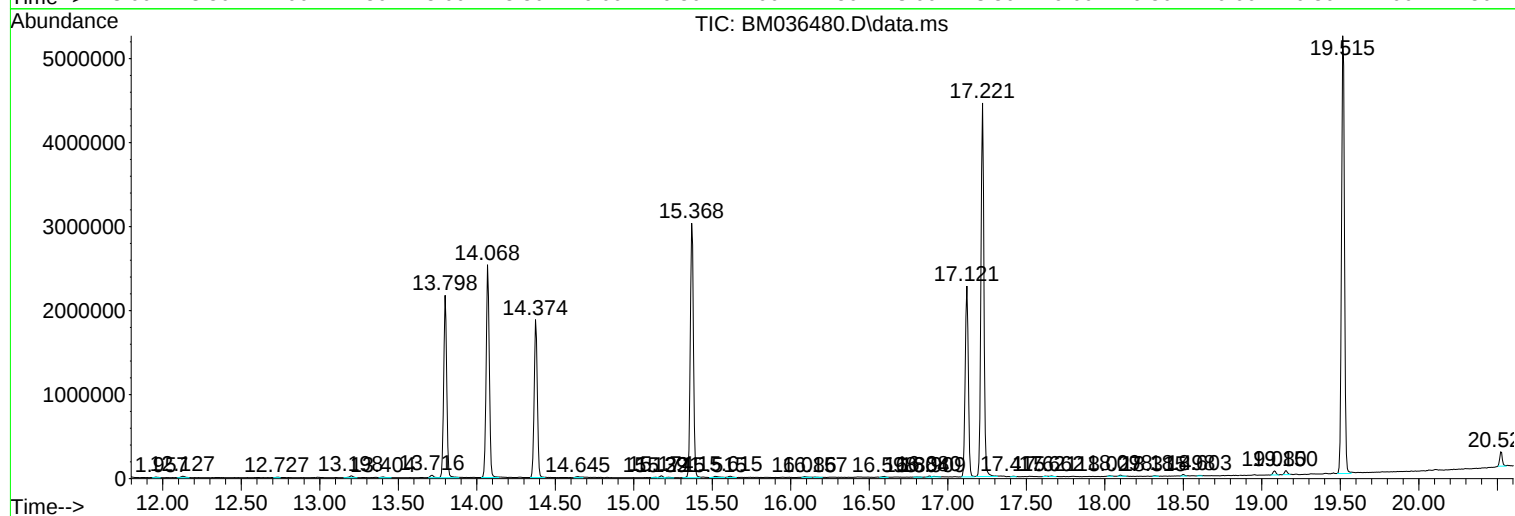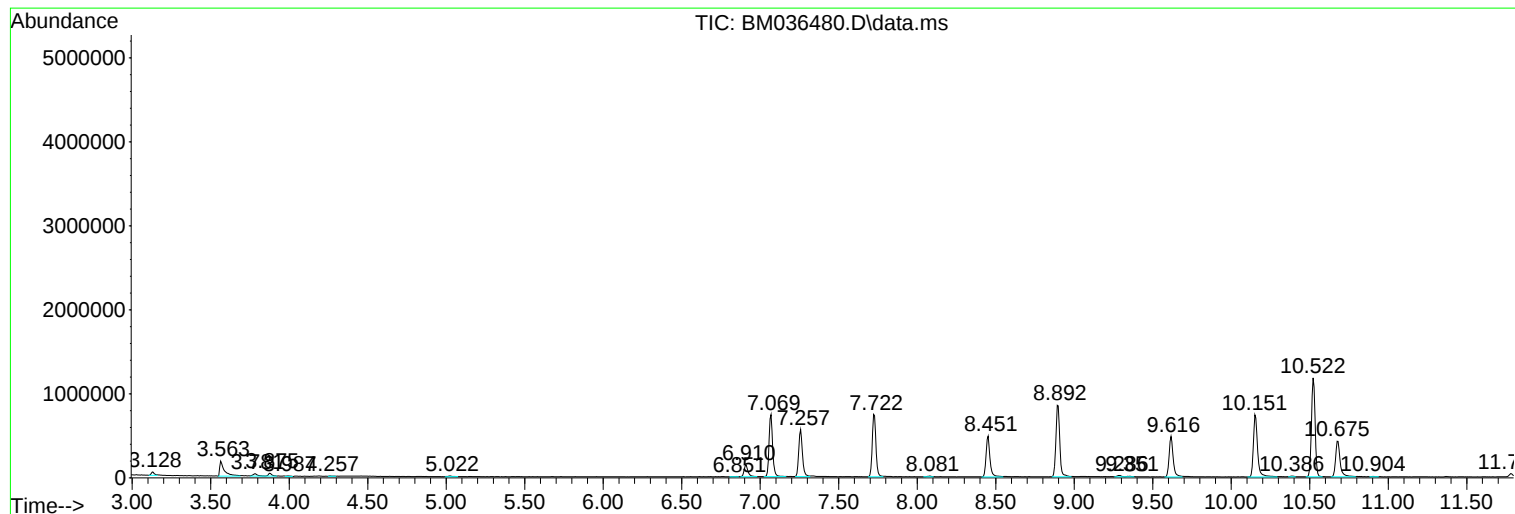

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
Data File : BM036480.D
Acq On : 01 Sep 2022 19:25
Operator : CG/JU
Sample : N4458-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090122\
Data File : BM036480.D
Acq On : 01 Sep 2022 19:25
Operator : CG/JU
Sample : N4458-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc