


Data Path : Z:\HPCHEM1\BNA_M\Data\BM090215\
Data File : BM002638.D
Acq On : 02 Sep 2015 10:58
Operator : UM/IZ
Sample : DFTPP10
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP10

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Title : SVOA CALIBRATION
Last Update : Wed Sep 02 17:21:03 2015

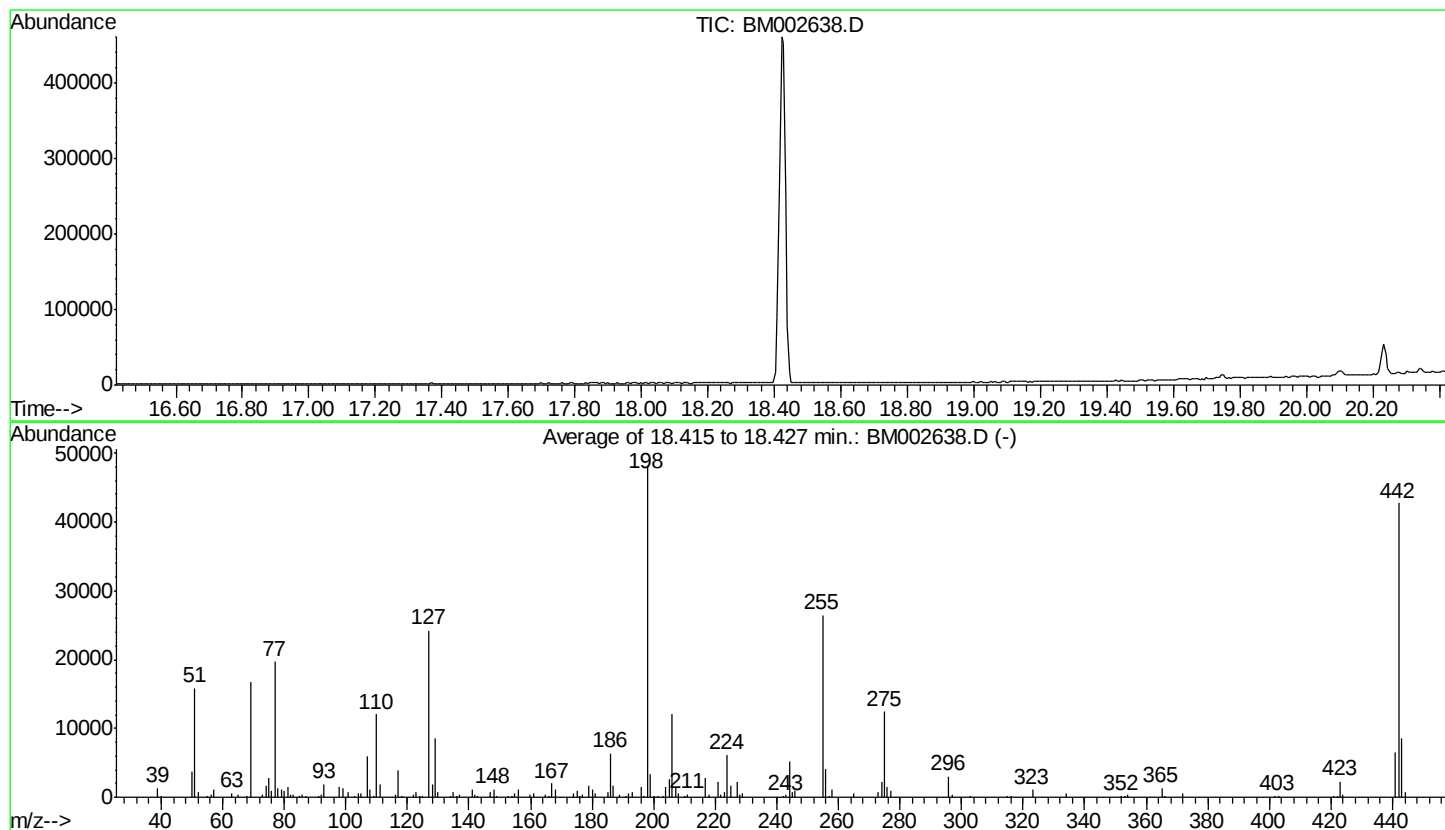

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	15872	PASS
68	69	0.00	2	0.7	124	PASS
69	198	0.00	100	34.9	16837	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	24218	PASS
197	198	0.00	2	0.5	236	PASS
198	198	100	100	100.0	48184	PASS
199	198	5	9	7.0	3367	PASS
275	198	10	60	25.7	12381	PASS
365	198	1	100	2.8	1338	PASS
441	443	0.01	100	75.6	6463	PASS
442	198	50	100	88.7	42762	PASS
443	442	15	24	20.0	8544	PASS

m/z	Abundance
39.00	1080.0
40.00	438.0
44.00	1879.0
50.00	2933.0
51.10	12688.0
52.00	620.0
55.00	310.0
56.00	424.0
57.00	928.0
62.90	488.0
65.10	334.0
69.00	13376.0
73.00	346.0
74.00	1314.0
75.00	2266.0
76.00	678.0
77.00	15481.0
78.10	1068.0
78.90	959.0
80.00	655.0
81.00	1068.0
81.90	354.0
82.90	340.0
85.90	301.0
92.00	350.0
93.00	1463.0
98.00	1252.0
99.00	1106.0
100.90	506.0
103.90	398.0
105.00	375.0
107.00	4486.0
108.00	714.0
110.00	9384.0
111.00	1494.0
117.00	3027.0
121.90	337.0
123.00	440.0
127.00	17752.0
128.00	1299.0
129.00	6519.0
130.00	597.0
135.00	571.0
137.00	342.0
141.00	804.0
141.90	305.0
146.90	482.0
148.00	874.0
148.90	323.0
154.90	461.0
156.00	865.0
160.90	453.0
164.90	360.0
167.00	1557.0
167.90	905.0
174.00	442.0
175.00	669.0
176.80	311.0
178.90	1178.0
180.00	772.0
181.00	405.0
185.00	619.0
186.00	4447.0
187.00	1327.0
189.00	433.0
191.90	485.0
193.00	420.0
196.00	1023.0
198.00	33384.0
198.90	2432.0
203.90	961.0
205.00	1996.0
206.00	8058.0
207.00	1684.0
207.90	408.0
211.10	338.0
216.90	1883.0
217.90	307.0
221.00	1383.0
223.00	433.0
224.00	4175.0
225.00	1065.0
227.00	1404.0
228.90	420.0
244.00	3426.0
245.00	395.0
245.90	570.0
255.00	17264.0
256.00	2724.0
258.00	676.0
265.00	405.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

272.90	463.0
274.00	1285.0
275.00	7297.0
276.00	1049.0
277.00	599.0
295.90	1946.0
323.00	603.0
334.00	352.0
365.00	664.0
371.90	388.0
423.00	1192.0
441.00	3167.0
442.00	21264.0
443.00	4300.0
444.00	385.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

m/z	Abundance
39.00	1629.0
39.90	392.0
44.00	1711.0
50.00	4627.0
51.00	19032.0
52.00	935.0
56.00	486.0
57.00	1398.0
63.00	807.0
65.00	384.0
68.10	374.0
69.00	20232.0
73.00	488.0
74.00	1799.0
75.00	3055.0
76.00	1073.0
77.00	23664.0
78.00	1490.0
79.00	1438.0
80.00	1095.0
81.00	1705.0
82.00	459.0
82.90	427.0
84.90	376.0
86.00	472.0
87.00	329.0
91.00	445.0
92.00	393.0
93.00	2262.0
98.00	1731.0
99.00	1504.0
101.00	902.0
103.00	320.0
104.00	568.0
104.90	630.0
107.00	7042.0
108.00	1315.0
109.00	316.0
110.00	14215.0
111.00	2076.0
116.00	505.0
117.00	4692.0
118.00	418.0
122.00	541.0
123.00	814.0
124.00	318.0
125.00	308.0
127.00	28608.0
128.00	2162.0
129.00	10087.0
129.90	980.0
134.00	390.0
135.00	948.0
135.90	374.0
137.00	396.0
141.00	1299.0
142.00	466.0
147.00	847.0
148.00	1307.0
152.90	410.0
153.90	357.0
154.90	681.0
156.00	1118.0
159.90	495.0
160.90	604.0
164.90	499.0
165.90	409.0
167.00	2332.0
168.00	1361.0
174.00	609.0
175.00	1086.0
176.00	400.0
176.90	529.0
179.00	1813.0
180.00	1383.0
180.90	678.0
185.00	889.0
186.00	7421.0
187.00	1838.0
189.00	387.0
191.90	536.0
193.00	765.0
195.90	1773.0
196.80	385.0
198.00	56464.0
198.90	4020.0
200.00	383.0
201.20	302.0
203.00	333.0
204.00	1920.0
205.00	3189.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

206.00	14422.0
207.00	2536.0
208.00	613.0
210.90	545.0
217.00	3113.0
218.00	428.0
221.00	2664.0
221.70	672.0
223.00	702.0
224.00	7352.0
225.00	2056.0
227.00	2821.0
227.90	509.0
228.90	656.0
241.90	382.0
243.10	411.0
244.00	6087.0
245.00	909.0
245.90	1041.0
255.00	30024.0
256.00	4681.0
257.00	407.0
257.90	1537.0
265.00	632.0
272.90	823.0
274.00	2397.0
275.00	14569.0
275.90	1898.0
276.90	1005.0
296.00	3534.0
297.00	430.0
314.90	397.0
316.00	310.0
323.00	1239.0
334.00	676.0
352.00	446.0
353.00	318.0
354.00	462.0
365.00	1554.0
372.00	685.0
402.90	309.0
421.90	360.0
423.00	2559.0
424.00	571.0
441.00	7210.0
442.00	48424.0
443.00	9792.0
444.00	850.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

m/z	Abundance
39.00	1313.0
40.00	406.0
44.00	1816.0
50.00	3779.0
51.10	15897.0
52.00	909.0
56.10	415.0
57.00	1218.0
63.00	640.0
65.00	346.0
69.00	16904.0
73.00	356.0
74.00	1760.0
75.00	2915.0
76.00	955.0
77.00	20000.0
78.00	1303.0
79.00	1210.0
80.00	963.0
81.00	1607.0
81.90	386.0
83.00	381.0
86.00	308.0
91.00	405.0
92.00	456.0
93.00	2051.0
98.00	1701.0
99.00	1315.0
100.90	853.0
104.00	511.0
104.90	454.0
107.00	6308.0
108.00	1065.0
110.00	12539.0
111.00	1873.0
116.00	434.0
117.00	4156.0
122.00	366.0
122.90	813.0
127.00	26296.0
128.00	1958.0
129.00	9335.0
129.90	954.0
135.00	863.0
136.00	439.0
137.00	445.0
141.00	1094.0
142.00	411.0
142.80	347.0
147.00	842.0
147.90	1181.0
148.90	334.0
152.90	416.0
154.00	303.0
155.00	773.0
156.00	1146.0
159.90	381.0
161.00	637.0
164.90	503.0
165.90	356.0
167.00	2253.0
167.90	1119.0
174.00	495.0
175.00	963.0
176.00	308.0
177.00	430.0
178.90	1822.0
180.00	1272.0
180.90	566.0
185.00	828.0
186.00	7117.0
187.00	2141.0
188.90	406.0
190.90	346.0
192.00	539.0
193.00	876.0
195.90	1905.0
196.80	324.0
197.90	54704.0
198.90	3649.0
202.90	384.0
204.00	1713.0
205.00	2855.0
206.00	13965.0
207.00	2407.0
208.00	559.0
210.20	379.0
210.90	480.0
217.00	3429.0
217.90	372.0
221.00	2862.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

221.80	596.0
223.00	922.0
224.00	7142.0
225.00	1857.0
227.00	2602.0
227.90	374.0
228.90	699.0
242.00	443.0
243.00	486.0
244.00	5896.0
245.00	800.0
246.00	1224.0
255.00	31960.0
256.00	4667.0
257.00	434.0
257.90	1258.0
265.00	708.0
272.90	905.0
274.00	2851.0
275.00	15277.0
276.00	1788.0
277.00	1125.0
296.00	3565.0
297.00	476.0
303.00	535.0
314.90	356.0
323.10	1290.0
334.00	912.0
352.00	358.0
353.00	329.0
354.00	566.0
365.00	1797.0
365.90	308.0
372.00	706.0
401.90	313.0
403.00	510.0
421.00	447.0
422.00	360.0
423.10	3058.0
424.00	622.0
441.00	9013.0
442.00	58600.0
443.00	11540.0
444.00	897.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10

Scan 2602 (18.392 min): BM002638.D
DFTPP10

m/z	Abundance
39.90	302.0
44.00	1939.0
207.00	650.0

Instrument :
BNA_M
ClientSampleId :
DFTPP10