


Data Path : Z:\HPCHEM1\BNA_M\Data\BM090216\
 Data File : BM007364.D
 Acq On : 02 Sep 2016 10:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM090116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 12:51:17 2016

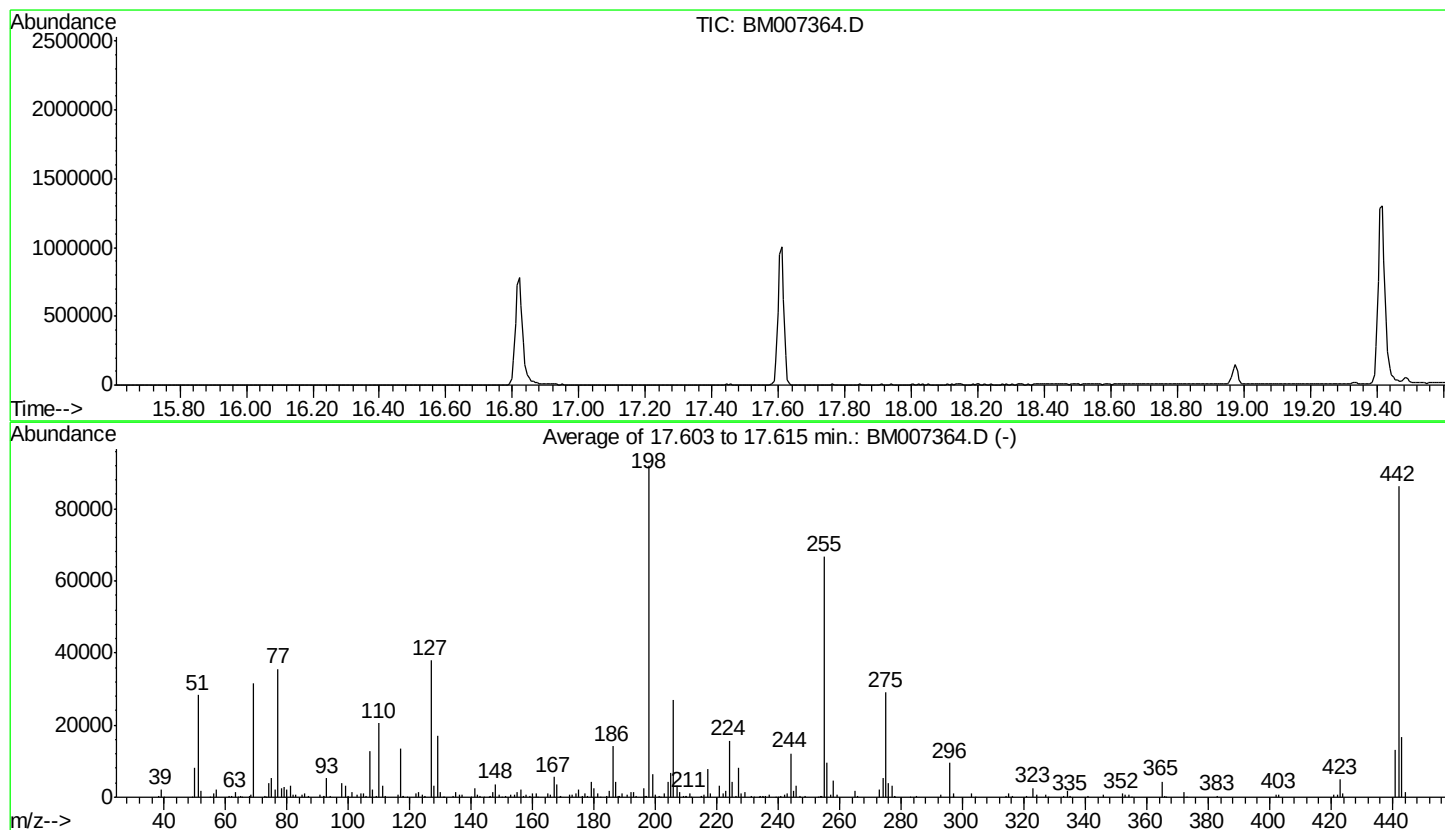

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	28261	PASS
68	69	0.00	2	2.0	628	PASS
69	198	0.00	100	34.2	31480	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	37826	PASS
197	198	0.00	2	0.3	302	PASS
198	198	100	100	100.0	91946	PASS
199	198	5	9	6.9	6336	PASS
275	198	10	60	31.5	28944	PASS
365	198	1	100	4.8	4431	PASS
441	442	0.01	24	15.4	13234	PASS
442	198	50	100	93.6	86098	PASS
443	442	15	24	19.5	16757	PASS