
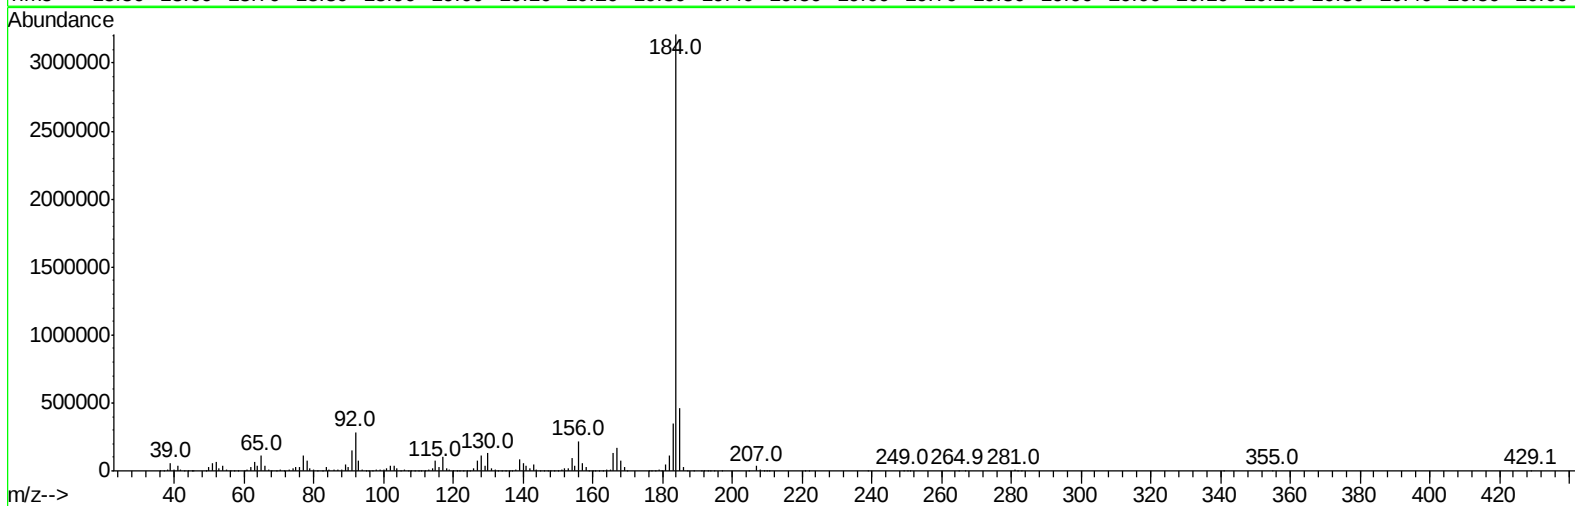


Data Path : Z:\HPCHEM1\BNA M\DATA\BM090217\
Data File : BM011407.D
Acq On : 02 Sep 2017 10:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 04:41:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

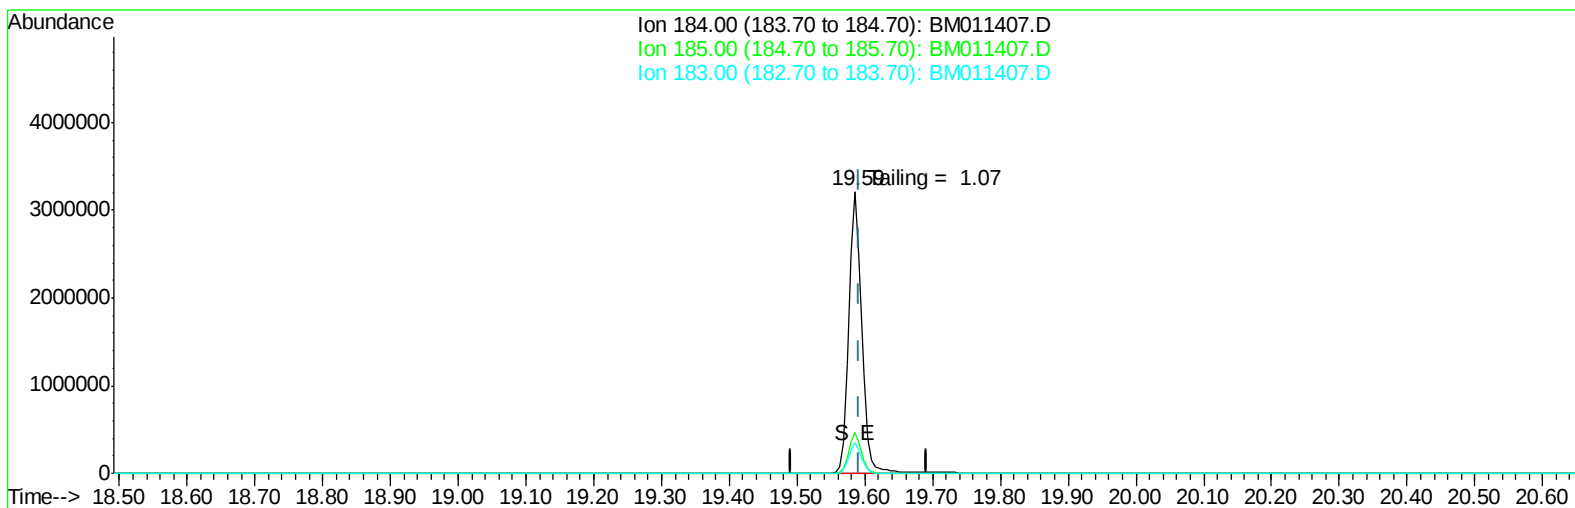

TIC: BM011407.D

(76) Benzidine



19.586min (-0.006) 5079.20ng

response 4187359

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.47
183.00	11.10	10.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM090217\
Data File : BM011407.D
Acq On : 02 Sep 2017 10:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 04:41:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

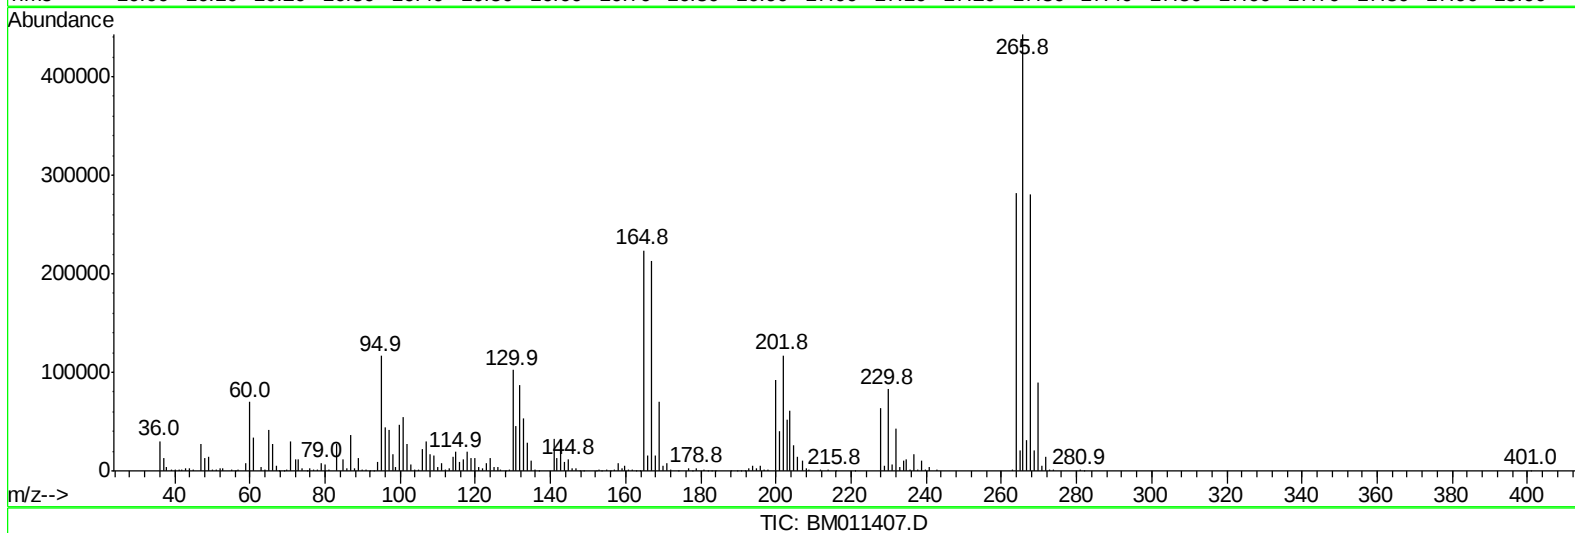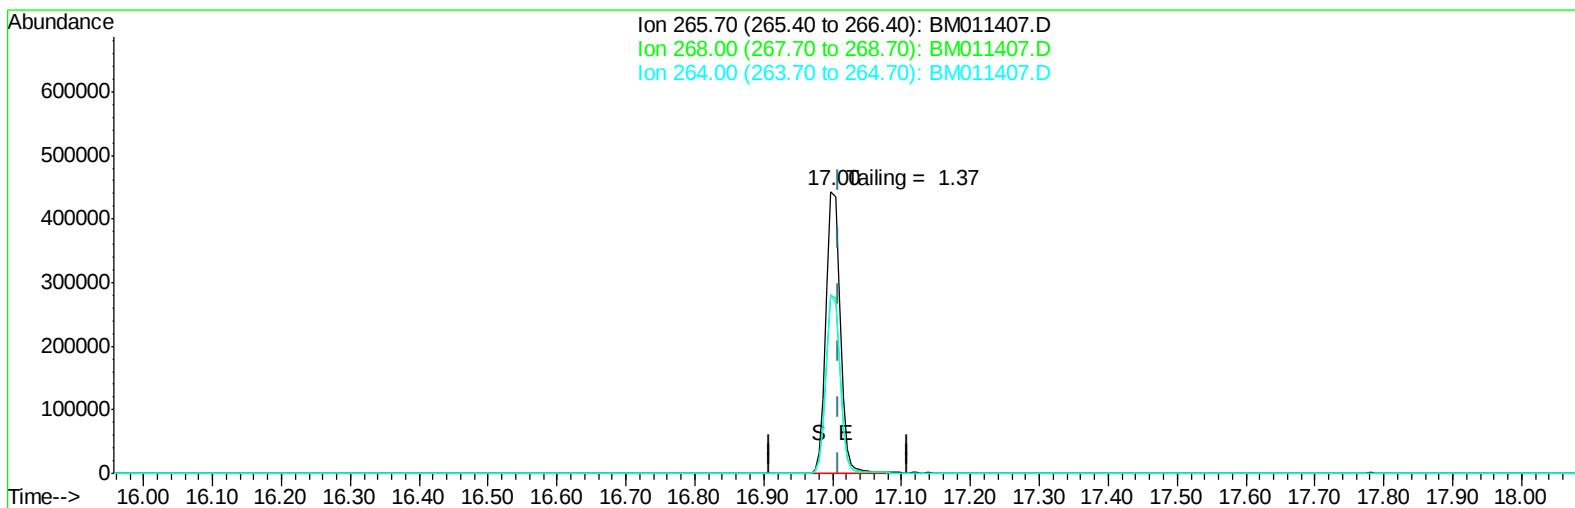

(69) Pentachlorophenol (C)

16.998min (-0.012) 83819.56ng

response 635039

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.39
264.00	61.20	63.59
0.00	0.00	0.00