


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM090217\
 Data File : BM011407.D
 Acq On : 02 Sep 2017 10:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

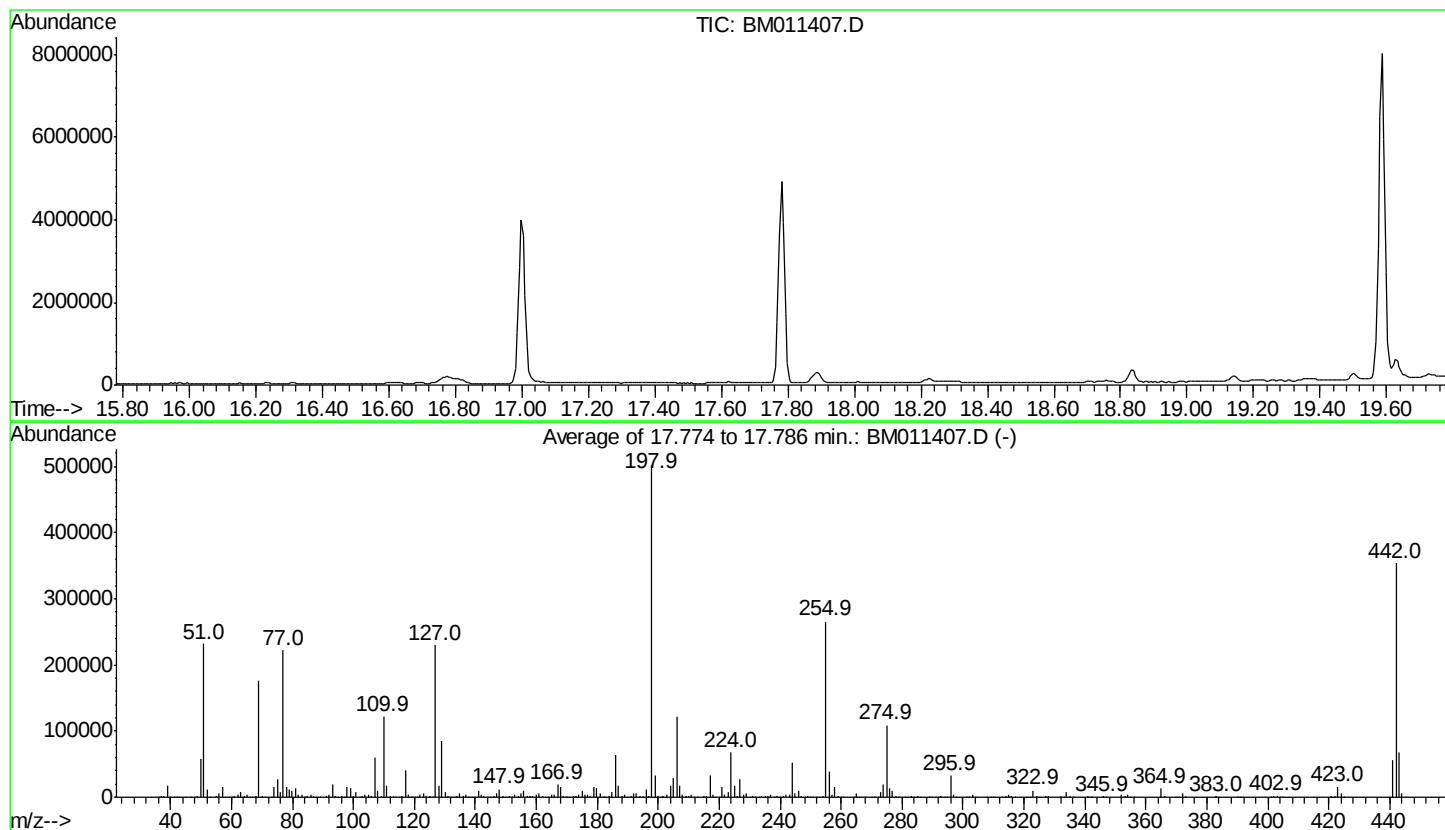

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	231812	PASS
68	69	0.00	2	1.5	2627	PASS
69	198	0.00	100	35.1	176109	PASS
70	69	0.00	2	0.7	1259	PASS
127	198	10	80	45.8	229589	PASS
197	198	0.00	2	0.4	2050	PASS
198	198	100	100	100.0	501525	PASS
199	198	5	9	6.6	33077	PASS
275	198	10	60	21.7	108981	PASS
365	198	1	100	2.6	13150	PASS
441	443	0.01	100	83.5	56346	PASS
442	198	50	100	70.6	353877	PASS
443	442	15	24	19.1	67445	PASS