

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
 Data File : BM007392.D
 Acq On : 03 Sep 2016 05:58
 Operator : UM/SJ
 Sample : H4655-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0006

Quant Time: Sep 03 06:28:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 03 01:45:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	198264	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	941227	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	669590	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1776429	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2551216	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	2618921	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	10334	2.66	ng/uL	0.00
5) Phenol-d5	6.96	99	219449	11.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	137862	14.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	182236	13.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	174845	10.70	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	98836	14.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	111064	13.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	199614	12.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	185826	9.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	817178	14.15	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	969081	14.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	130361	11.95	ng/ul	0.00
57) Fluorene-d10	15.42	176	719493	14.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	119669	10.71	ng/ul	0.00
70) Anthracene-d10	17.26	188	1245178	15.01	ng/ul	0.00
76) Pyrene-d10	19.56	212	1722983	16.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	1984030	16.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	327624	5.69	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
Data File : BM007392.D
Acq On : 03 Sep 2016 05:58
Operator : UM/SJ
Sample : H4655-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0006

Quant Time: Sep 03 06:28:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 03 01:45:38 2016
Response via : Initial Calibration

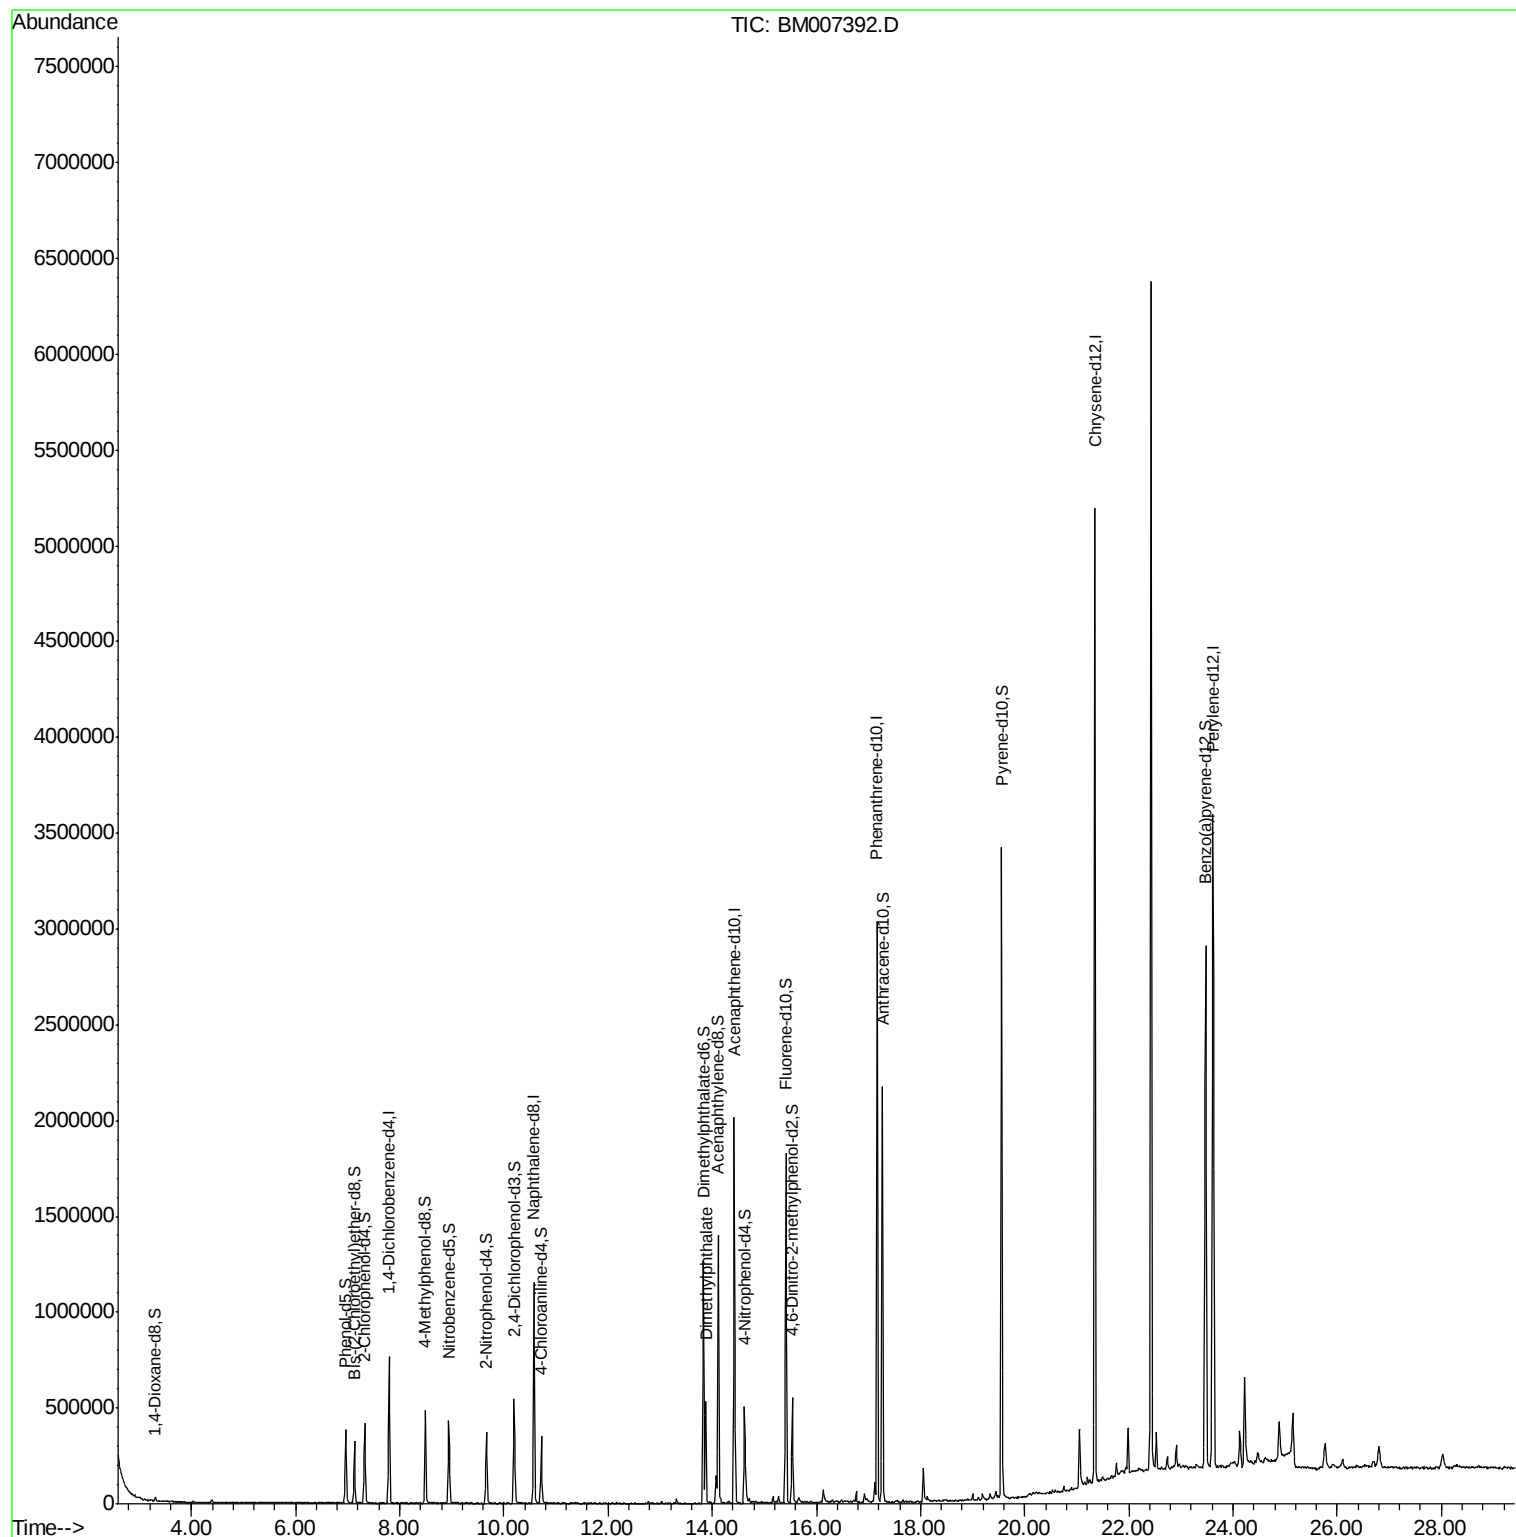

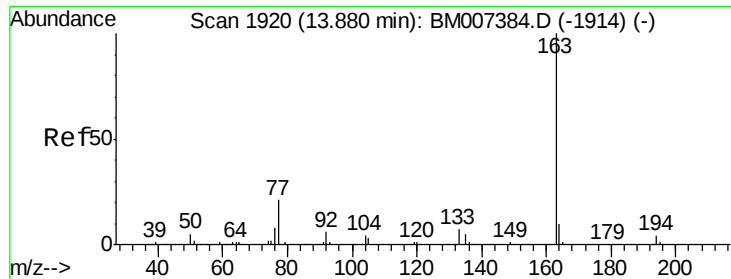

#44

Dimethylphthalate

Concen: 5.69 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. 0.00 min

Lab File: BM007392.D

Acq: 03 Sep 2016 05:58

Instrument :

BNA_M

ClientSampleId :

C0006


Tgt Ion:163 Resp: 327624

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.3 7.8 11.8

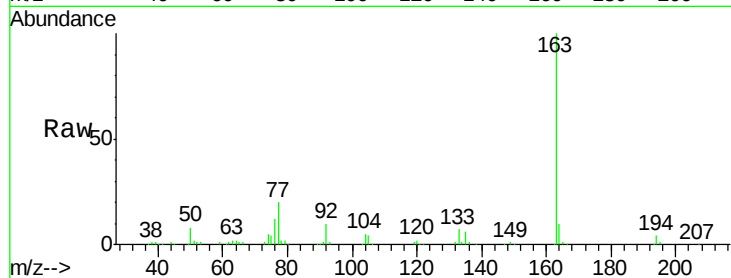

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

