

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
 Data File : BM007408.D
 Acq On : 03 Sep 2016 15:33
 Operator : UM/SJ
 Sample : H4655-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0025

Quant Time: Sep 05 01:46:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 05 01:45:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	268822	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	1221543	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	805191	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	2015274	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2405405	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2031685	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	22339	4.25	ng/uL	0.00
5) Phenol-d5	6.96	99	529501	20.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	293663	22.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	416990	22.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	442837	20.00	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	220492	24.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	259681	24.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	484028	23.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	526189	20.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1639365	23.60	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1999796	24.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	258577	19.72	ng/ul	0.00
57) Fluorene-d10	15.42	176	1468016	24.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	224850	17.74	ng/ul	0.00
70) Anthracene-d10	17.27	188	2405390	25.55	ng/ul	0.00
76) Pyrene-d10	19.56	212	2944666	29.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	2451189	26.19	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	663981	9.60	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
Data File : BM007408.D
Acq On : 03 Sep 2016 15:33
Operator : UM/SJ
Sample : H4655-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0025

Quant Time: Sep 05 01:46:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 05 01:45:04 2016
Response via : Initial Calibration

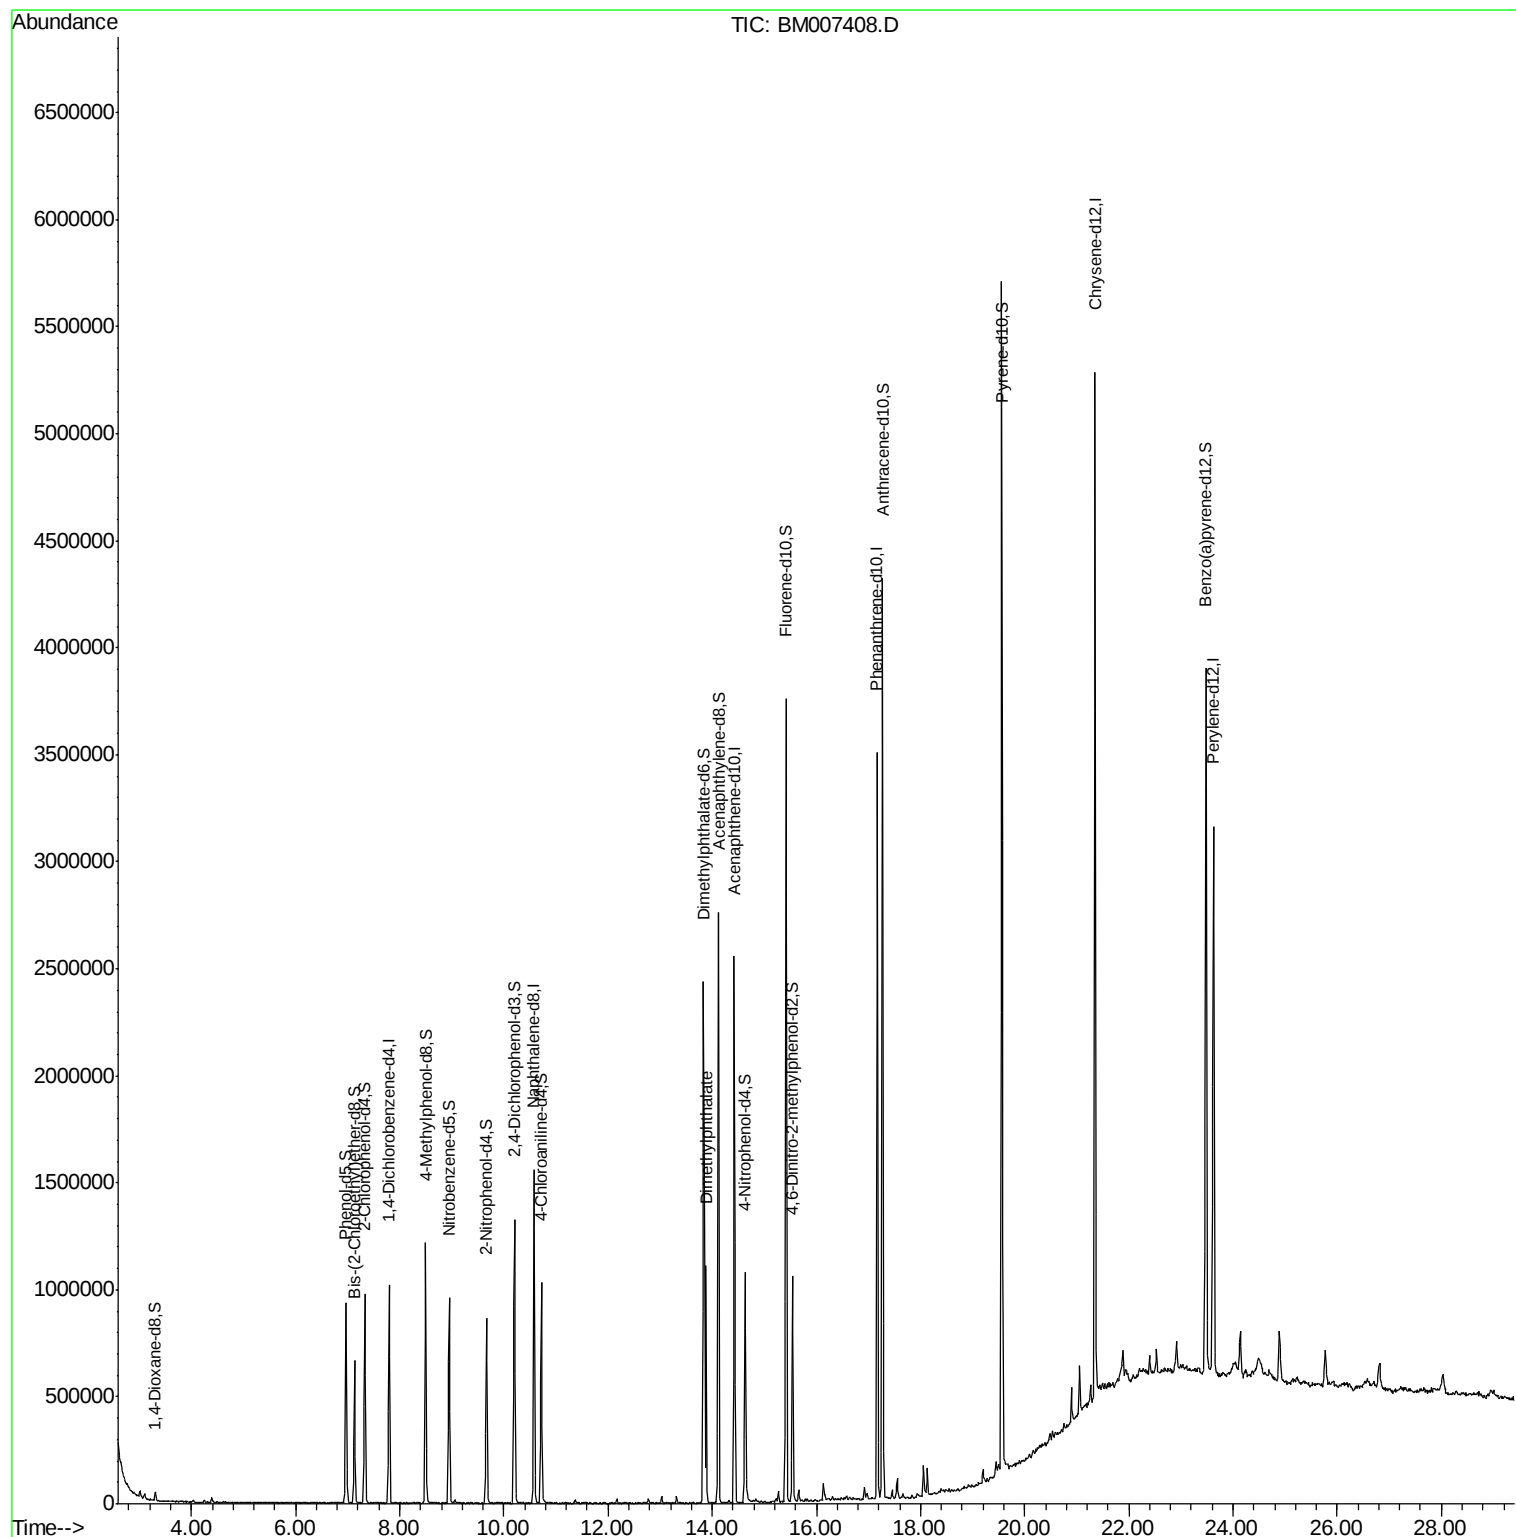

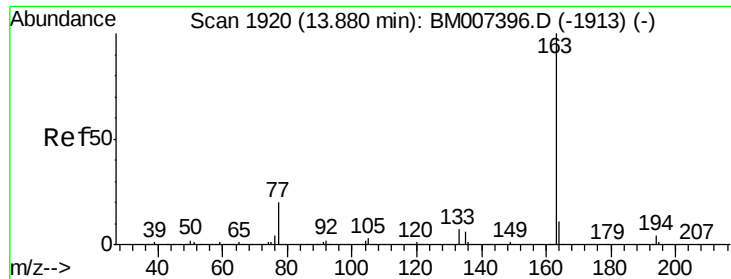

#44

Dimethylphthalate

Concen: 9.60 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. 0.00 min

Lab File: BM007408.D

Acq: 03 Sep 2016 15:33

Instrument :

BNA_M

ClientSampleId :

C0025


Tgt Ion:163 Resp: 663981

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.3 7.8 11.8

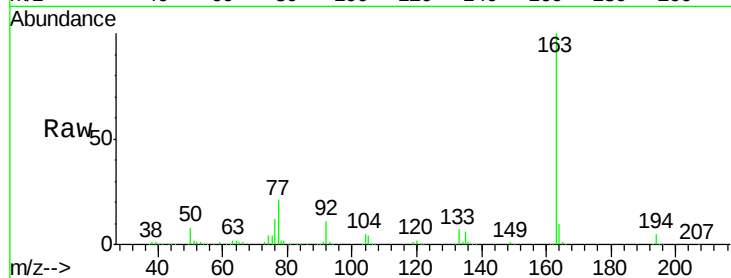

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

