

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
 Data File : BM007379.D
 Acq On : 02 Sep 2016 22:10
 Operator : UM/SJ
 Sample : H4639-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD388

Quant Time: Sep 03 00:41:14 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 03 00:40:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	176133	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	813150	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	560622	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1471018	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2061388	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2133879	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	15899	4.61	ng/uL	0.00
5) Phenol-d5	6.96	99	369205	22.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	217302	24.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	289490	23.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	320147	22.06	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	157791	26.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	184198	26.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	338890	24.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	225512	13.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1385394	28.64	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1585111	28.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	217750	23.85	ng/ul	0.00
57) Fluorene-d10	15.42	176	1198770	28.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	210048	22.71	ng/ul	0.00
70) Anthracene-d10	17.27	188	1996437	29.05	ng/ul	0.00
76) Pyrene-d10	19.56	212	2590944	30.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	2921742	29.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	516036	10.71	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
Data File : BM007379.D
Acq On : 02 Sep 2016 22:10
Operator : UM/SJ
Sample : H4639-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD388

Quant Time: Sep 03 00:41:14 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 03 00:40:49 2016
Response via : Initial Calibration

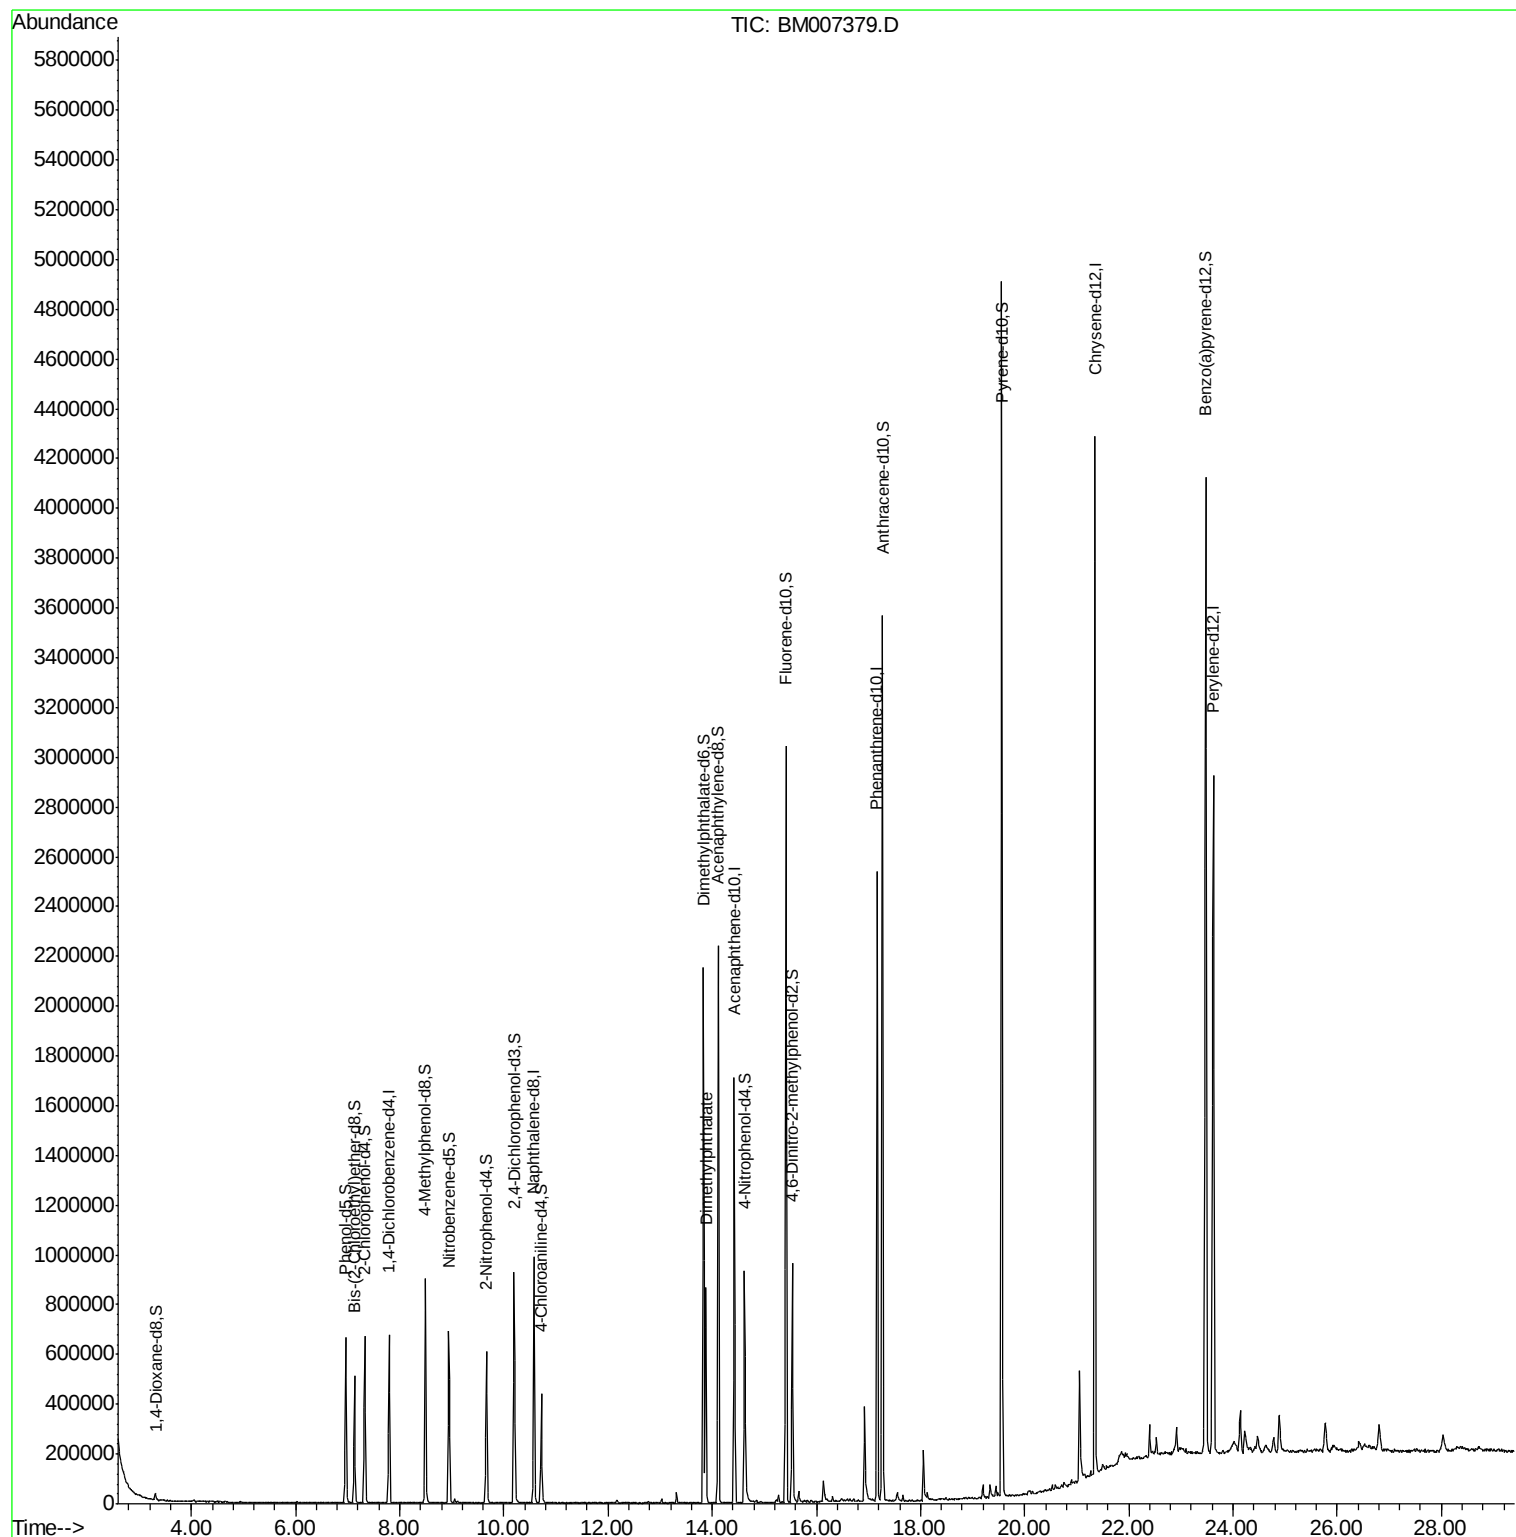

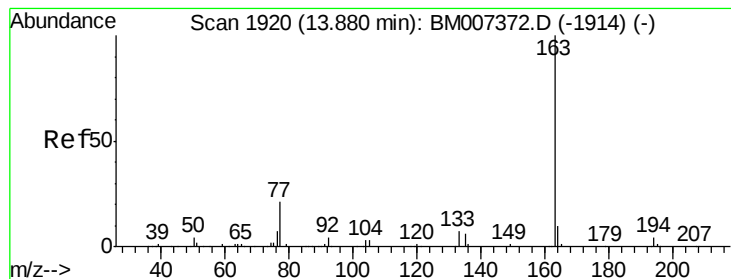

#44

Dimethylphthalate

Concen: 10.71 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. -0.00 min

Lab File: BM007379.D

Acq: 02 Sep 2016 22:10

Instrument :

BNA_M

ClientSampleId :

BD388


Tgt Ion:163 Resp: 516036

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.3 7.8 11.8

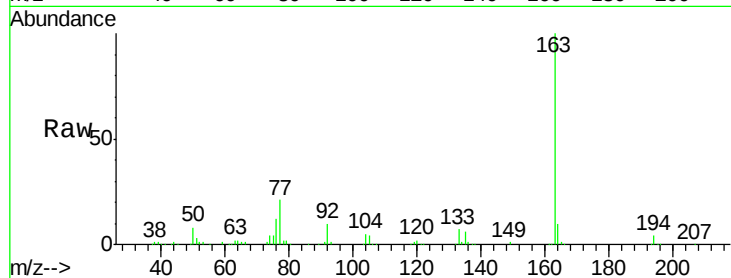

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

